

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040723\
Data File : FE041235.D
Signal(s) : FID1B.ch
Acq On : 07 Apr 2023 22:38
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 10 02:14:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040523.M
Quant Title :
QLast Update : Thu Apr 06 02:04:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.651	3202502	21.107 ug/ml
12) N-OCTACOSANE	17.108	2993778	21.792 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE040723\
Data File : FE041235.D
Signal(s) : FID1B.ch
Acq On : 07 Apr 2023 22:38
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 10 02:14:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040523.M
Quant Title :
QLast Update : Thu Apr 06 02:04:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

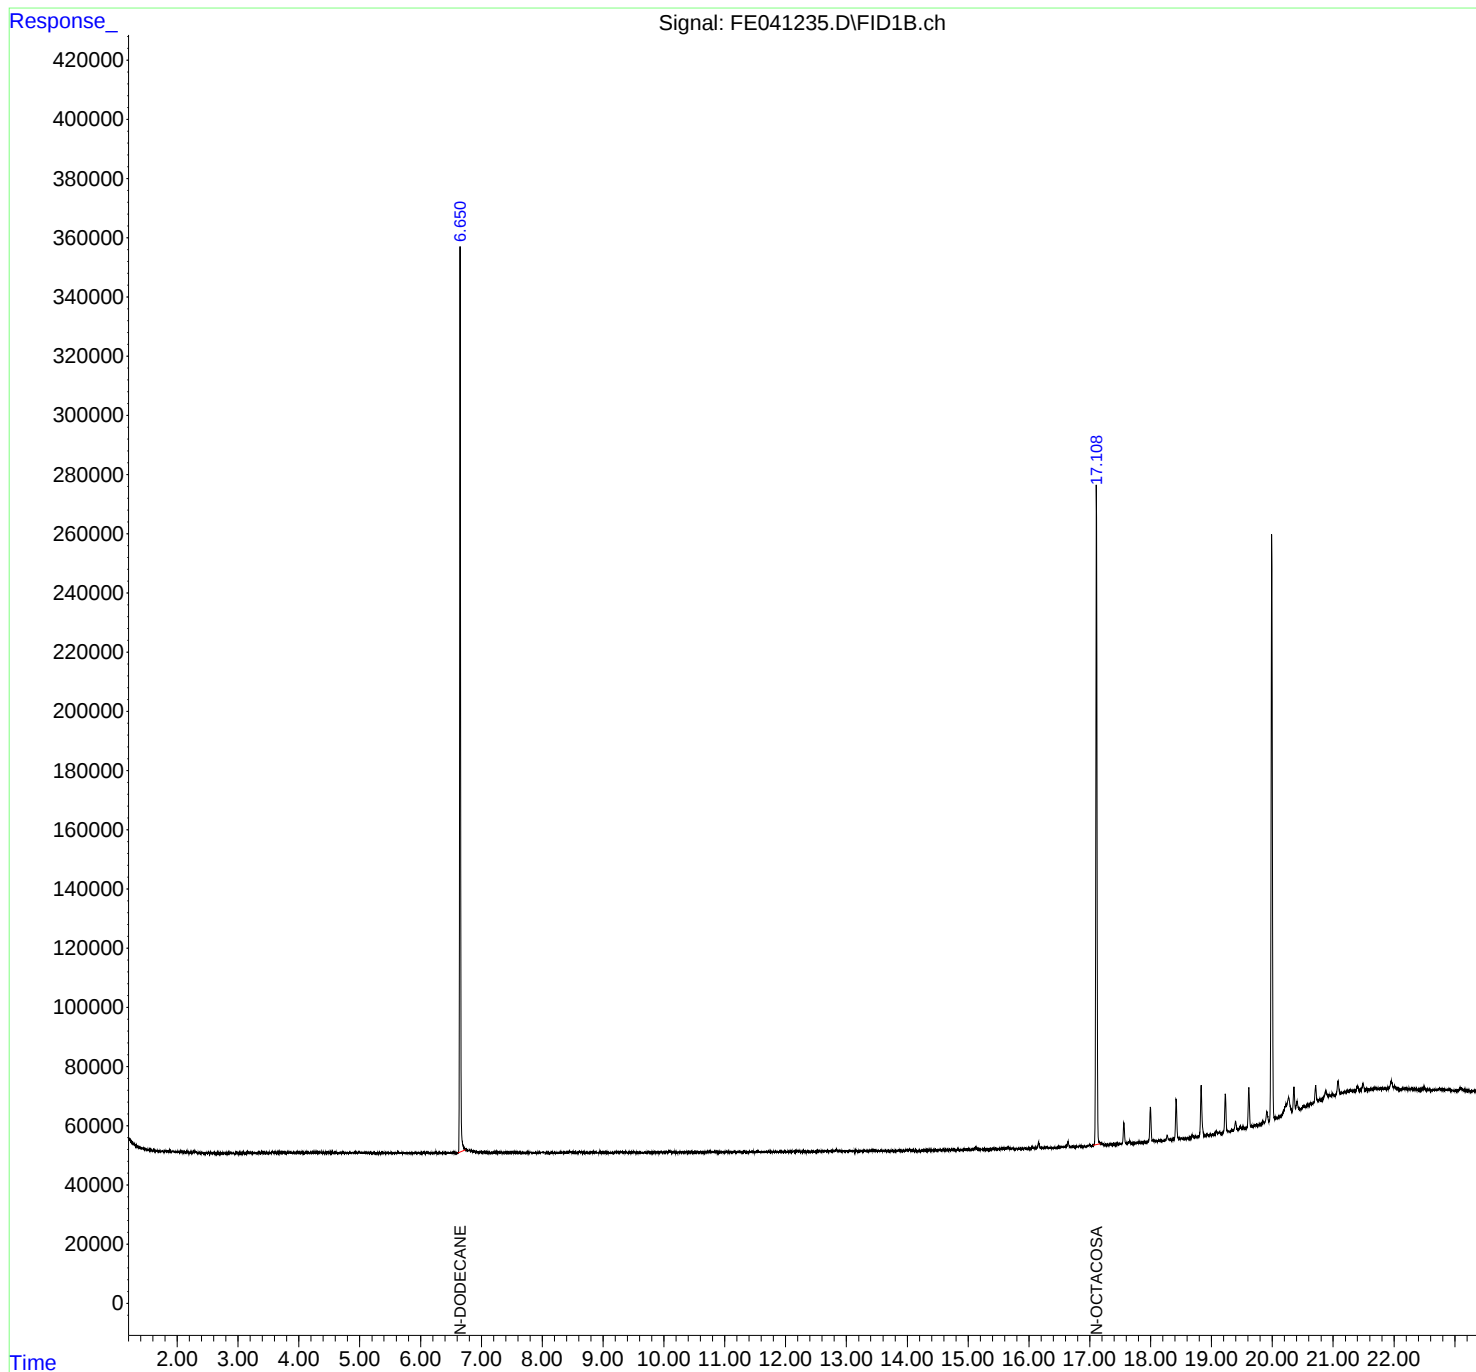


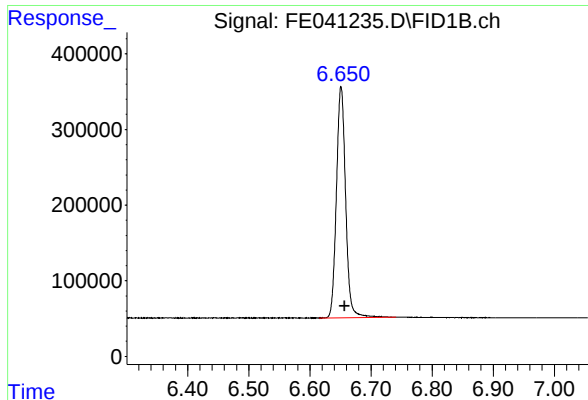

#3 N-DODECANE


R.T.: 6.651 min
Delta R.T.: -0.006 min
Response: 3202502
Conc: 21.11 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

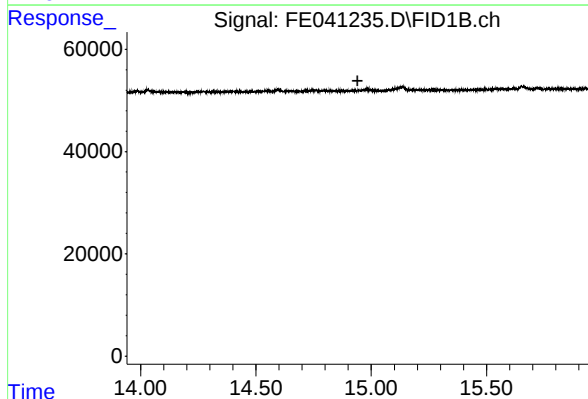

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.940 min
Response: 0
Conc: N.D.

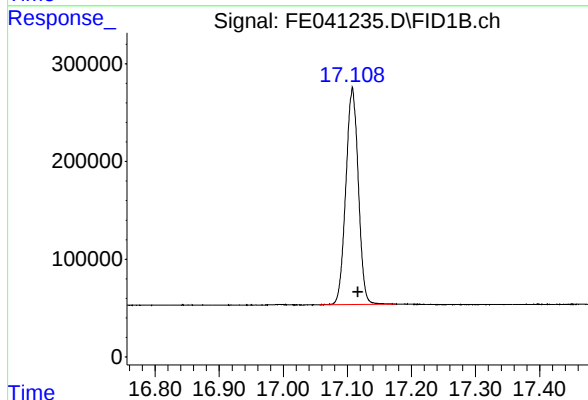

#12 N-OCTACOSANE

R.T.: 17.108 min
Delta R.T.: -0.009 min
Response: 2993778
Conc: 21.79 ug/ml