

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041023\
Data File : FE041269.D
Signal(s) : FID1B.ch
Acq On : 10 Apr 2023 10:57
Operator : YP\AJ
Sample : PB151947BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB151947BL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2023
Supervised By :Ankita Jodhani 04/11/2023

Integration File: autoint1.e
Quant Time: Apr 10 12:03:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040523.M
Quant Title :
QLast Update : Thu Apr 06 02:04:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.928	2786026	21.889 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041023\
Data File : FE041269.D
Signal(s) : FID1B.ch
Acq On : 10 Apr 2023 10:57
Operator : YP\AJ
Sample : PB151947BL
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
PB151947BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2023
Supervised By :Ankita Jodhani 04/11/2023

Integration File: autoint1.e
Quant Time: Apr 10 12:03:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040523.M
Quant Title :
QLast Update : Thu Apr 06 02:04:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

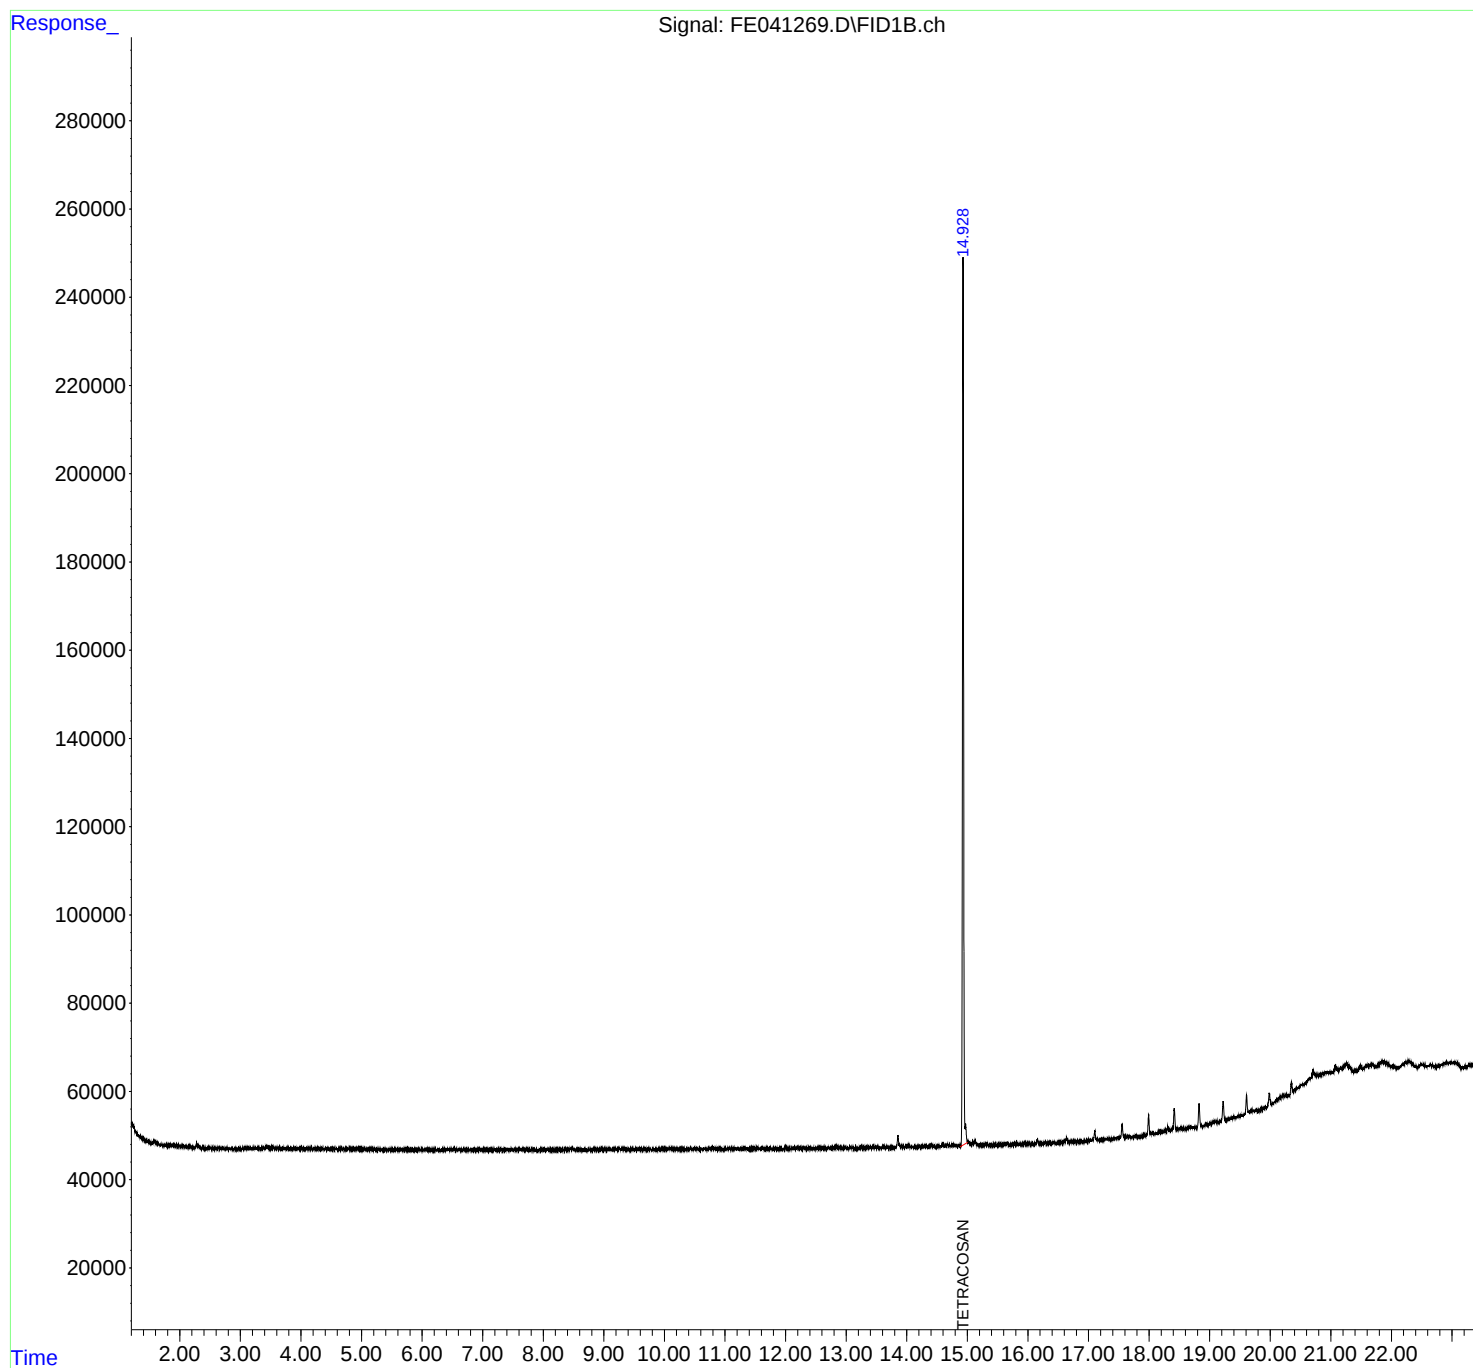

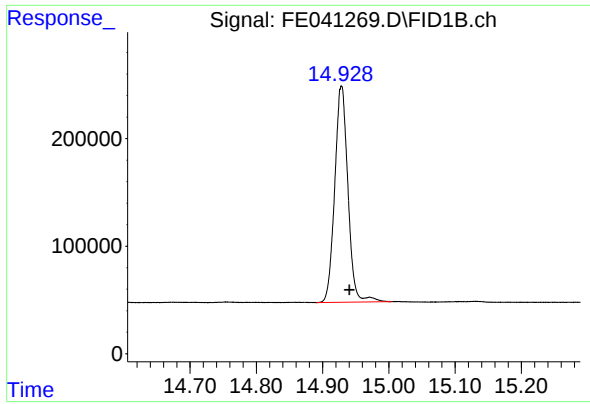

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.928 min
Delta R.T.: -0.013 min
Response: 2786026
Conc: 21.89 ug/ml

Instrument :

FID_E

ClientSampleId :

PB151947BL

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/11/2023

Supervised By :Ankita Jodhani 04/11/2023