

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041123AL\
Data File : FE041297.D
Signal(s) : FID1B.ch
Acq On : 11 Apr 2023 07:46
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 11 15:15:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

11) T	n-Heneicosane (C21)	13.441	28719	0.170 ug/ml
13) T	n-Docosane (C22)	14.028	23322	0.141 ug/ml
14) T	n-Tetracosane (C24)	15.110f	73250	0.453 ug/ml
17) T	n-Tricontane (C30)	17.993	41229	0.270 ug/ml
18) T	n-Dotriacontane (C32)	18.826	32666	0.209 ug/ml
20) T	n-Hexatriacontane (C36)	20.408	11451	0.075 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041123AL\
Data File : FE041297.D
Signal(s) : FID1B.ch
Acq On : 11 Apr 2023 07:46
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 11 15:15:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

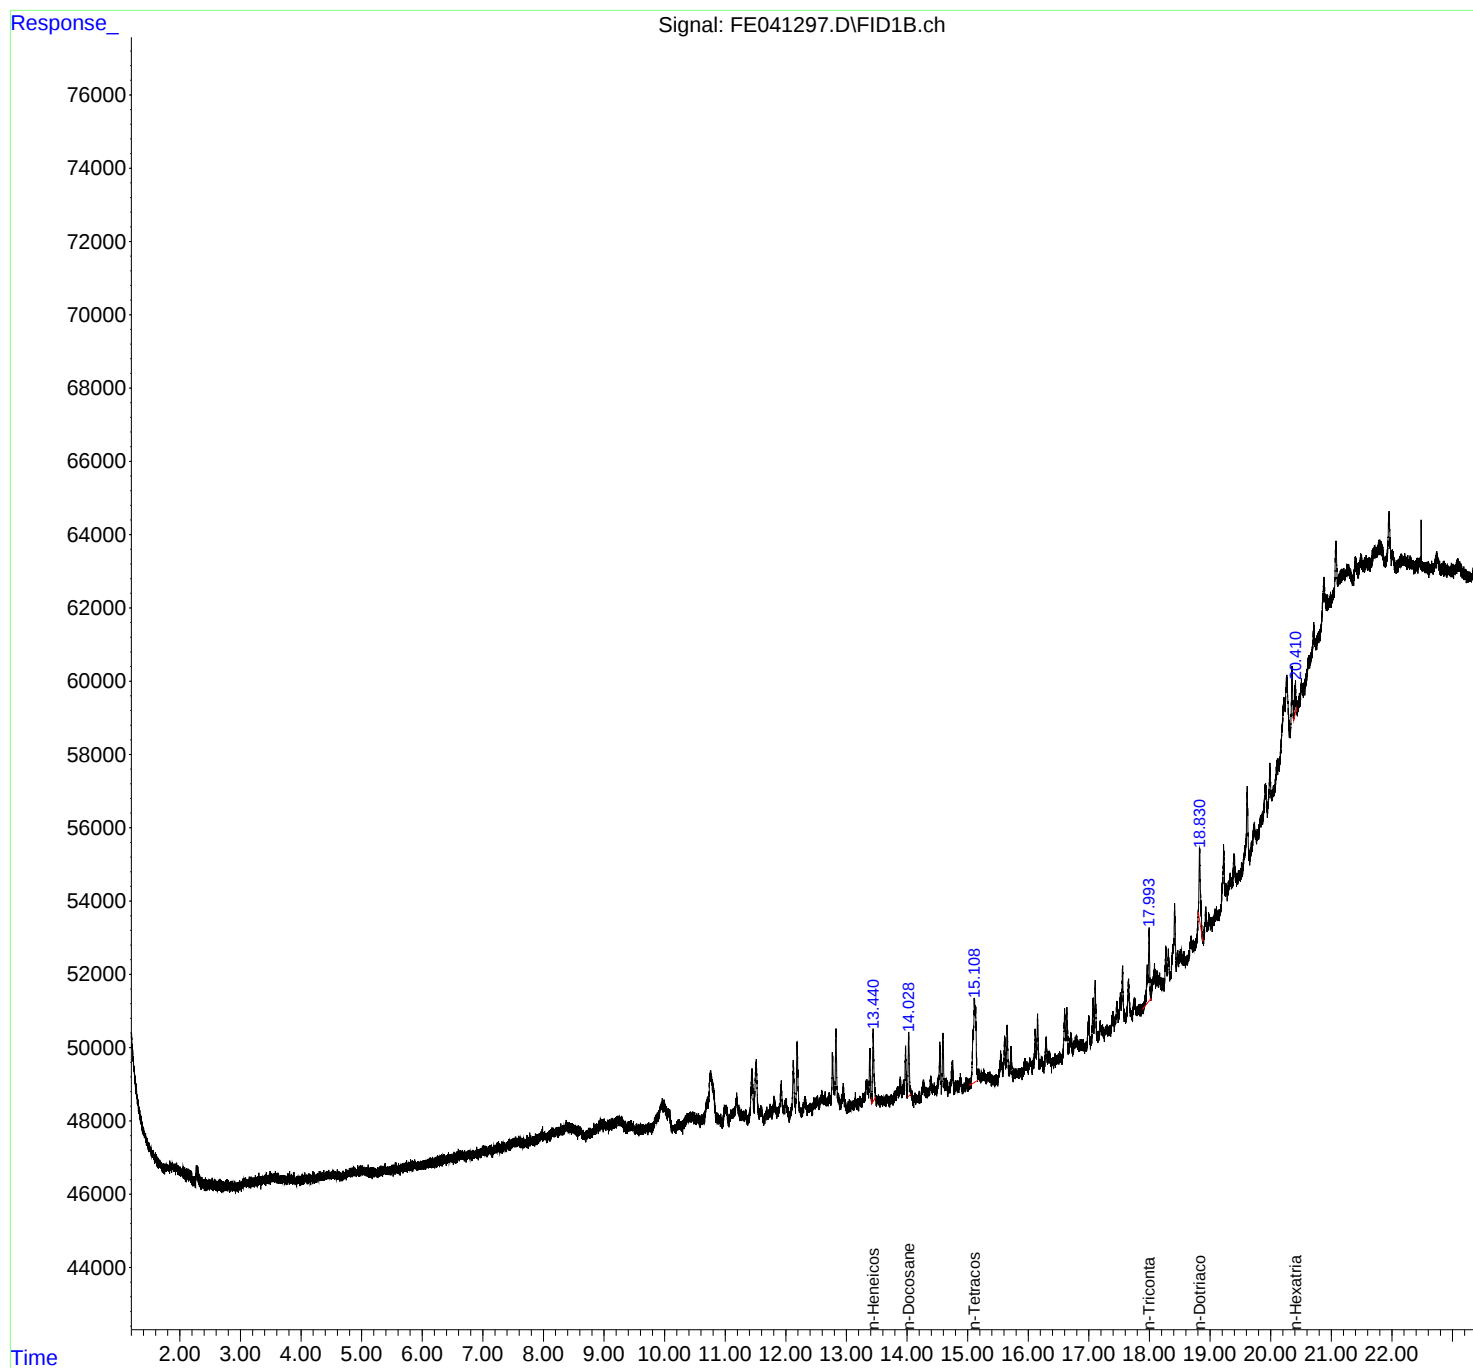


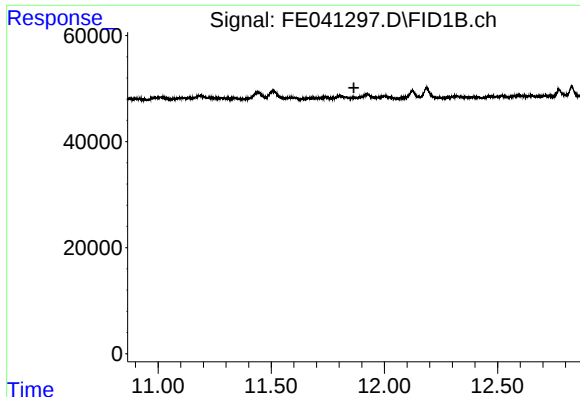

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

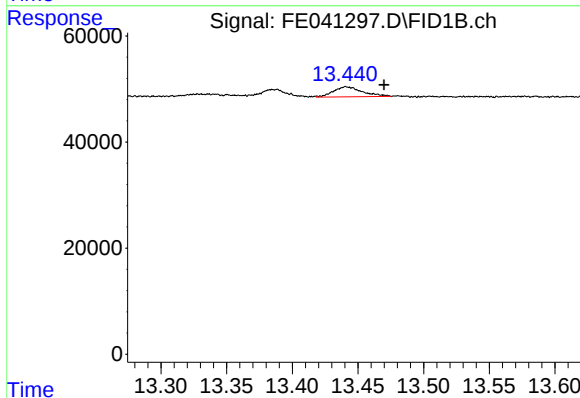


#11 n-Heneicosane (C21)

R.T.: 13.441 min
Delta R.T.: -0.029 min
Response: 28719
Conc: 0.17 ug/ml

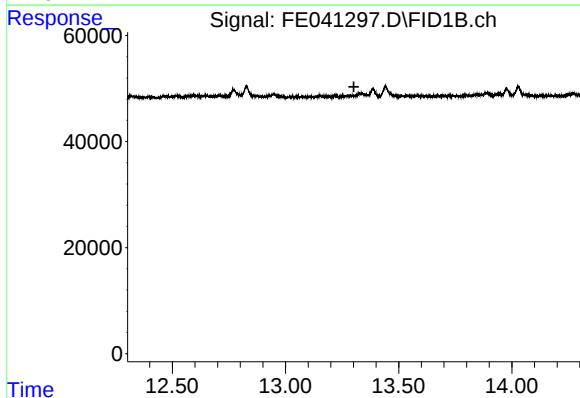


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

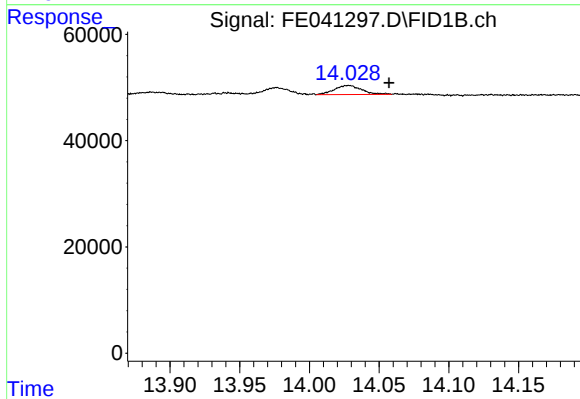

#13 n-Docosane (C22)


R.T.: 14.028 min
Delta R.T.: -0.029 min
Response: 23322
Conc: 0.14 ug/ml

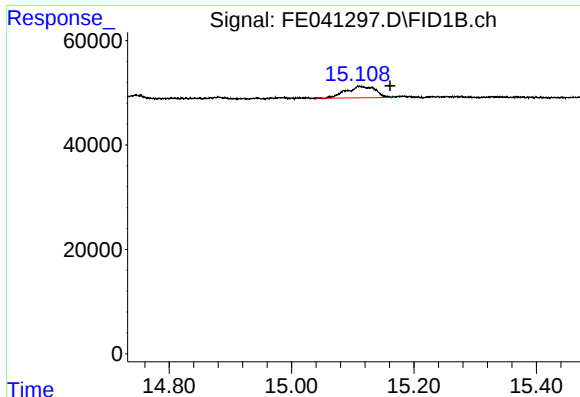

#14 n-Tetracosane (C24)


R.T.: 15.110 min
Delta R.T.: -0.051 min
Response: 73250
Conc: 0.45 ug/ml

Instrument :
FID_E
ClientSampleId :

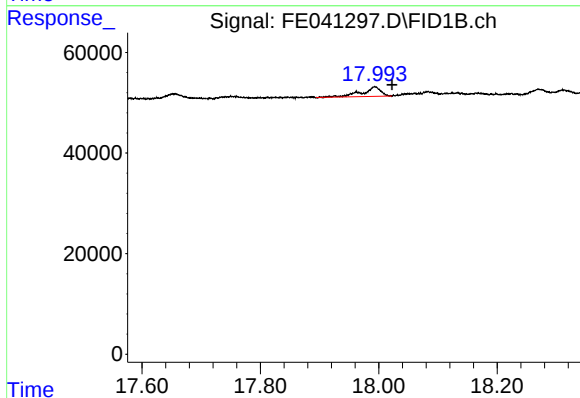


#17 n-Tricontane (C30)

R.T.: 17.993 min
Delta R.T.: -0.029 min
Response: 41229
Conc: 0.27 ug/ml

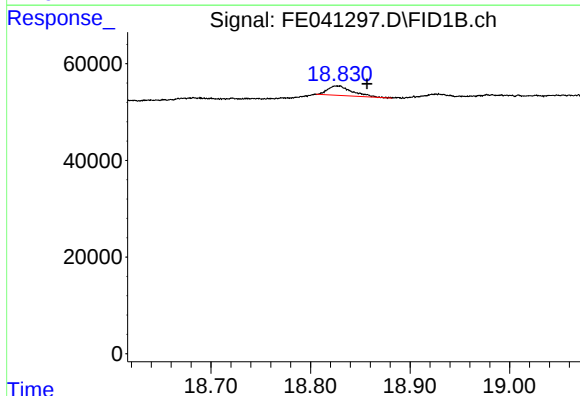

#18 n-Dotriacontane (C32)

R.T.: 18.826 min
Delta R.T.: -0.031 min
Response: 32666
Conc: 0.21 ug/ml

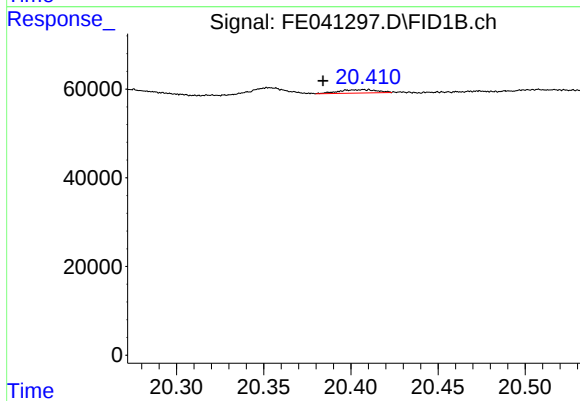

#20 n-Hexatriacontane (C36)

R.T.: 20.408 min
Delta R.T.: 0.024 min
Response: 11451
Conc: 0.08 ug/ml