

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041123AL\
Data File : FE041315.D
Signal(s) : FID1B.ch
Acq On : 11 Apr 2023 21:13
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 00:21:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.994	43148	0.282 ug/ml
18) T	n-Dotriacontane (C32)	18.827	37037	0.237 ug/ml
20) T	n-Hexatriacontane (C36)	20.408	163077	1.074 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041123AL\
Data File : FE041315.D
Signal(s) : FID1B.ch
Acq On : 11 Apr 2023 21:13
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 00:21:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

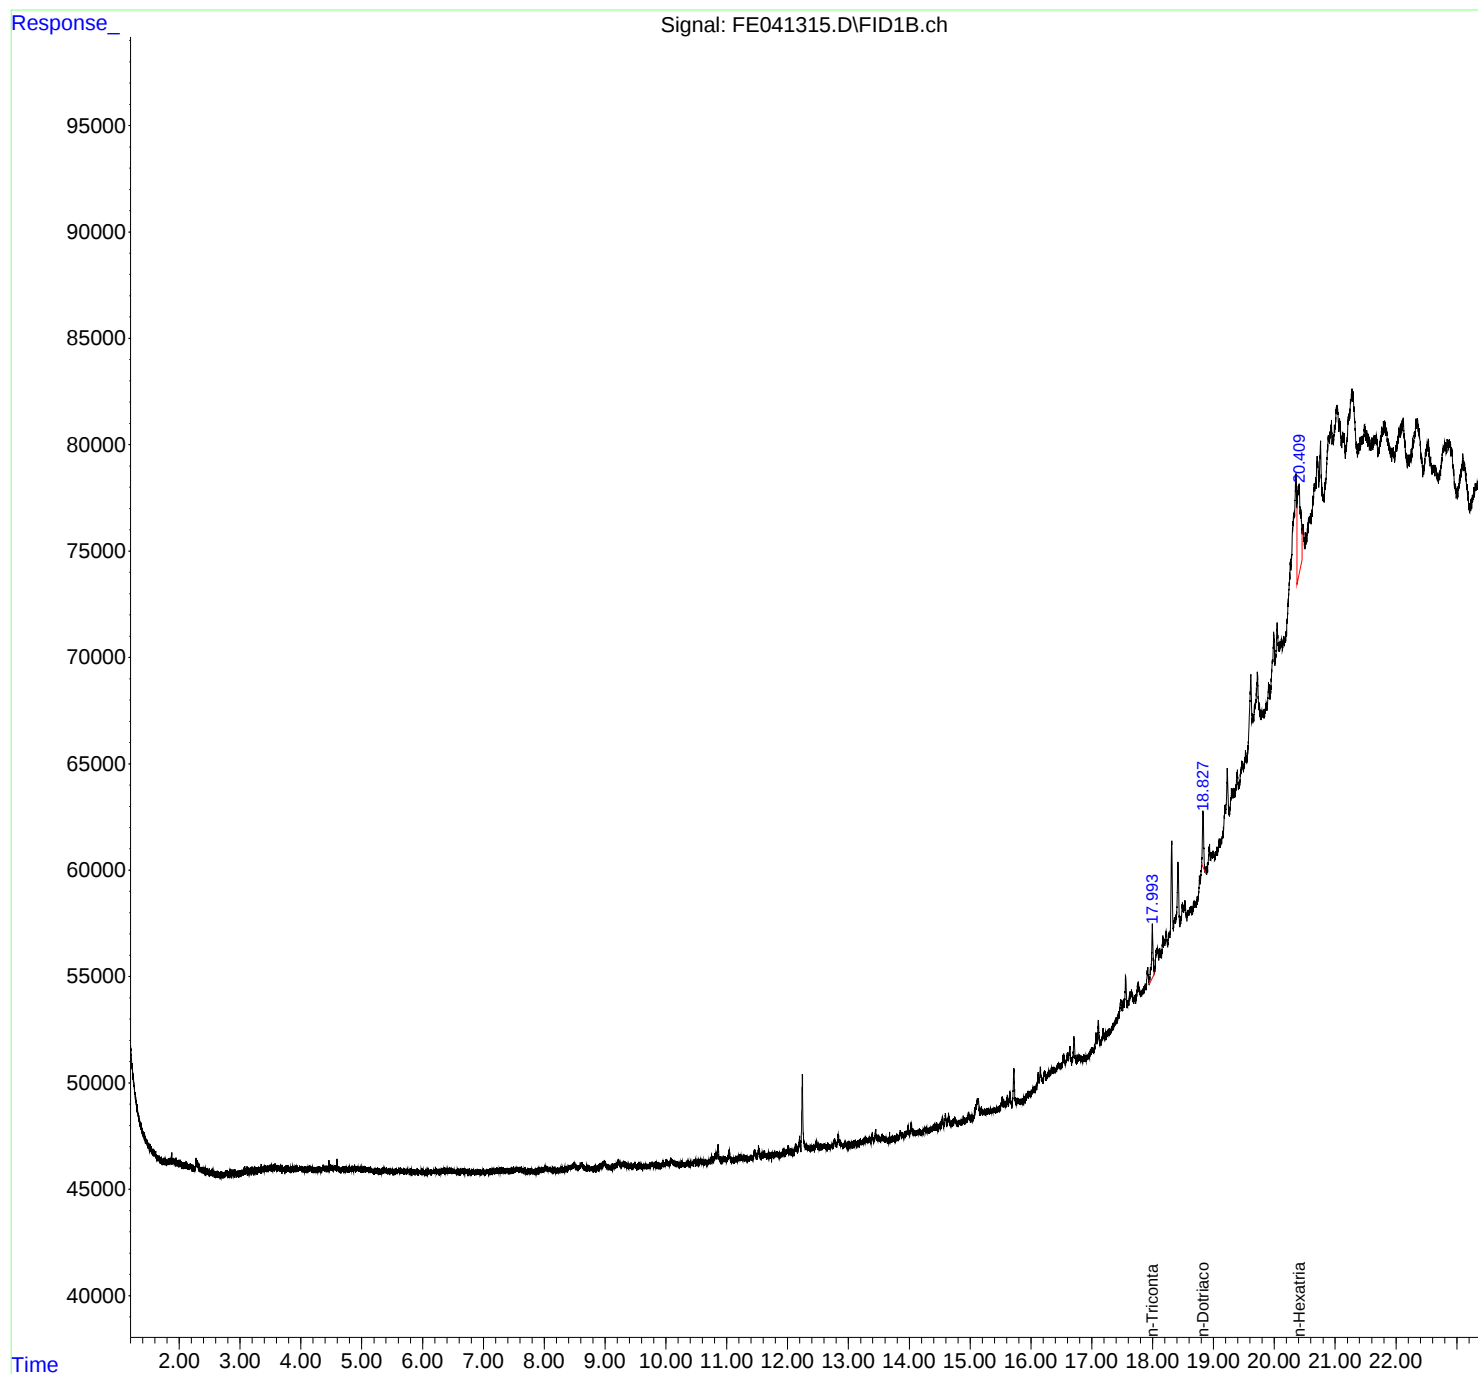


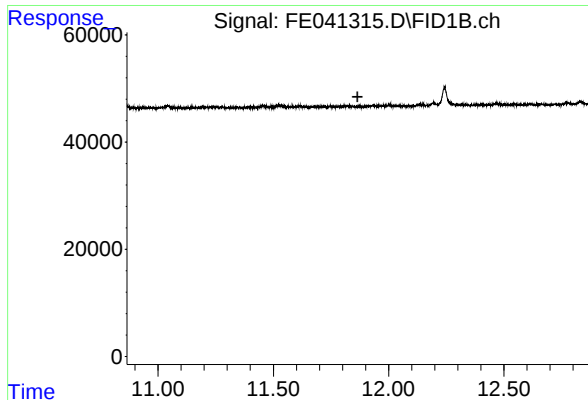

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

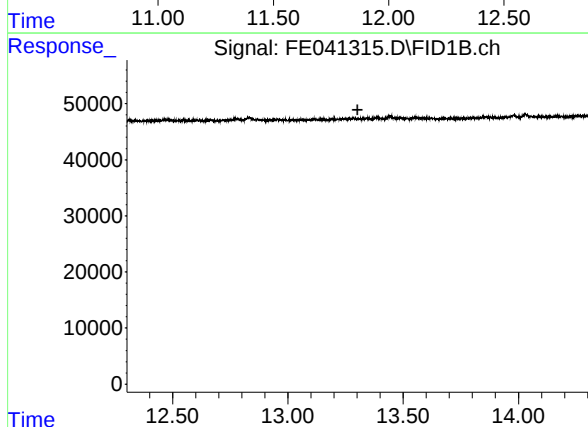


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

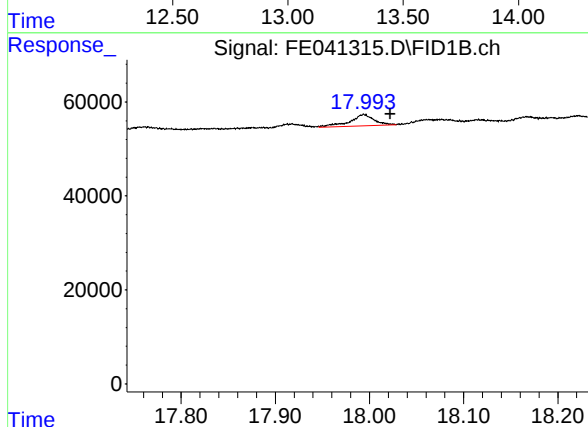


#17 n-Tricontane (C30)

R.T.: 17.994 min
Delta R.T.: -0.028 min
Response: 43148
Conc: 0.28 ug/ml

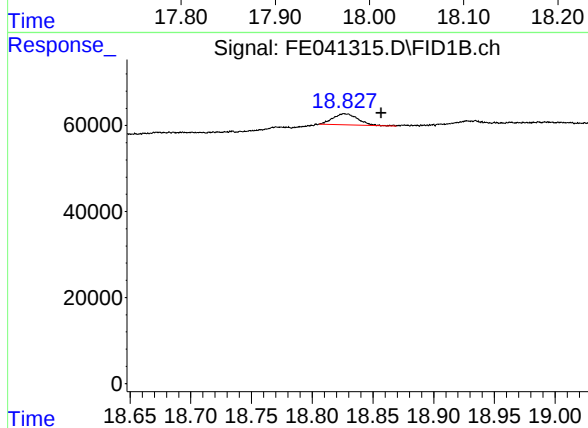

#18 n-Dotriacontane (C32)

R.T.: 18.827 min
Delta R.T.: -0.030 min
Response: 37037
Conc: 0.24 ug/ml

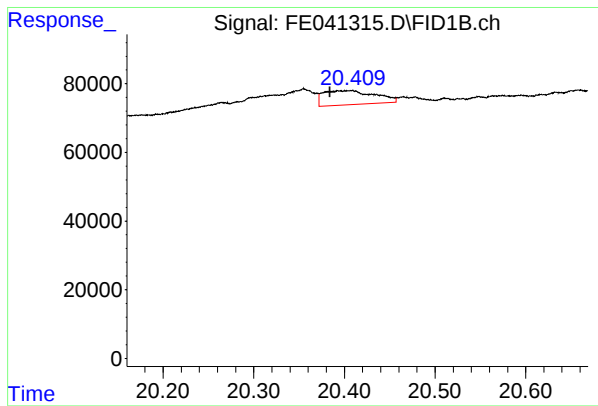

#20 n-Hexatriacontane (C36)

R.T.: 20.408 min
Delta R.T.: 0.024 min
Response: 163077
Conc: 1.07 ug/ml

Instrument :
FID_E
ClientSampleId :