

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE041323AL\  
 Data File : FE041351.D  
 Signal(s) : FID1B.ch  
 Acq On : 13 Apr 2023 19:59  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Apr 14 01:05:48 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 032523.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Mar 25 06:32:15 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units  |
|--------------------------------|--------|----------|-------------|
| -----                          |        |          |             |
| System Monitoring Compounds    |        |          |             |
| Target Compounds               |        |          |             |
| 16) T n-Octacosane (C28)       | 17.110 | 15502    | 0.101 ug/ml |
| 17) T n-Tricontane (C30)       | 17.998 | 7990     | 0.052 ug/ml |
| 18) T n-Dotriacontane (C32)    | 18.830 | 61567    | 0.394 ug/ml |
| 19) T n-Tetratriacontane (C34) | 19.637 | 39810    | 0.257 ug/ml |
| 20) T n-Hexatriacontane (C36)  | 20.389 | 78948    | 0.520 ug/ml |
| 21) T n-Octatriacontane (C38)  | 21.118 | 19754    | 0.126 ug/ml |
| 22) T n-Tetracontane (C40)     | 22.010 | 106532   | 0.667 ug/ml |
| -----                          |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE041323AL\  
Data File : FE041351.D  
Signal(s) : FID1B.ch  
Acq On : 13 Apr 2023 19:59  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Apr 14 01:05:48 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 032523.M  
Quant Title : GC Extractables  
QLast Update : Sat Mar 25 06:32:15 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

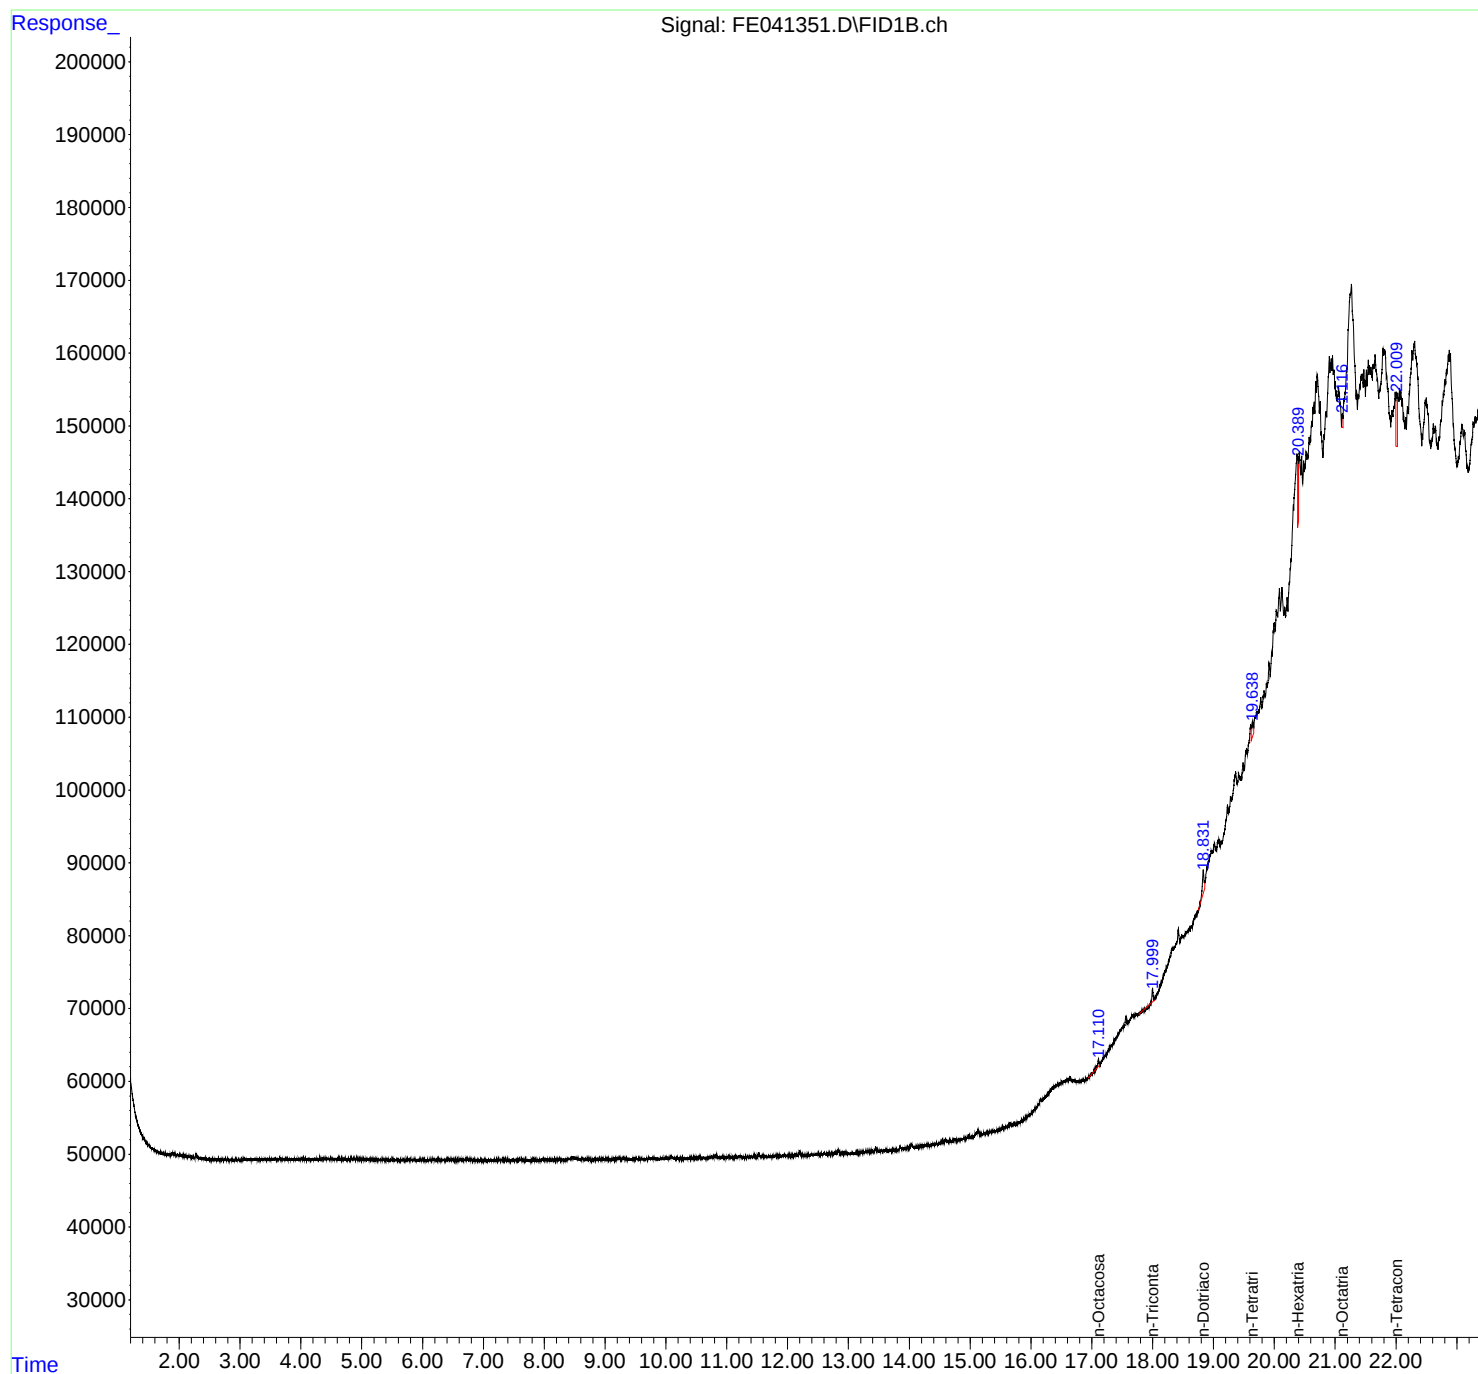


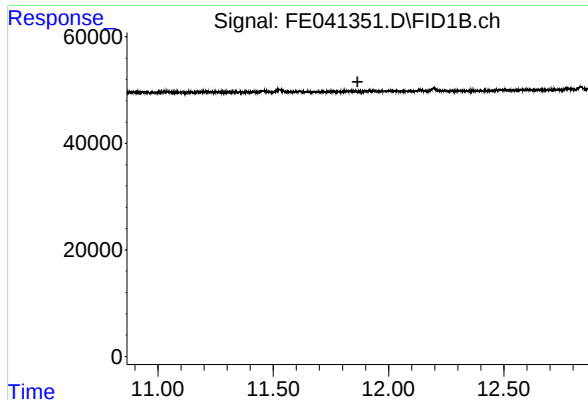

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min  
Exp R.T.: 11.865 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :

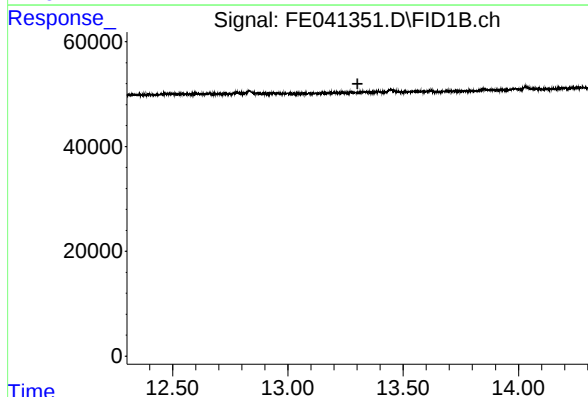


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min  
Exp R.T.: 13.302 min  
Response: 0  
Conc: N.D.

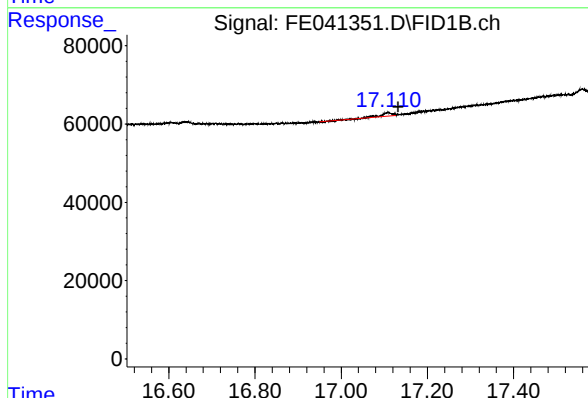


#16 n-Octacosane (C28)

R.T.: 17.110 min  
Delta R.T.: -0.023 min  
Response: 15502  
Conc: 0.10 ug/ml

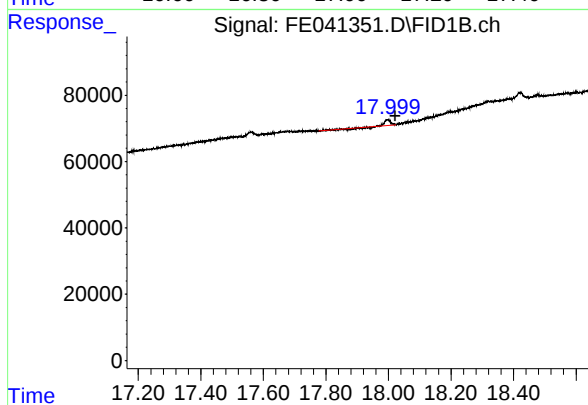

#17 n-Tricontane (C30)


R.T.: 17.998 min  
Delta R.T.: -0.024 min  
Response: 7990  
Conc: 0.05 ug/ml

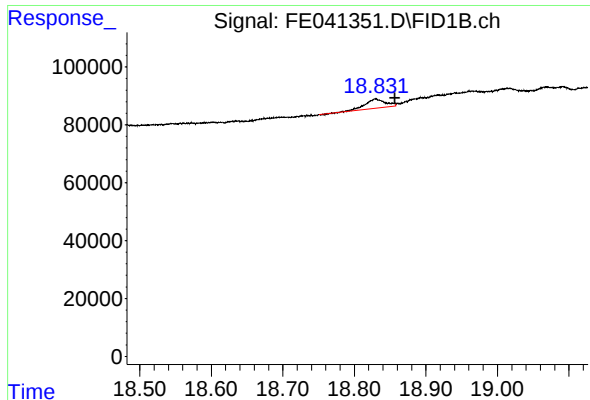

#18 n-Dotriacontane (C32)


R.T.: 18.830 min  
Delta R.T.: -0.027 min  
Response: 61567  
Conc: 0.39 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

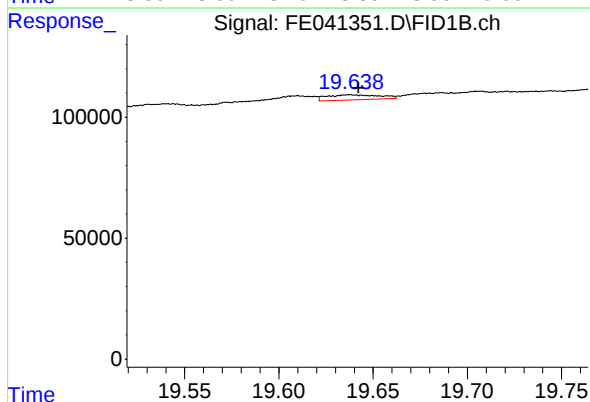


#19 n-Tetratriacontane (C34)

R.T.: 19.637 min  
Delta R.T.: -0.005 min  
Response: 39810  
Conc: 0.26 ug/ml

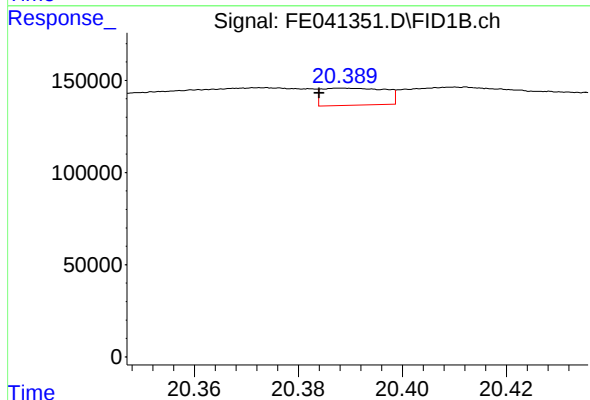


#20 n-Hexatriacontane (C36)

R.T.: 20.389 min  
Delta R.T.: 0.005 min  
Response: 78948  
Conc: 0.52 ug/ml

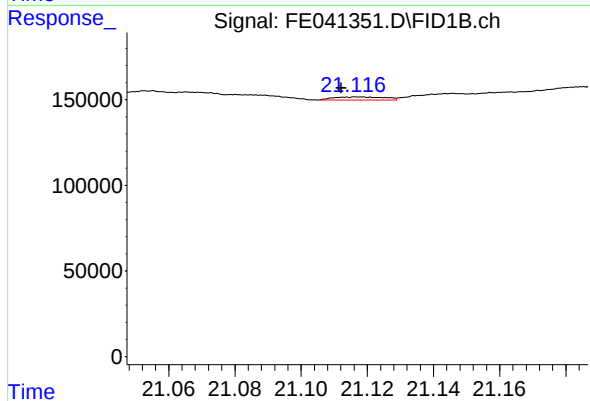

#21 n-Octatriacontane (C38)

R.T.: 21.118 min  
Delta R.T.: 0.006 min  
Response: 19754  
Conc: 0.13 ug/ml

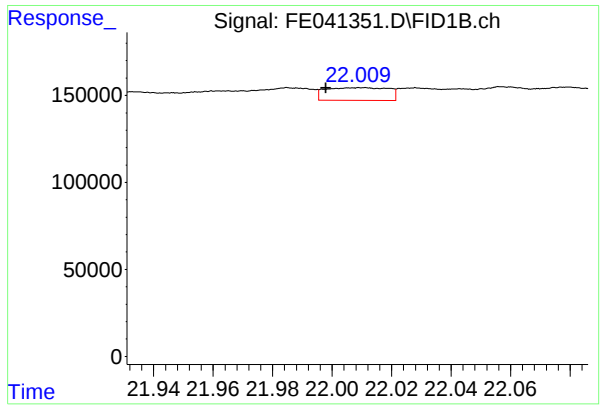

#22 n-Tetracontane (C40)

R.T.: 22.010 min  
Delta R.T.: 0.012 min  
Response: 106532  
Conc: 0.67 ug/ml

Instrument :

FID\_E

ClientSampleId :