

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE041420\  
Data File : FE031742.D  
Signal(s) : FID1B.CH  
Acq On : 14 Apr 2020 23:58  
Operator : DD\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Apr 15 00:53:28 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE040720.M  
Quant Title :  
QLast Update : Tue Apr 07 15:06:47 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                   | R.T.   | Response | Conc Units  |
|-----------------------------|-------------------|--------|----------|-------------|
| -----                       |                   |        |          |             |
| System Monitoring Compounds |                   |        |          |             |
| Target Compounds            |                   |        |          |             |
| 13)                         | N-TRIACONTANE     | 17.443 | 20301    | 0.049 ug/ml |
| 14)                         | N-DOTRIACONTANE   | 18.275 | 684231   | 1.740 ug/ml |
| 16)                         | N-HEXATRIACONTANE | 19.799 | 138210   | 0.401 ug/ml |
| -----                       |                   |        |          |             |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE041420\  
Data File : FE031742.D  
Signal(s) : FID1B.CH  
Acq On : 14 Apr 2020 23:58  
Operator : DD\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Apr 15 00:53:28 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE040720.M  
Quant Title :  
QLast Update : Tue Apr 07 15:06:47 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

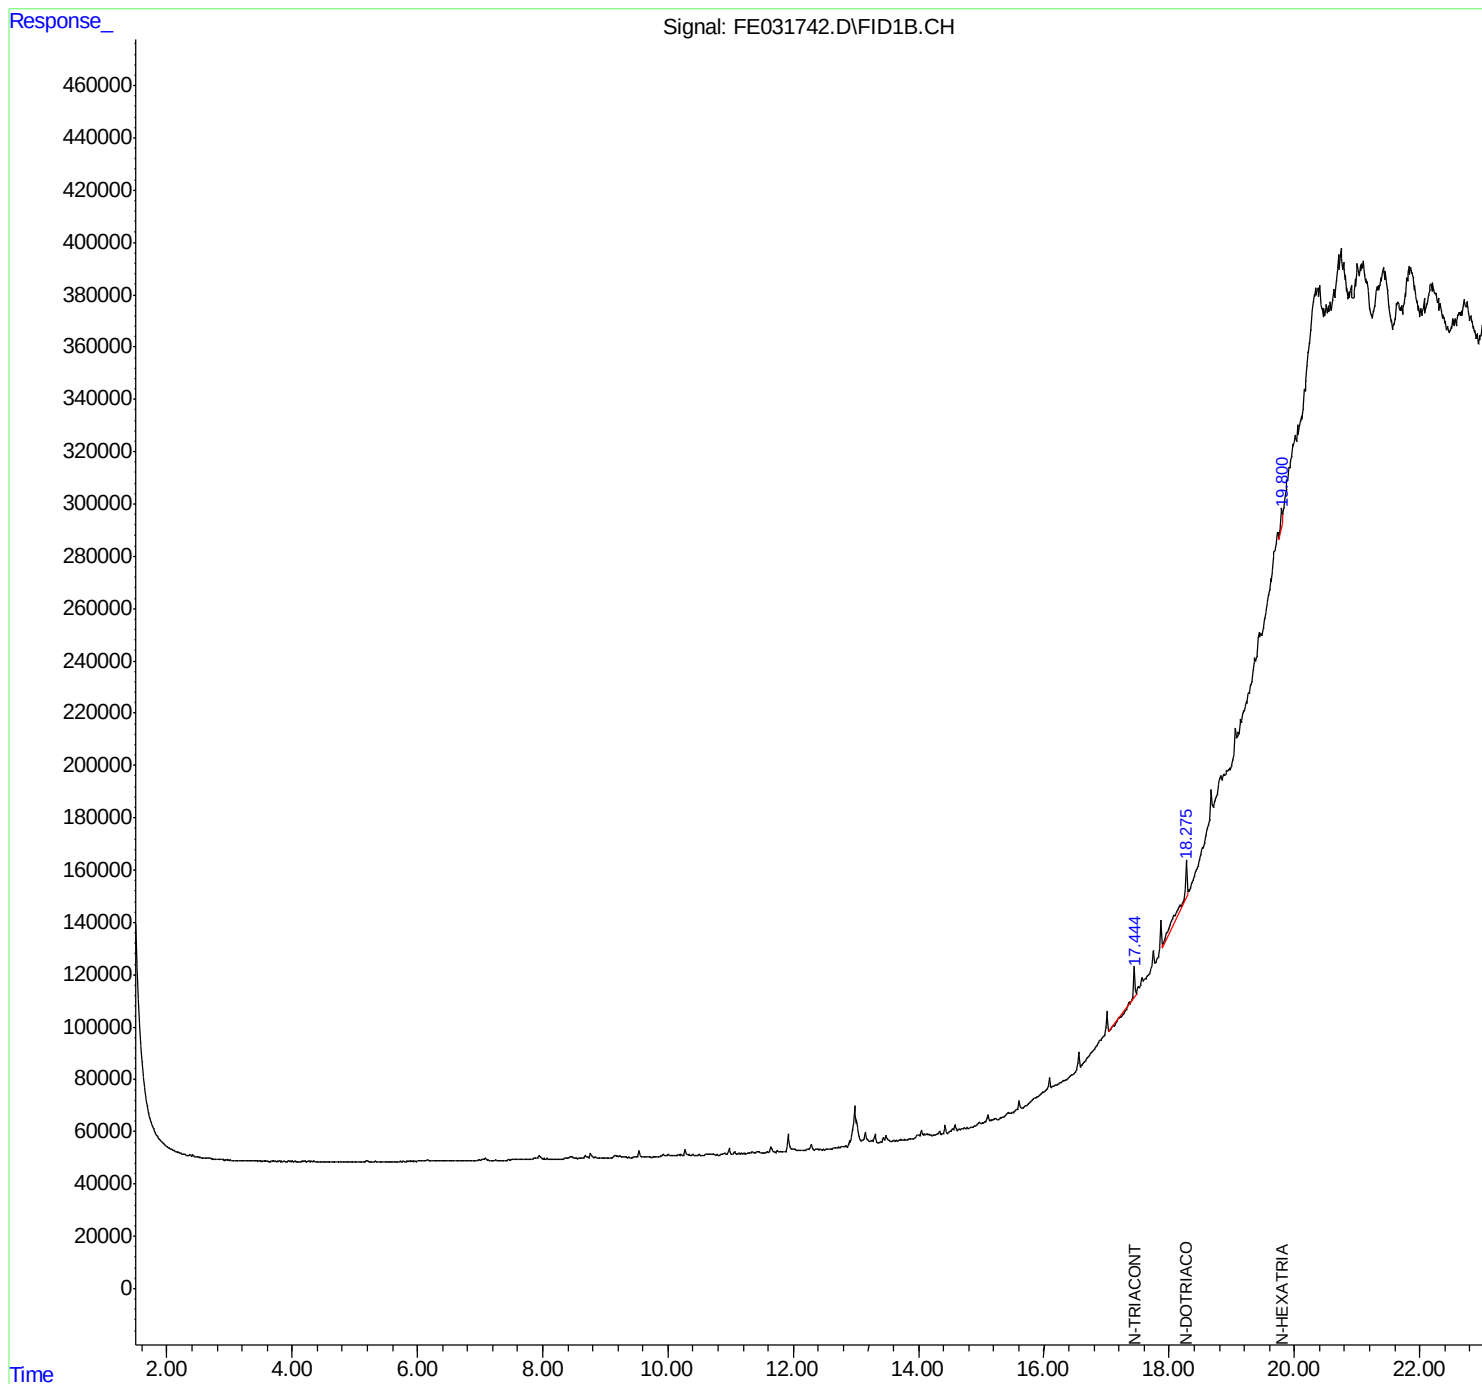

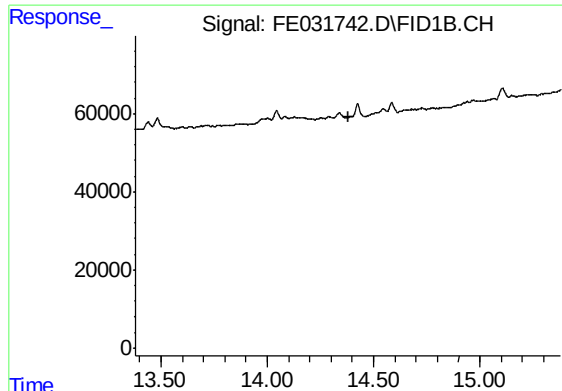


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.379 min  
Response: 0  
Conc: N.D.

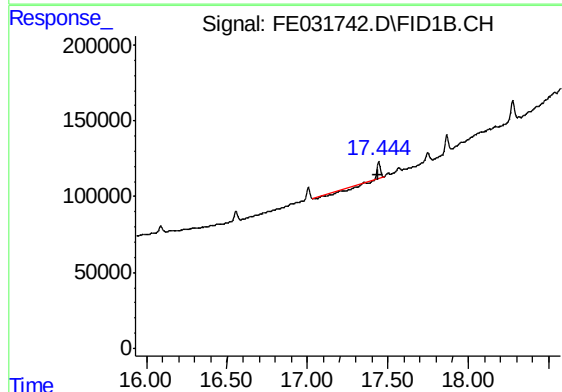


#13 N-TRIACONTANE

R.T.: 17.443 min  
Delta R.T.: 0.005 min  
Response: 20301  
Conc: 0.05 ug/ml

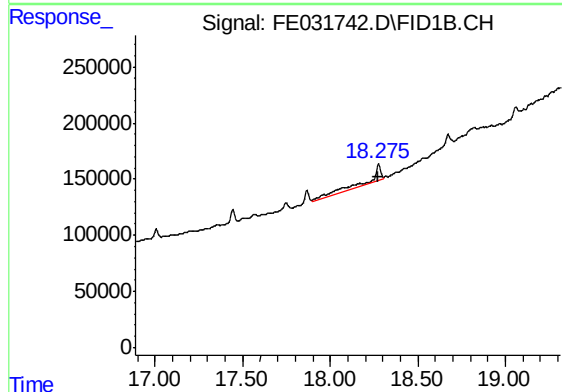

#14 N-DOTRIACONTANE

R.T.: 18.275 min  
Delta R.T.: 0.006 min  
Response: 684231  
Conc: 1.74 ug/ml

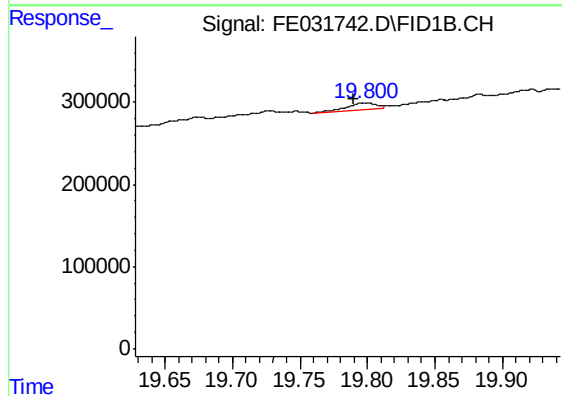

#16 N-HEXATRIACONTANE

R.T.: 19.799 min  
Delta R.T.: 0.009 min  
Response: 138210  
Conc: 0.40 ug/ml