

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041423AL\
Data File : FE041354.D
Signal(s) : FID1B.ch
Acq On : 14 Apr 2023 08:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 15 01:19:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.834	10494	0.067 ug/ml
20) T	n-Hexatriacontane (C36)	20.436f	206743	1.361 ug/ml
21) T	n-Octatriacontane (C38)	21.088	44554	0.285 ug/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041423AL\
Data File : FE041354.D
Signal(s) : FID1B.ch
Acq On : 14 Apr 2023 08:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 15 01:19:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um



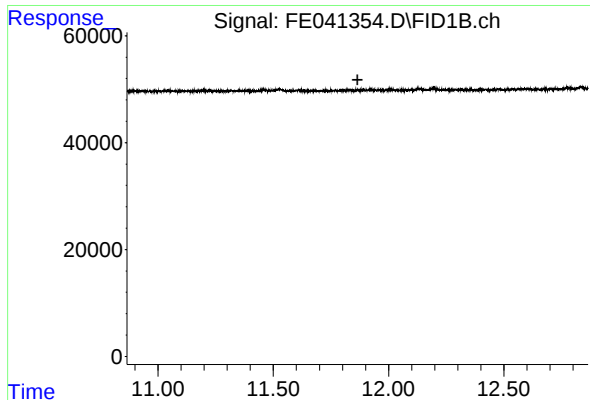


#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :


FID_E

ClientSampleId :

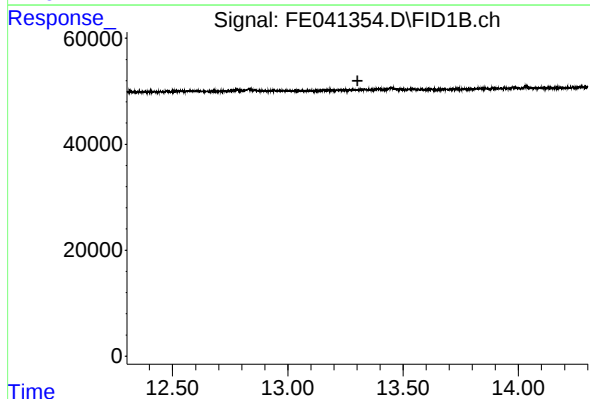


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

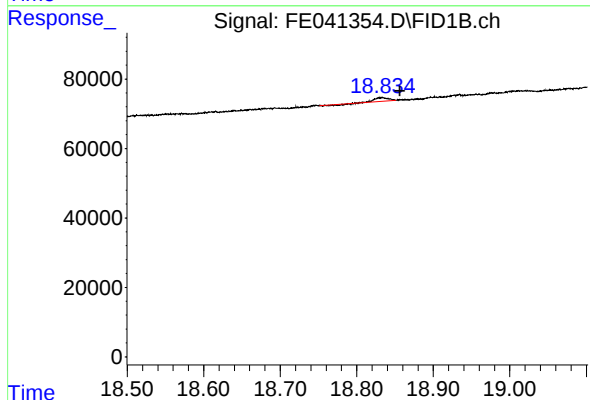


#18 n-Dotriacontane (C32)

R.T.: 18.834 min
Delta R.T.: -0.023 min
Response: 10494
Conc: 0.07 ug/ml

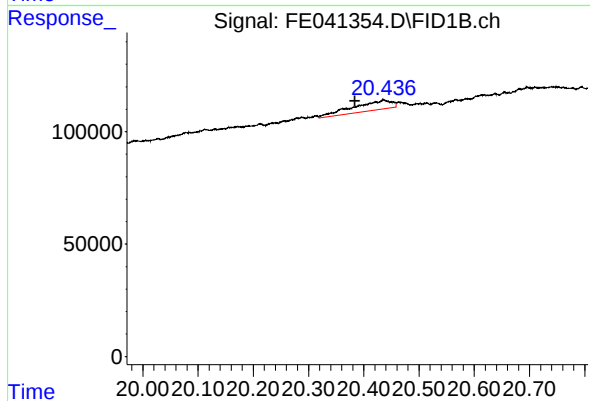

#20 n-Hexatriacontane (C36)

R.T.: 20.436 min
Delta R.T.: 0.052 min
Response: 206743
Conc: 1.36 ug/ml

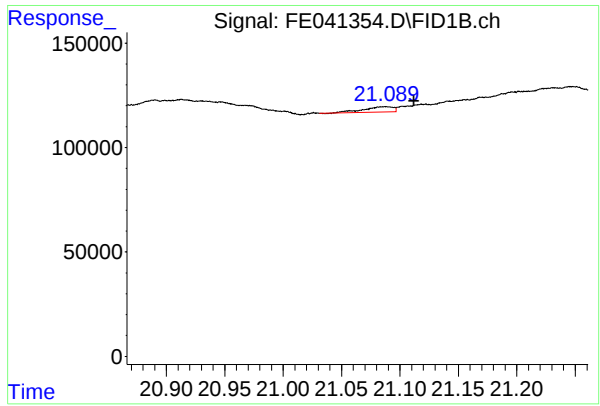

#21 n-Octatriacontane (C38)

R.T.: 21.088 min
Delta R.T.: -0.025 min
Response: 44554
Conc: 0.29 ug/ml

Instrument :

FID_E

ClientSampleId :