

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041423AL\
 Data File : FE041373.D
 Signal(s) : FID1B.ch
 Acq On : 14 Apr 2023 20:45
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 15 01:23:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 25 06:32:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
15) T n-Hexacosane (C26)	16.161	11107	0.072 ug/ml
16) T n-Octacosane (C28)	17.110	12399	0.081 ug/ml
17) T n-Tricontane (C30)	18.001	2429	0.016 ug/ml
18) T n-Dotriacontane (C32)	18.833	71954	0.461 ug/ml
19) T n-Tetratriacontane (C34)	19.628	45541	0.294 ug/ml
20) T n-Hexatriacontane (C36)	20.368	238439	1.570 ug/ml
21) T n-Octatriacontane (C38)	21.104	36330	0.233 ug/ml
22) T n-Tetracontane (C40)	21.975	19123	0.120 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041423AL\
Data File : FE041373.D
Signal(s) : FID1B.ch
Acq On : 14 Apr 2023 20:45
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 15 01:23:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

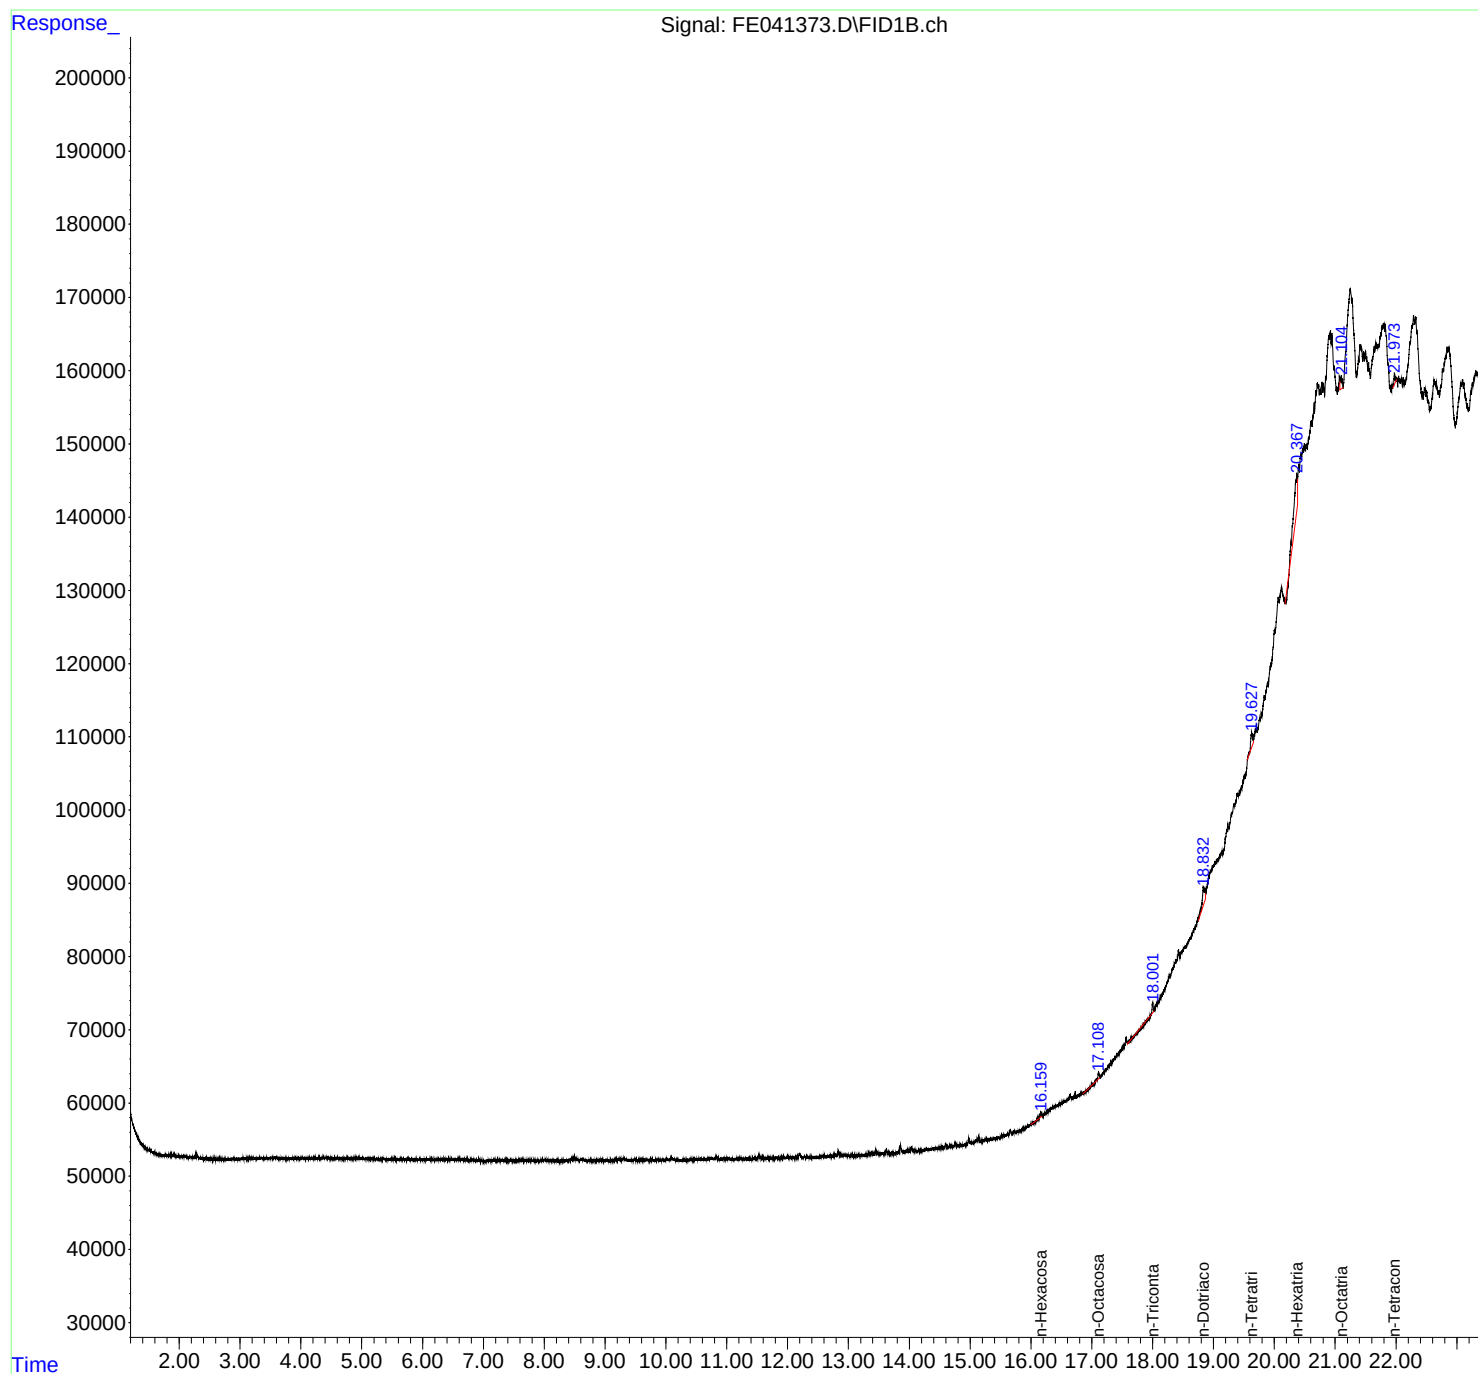


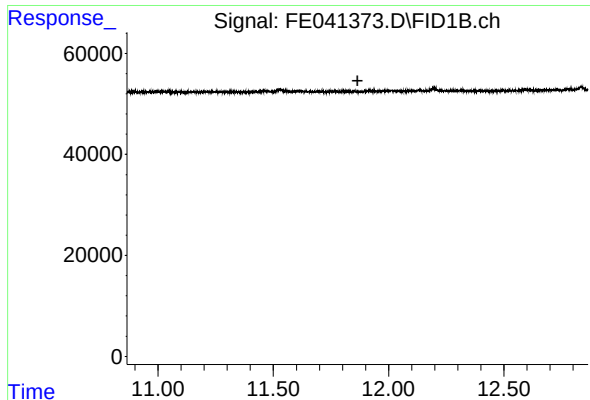

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

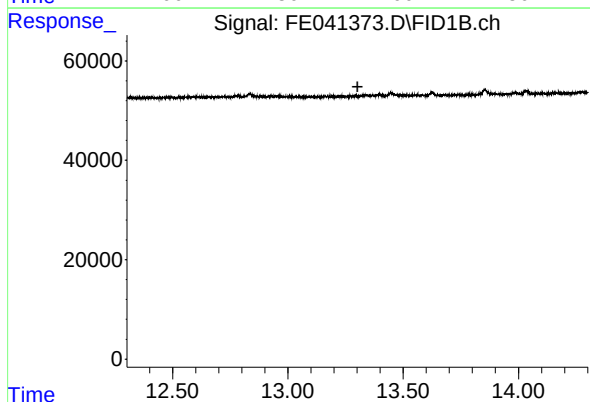


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

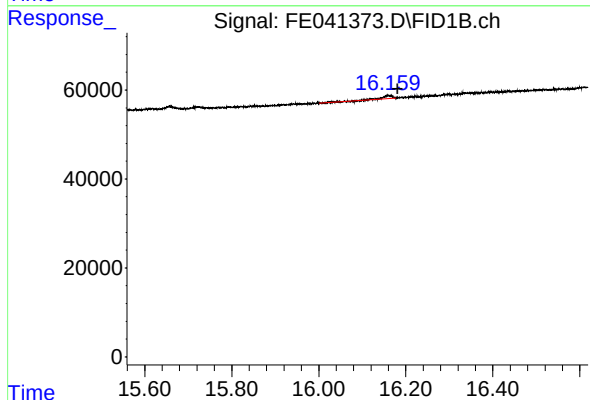


#15 n-Hexacosane (C26)

R.T.: 16.161 min
Delta R.T.: -0.021 min
Response: 11107
Conc: 0.07 ug/ml

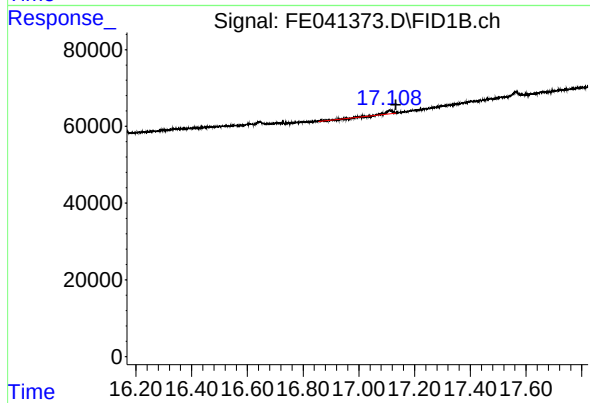

#16 n-Octacosane (C28)


R.T.: 17.110 min
Delta R.T.: -0.023 min
Response: 12399
Conc: 0.08 ug/ml

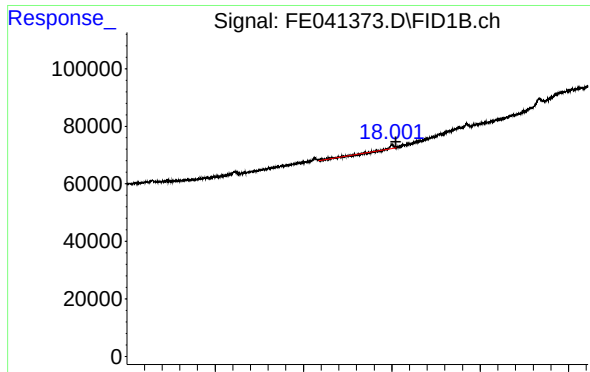

#17 n-Tricontane (C30)


R.T.: 18.001 min
Delta R.T.: -0.021 min
Response: 2429
Conc: 0.02 ug/ml

Instrument :
FID_E
ClientSampleId :

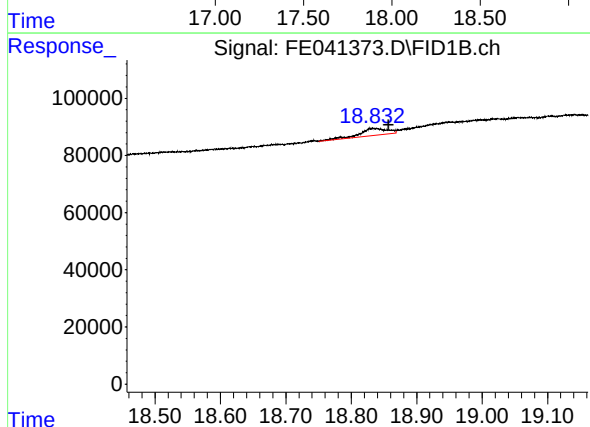


#18 n-Dotriacontane (C32)

R.T.: 18.833 min
Delta R.T.: -0.023 min
Response: 71954
Conc: 0.46 ug/ml

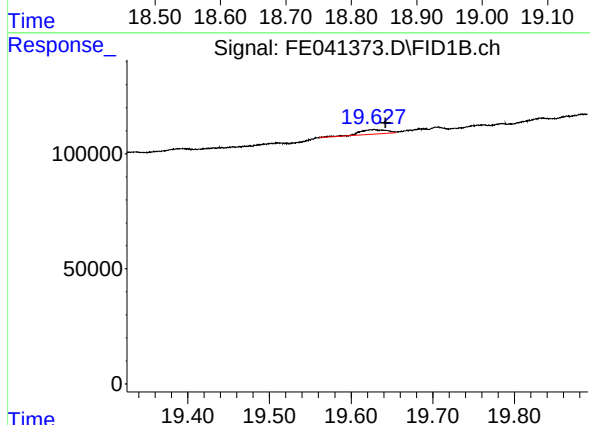


#19 n-Tetratriacontane (C34)

R.T.: 19.628 min
Delta R.T.: -0.014 min
Response: 45541
Conc: 0.29 ug/ml

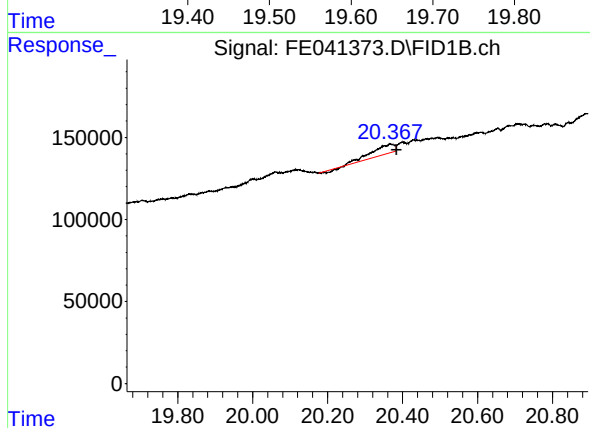

#20 n-Hexatriacontane (C36)


R.T.: 20.368 min
Delta R.T.: -0.017 min
Response: 238439
Conc: 1.57 ug/ml

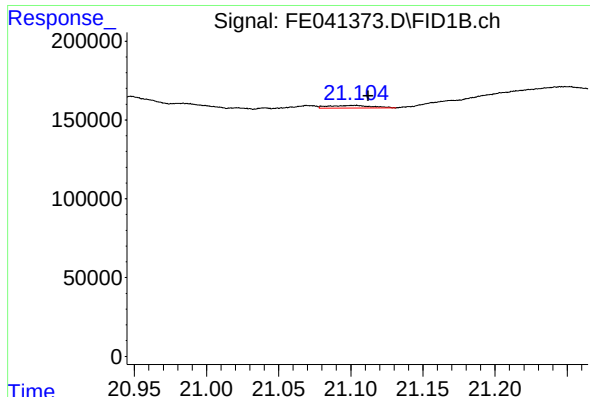

#21 n-Octatriacontane (C38)

R.T.: 21.104 min
Delta R.T.: -0.009 min
Response: 36330
Conc: 0.23 ug/ml

Instrument :
FID_E
ClientSampleId :

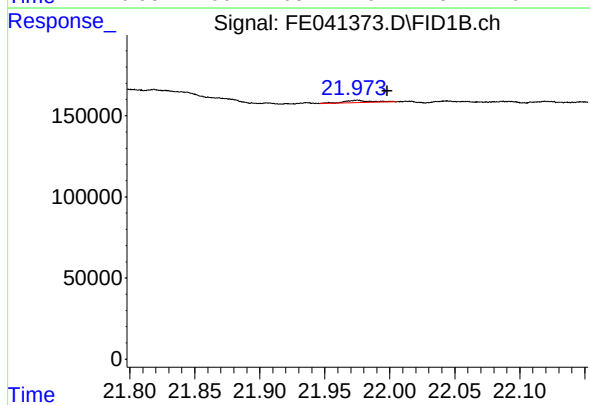

#22 n-Tetracontane (C40)

R.T.: 21.975 min
Delta R.T.: -0.023 min
Response: 19123
Conc: 0.12 ug/ml