

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041620\
 Data File : FE031752.D
 Signal(s) : FID1B.CH
 Acq On : 16 Apr 2020 19:09
 Operator : DD\AJ
 Sample : L2284-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 17 01:57:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
 Quant Title :
 QLast Update : Tue Apr 07 15:06:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.384	6873137	18.872 ug/ml
Target Compounds			
4) N-TETRADECANE	8.005f	3181718	8.027 ug/ml
8) N-DOCOSANE	13.479	289340	0.682 ug/ml
10) N-TETRACOSANE	14.581	222292	0.531 ug/ml
11) N-HEXACOSANE	15.601	948092	2.288 ug/ml
12) N-OCTACOSANE	16.554	2711598	6.591 ug/ml
13) N-TRIACONTANE	17.440	2950440	7.174 ug/ml
14) N-DOTRIACONTANE	18.271	1566081	3.983 ug/ml
15) N-TETRATRIACONTANE	19.054	254857	0.688 ug/ml
16) N-HEXATRIACONTANE	19.796	567476	1.646 ug/ml
17) N-OCTATRIACONTANE	20.496	5828248	18.846 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041620\
Data File : FE031752.D
Signal(s) : FID1B.CH
Acq On : 16 Apr 2020 19:09
Operator : DD\AJ
Sample : L2284-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 17 01:57:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
Quant Title :
QLast Update : Tue Apr 07 15:06:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

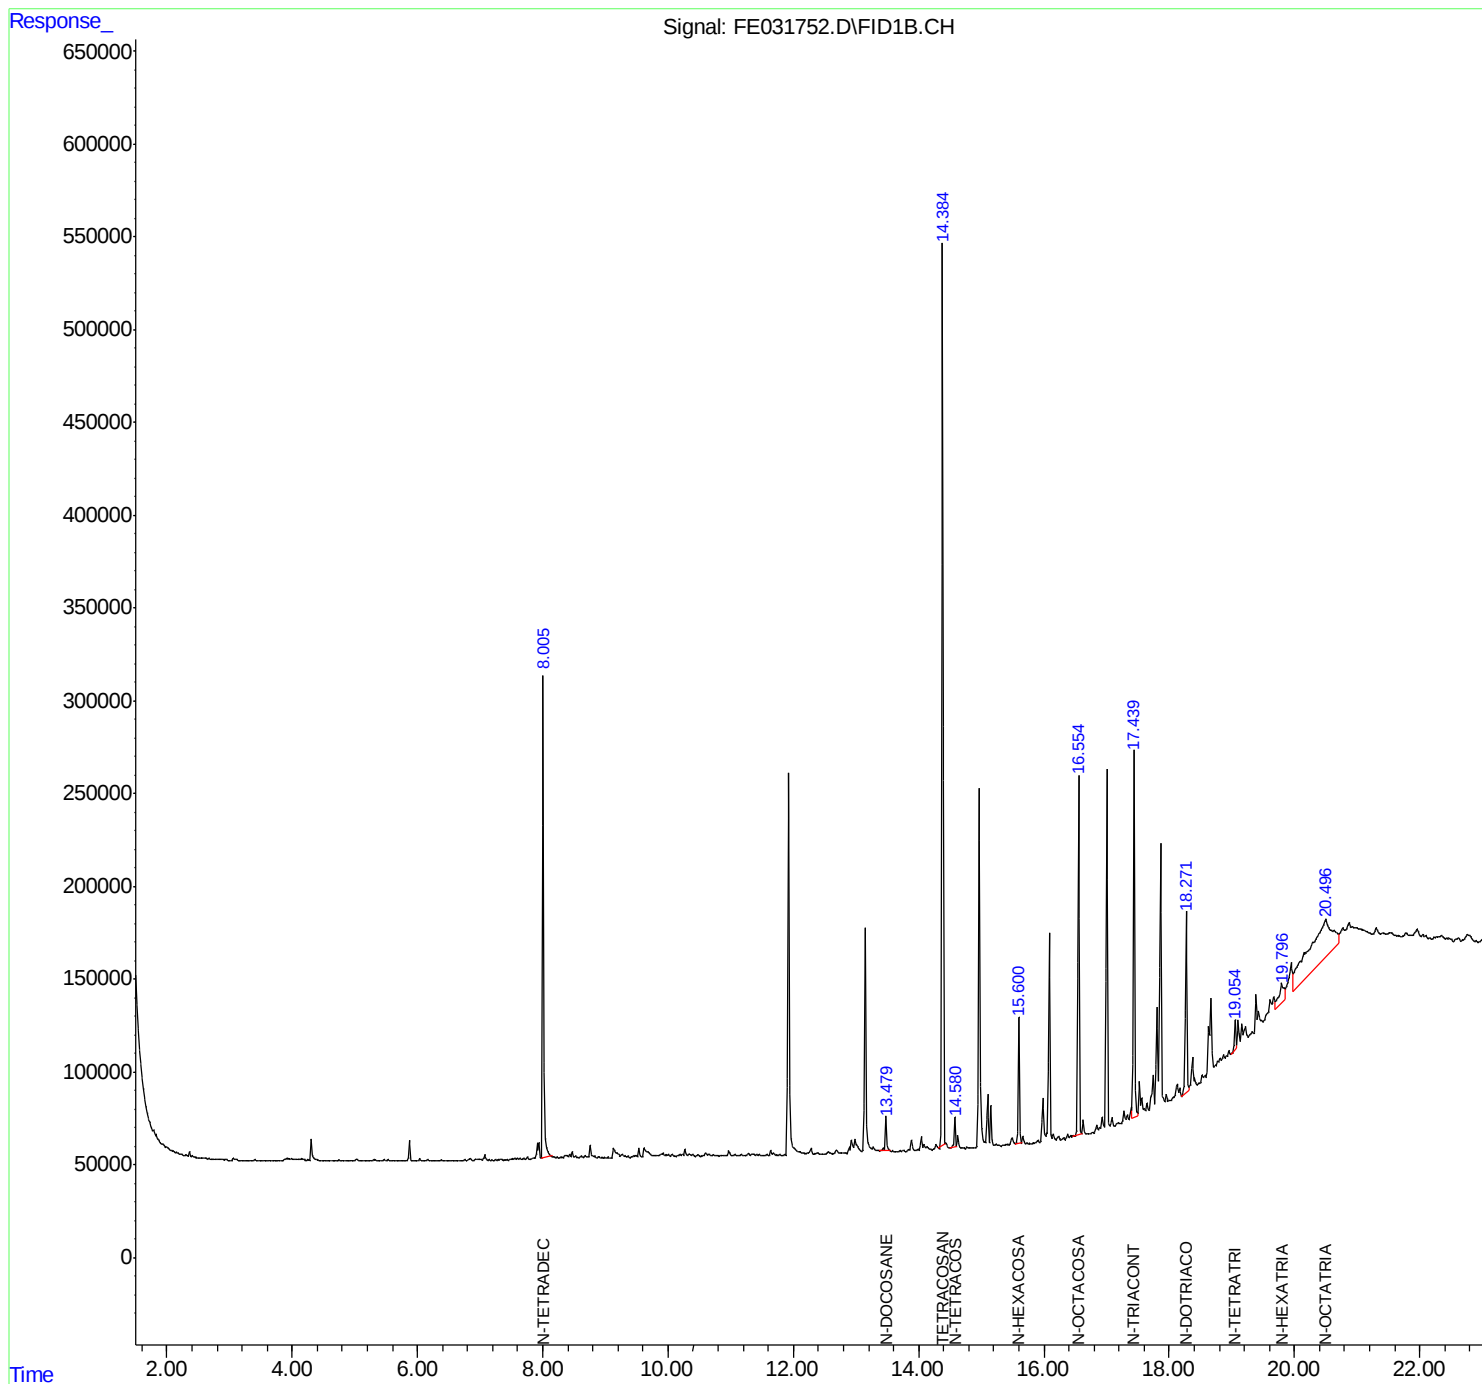

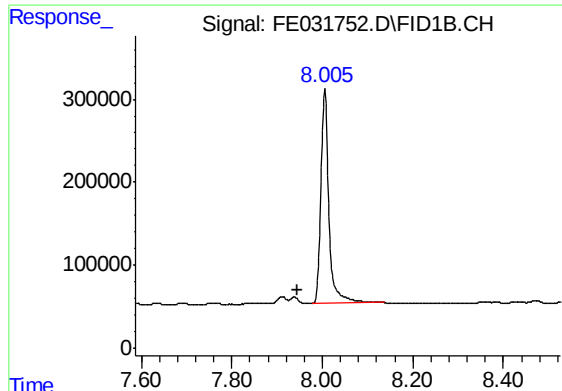


#4 N-TETRADECANE

R.T.: 8.005 min
Delta R.T.: 0.061 min
Response: 3181718
Conc: 8.03 ug/ml

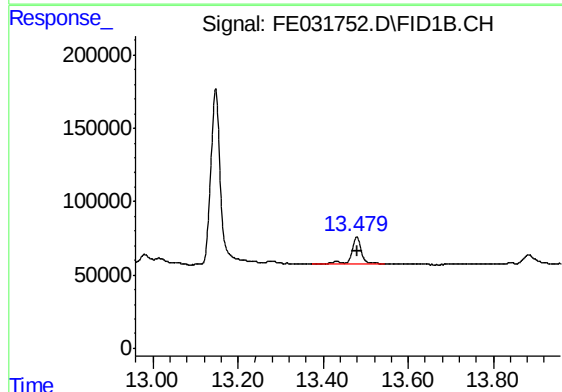


#8 N-DOCOSANE

R.T.: 13.479 min
Delta R.T.: -0.003 min
Response: 289340
Conc: 0.68 ug/ml

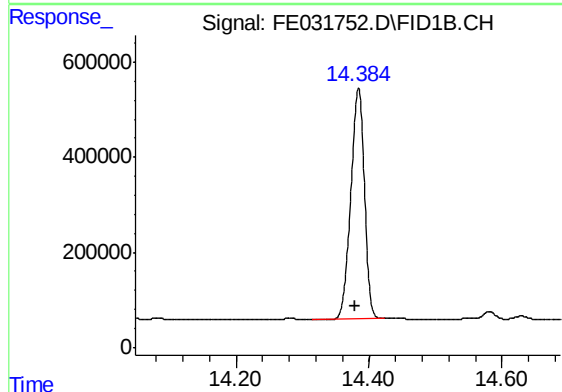


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.384 min
Delta R.T.: 0.005 min
Response: 6873137
Conc: 18.87 ug/ml

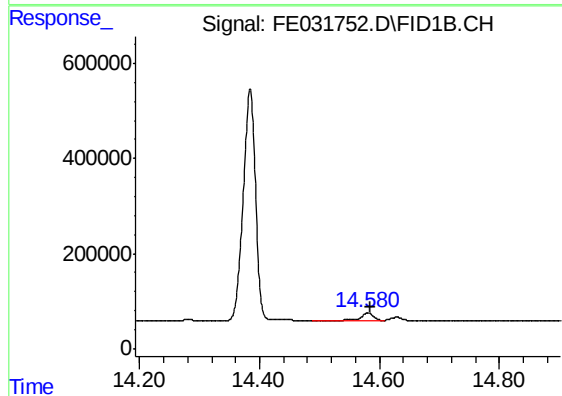


#10 N-TETRACOSANE

R.T.: 14.581 min
Delta R.T.: -0.003 min
Response: 222292
Conc: 0.53 ug/ml

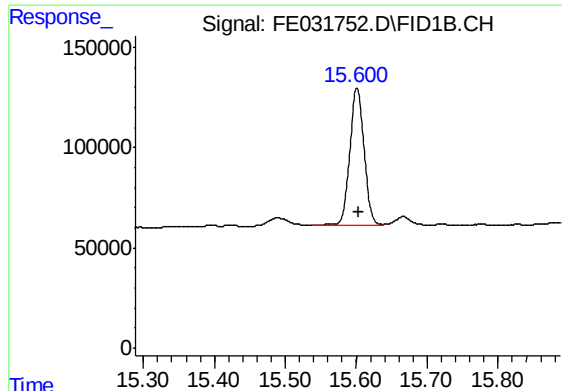


#11 N-HEXACOSANE

R.T.: 15.601 min
Delta R.T.: -0.002 min
Response: 948092
Conc: 2.29 ug/ml

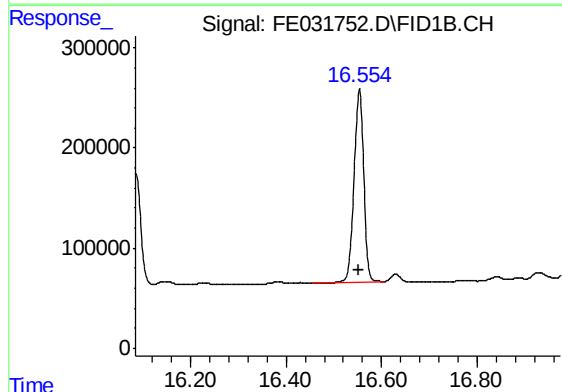


#12 N-OCTACOSANE

R.T.: 16.554 min
Delta R.T.: 0.001 min
Response: 2711598
Conc: 6.59 ug/ml

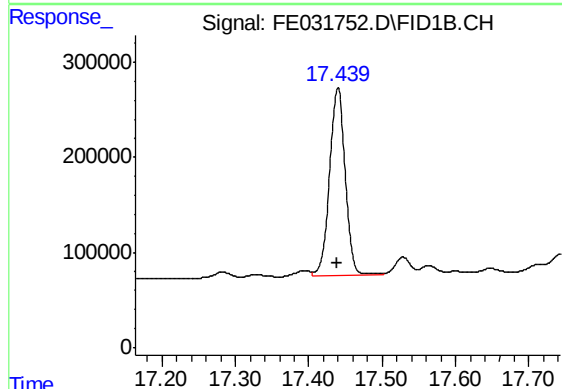


#13 N-TRIACONTANE

R.T.: 17.440 min
Delta R.T.: 0.001 min
Response: 2950440
Conc: 7.17 ug/ml

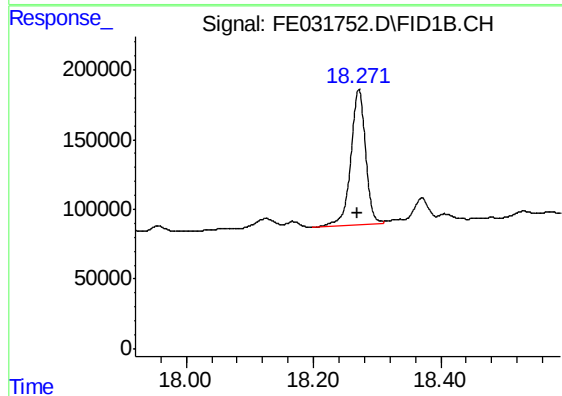


#14 N-DOTRIACONTANE

R.T.: 18.271 min
Delta R.T.: 0.001 min
Response: 1566081
Conc: 3.98 ug/ml

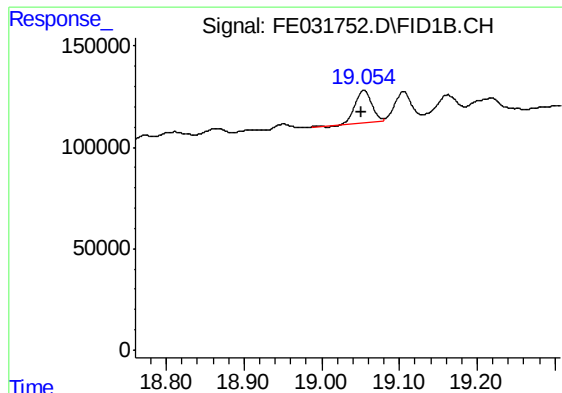


#15 N-TETRATRIACONTANE

R.T.: 19.054 min
Delta R.T.: 0.003 min
Response: 254857
Conc: 0.69 ug/ml

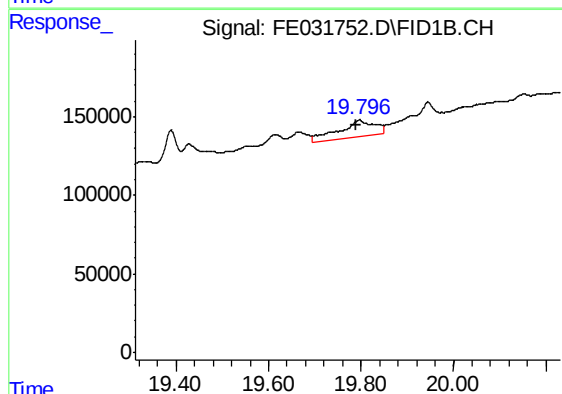

#16 N-HEXATRIACONTANE

R.T.: 19.796 min
Delta R.T.: 0.006 min
Response: 567476
Conc: 1.65 ug/ml

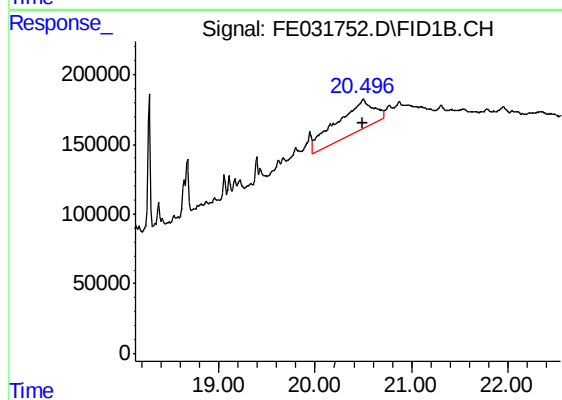

#17 N-OCTATRIACONTANE

R.T.: 20.496 min
Delta R.T.: 0.005 min
Response: 5828248
Conc: 18.85 ug/ml