

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041719\
 Data File : FE029887.D
 Signal(s) : FID1B.CH
 Acq On : 17 Apr 2019 14:03
 Operator : AJ\SJ
 Sample : PB118964BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Apr 18 02:07:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
 Quant Title :
 QLast Update : Wed Apr 10 08:20:21 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.634	4328716	21.338 ug/ml
Target Compounds			
2) N-DECANE	4.376	4889739	22.252 ug/ml
3) N-DODECANE	6.384	4981153	22.238 ug/ml
4) N-TETRADECANE	8.178	5054171	21.886 ug/ml
5) N-HEXADECANE	9.780	5105330	21.714 ug/ml
6) N-OCTADECANE	11.222	5133524	21.620 ug/ml
7) N-EICOSANE	12.534	5076390	21.424 ug/ml
8) N-DOCOSANE	13.734	5001555	21.298 ug/ml
10) N-TETRACOSANE	14.839	4942568	21.297 ug/ml
11) N-HEXACOSANE	15.861	4873130	21.133 ug/ml
12) N-OCTACOSANE	16.812	4886930	21.224 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041719\
Data File : FE029887.D
Signal(s) : FID1B.CH
Acq On : 17 Apr 2019 14:03
Operator : AJ\SJ
Sample : PB118964BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Apr 18 02:07:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
Quant Title :
QLast Update : Wed Apr 10 08:20:21 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

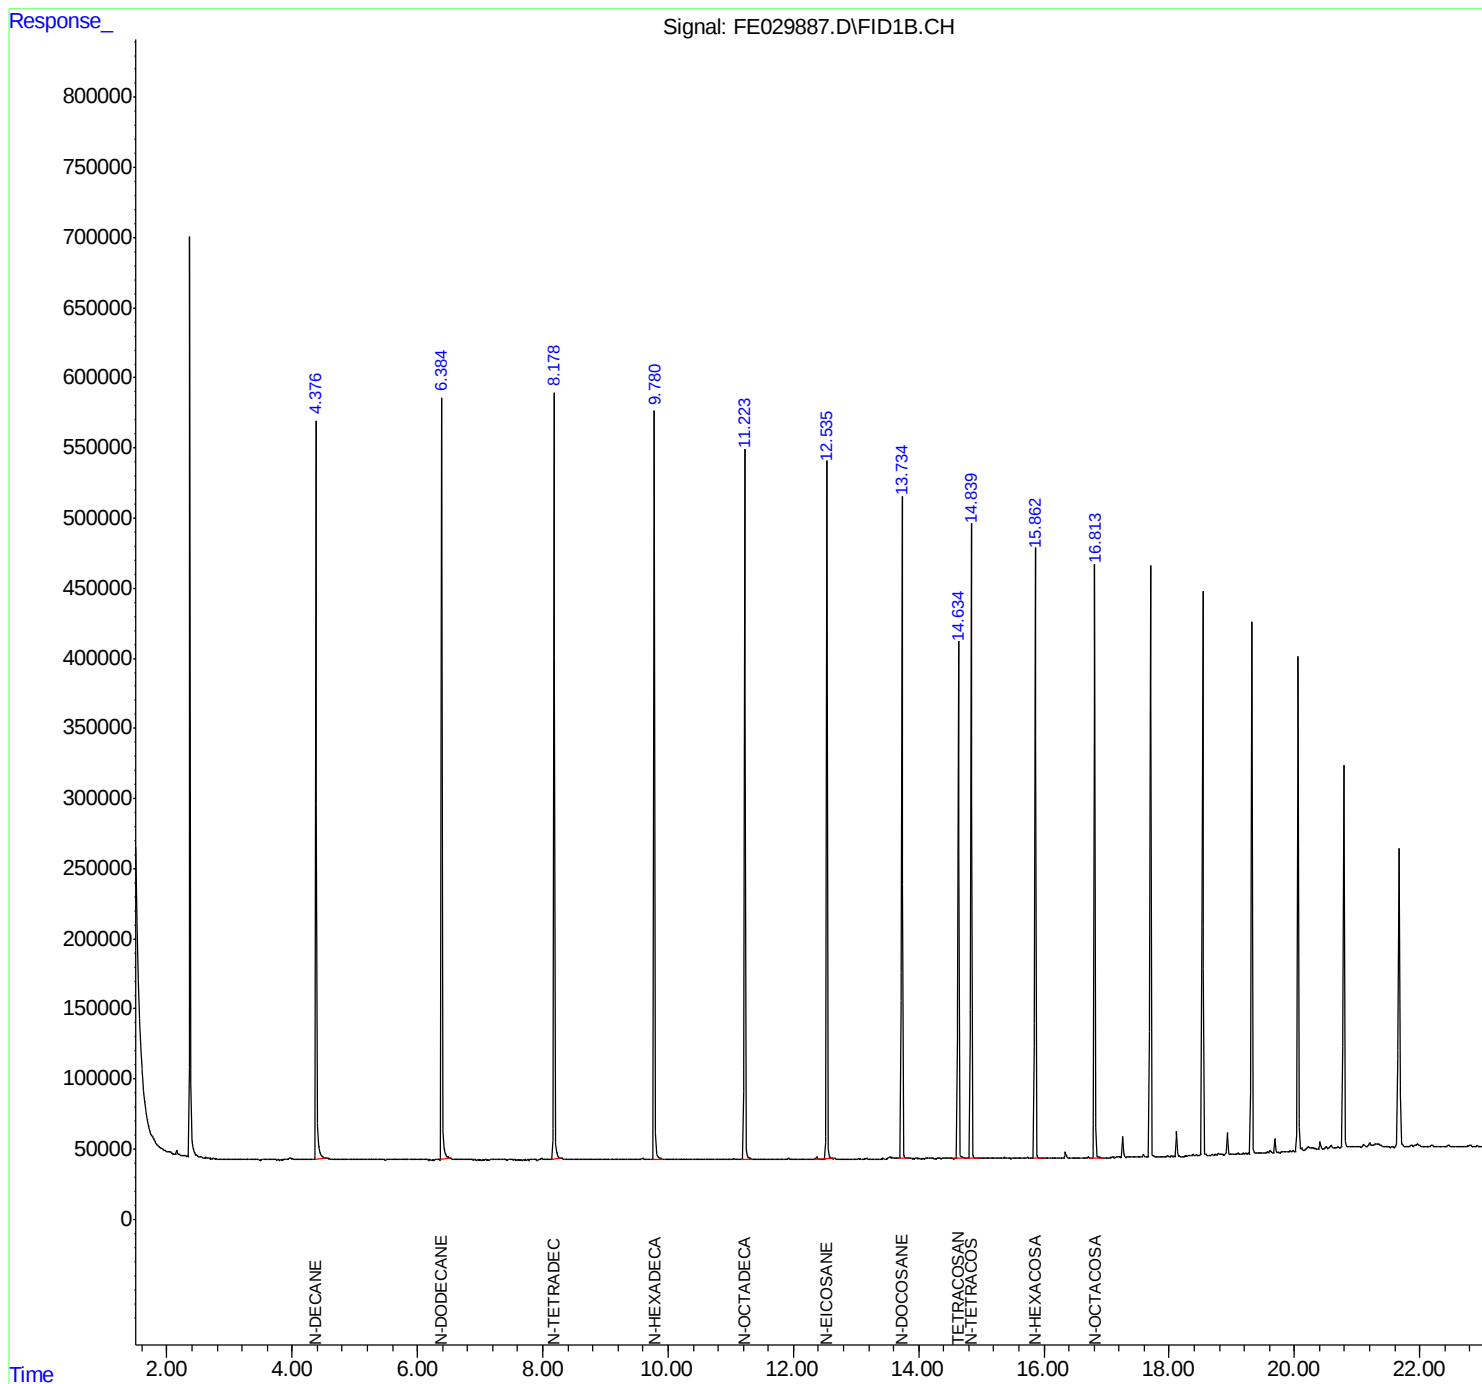

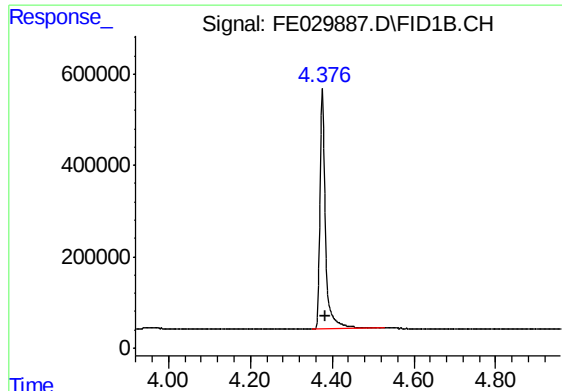


#2 N-DECANE

R.T.: 4.376 min
Delta R.T.: -0.009 min
Response: 4889739
Conc: 22.25 ug/ml

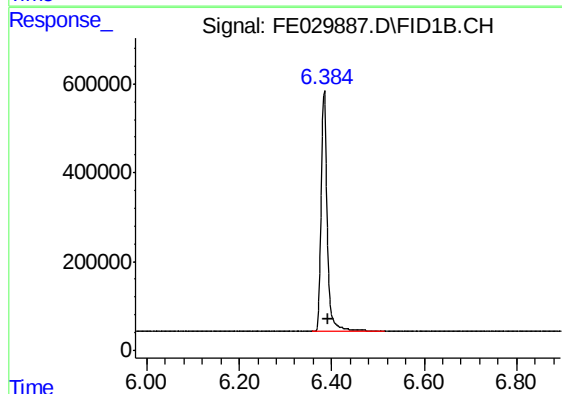


#3 N-DODECANE

R.T.: 6.384 min
Delta R.T.: -0.008 min
Response: 4981153
Conc: 22.24 ug/ml

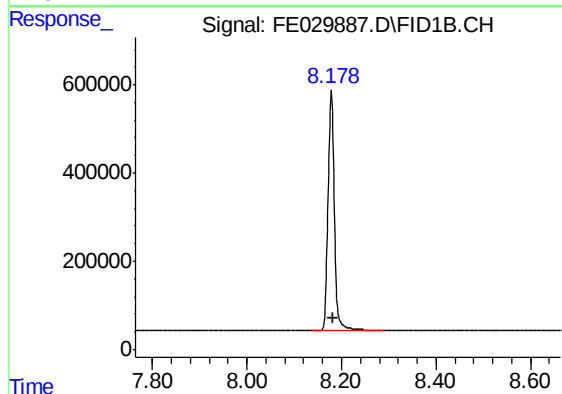


#4 N-TETRADECANE

R.T.: 8.178 min
Delta R.T.: -0.005 min
Response: 5054171
Conc: 21.89 ug/ml

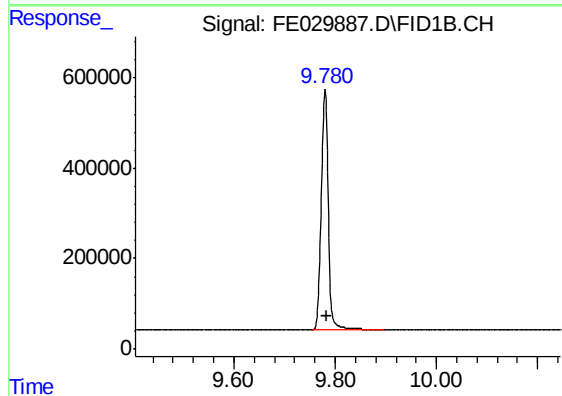


#5 N-HEXADECANE

R.T.: 9.780 min
Delta R.T.: -0.004 min
Response: 5105330
Conc: 21.71 ug/ml

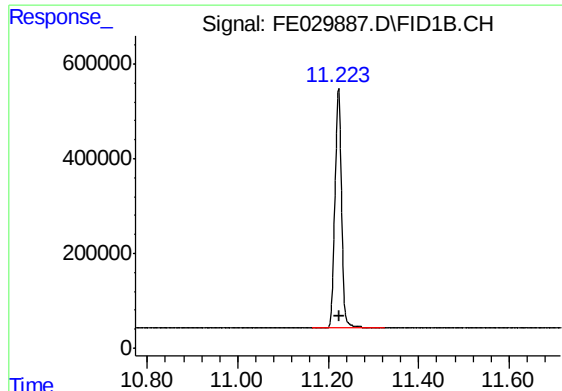


#6 N-OCTADECANE

R.T.: 11.222 min
Delta R.T.: -0.004 min
Response: 5133524
Conc: 21.62 ug/ml

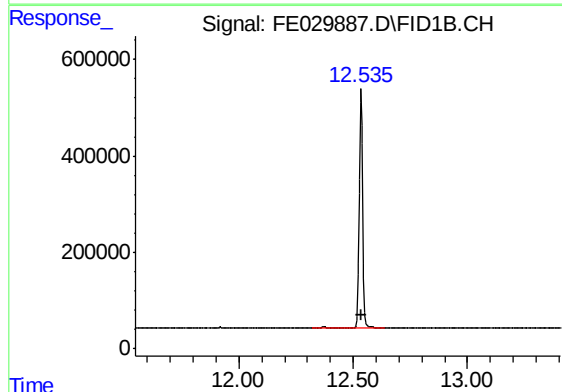


#7 N-EICOSANE

R.T.: 12.534 min
Delta R.T.: -0.002 min
Response: 5076390
Conc: 21.42 ug/ml

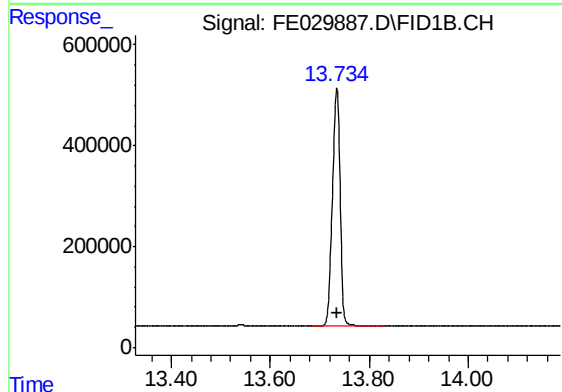


#8 N-DOCOSANE

R.T.: 13.734 min
Delta R.T.: -0.002 min
Response: 5001555
Conc: 21.30 ug/ml

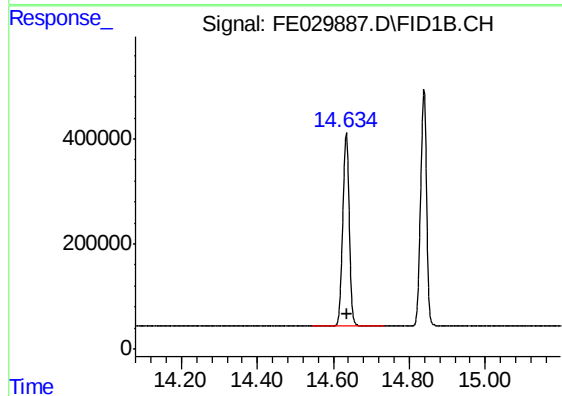


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.634 min
Delta R.T.: -0.003 min
Response: 4328716
Conc: 21.34 ug/ml

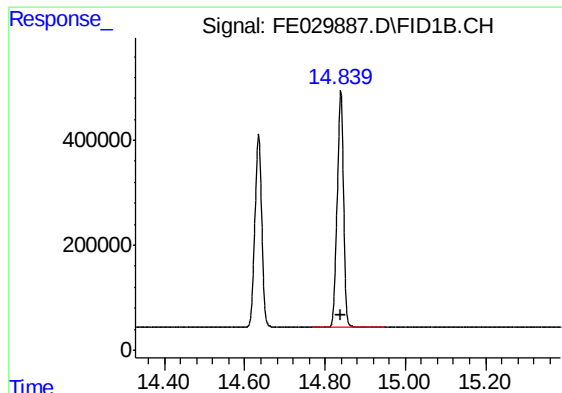


#10 N-TETRACOSANE

R.T.: 14.839 min
Delta R.T.: -0.002 min
Response: 4942568
Conc: 21.30 ug/ml

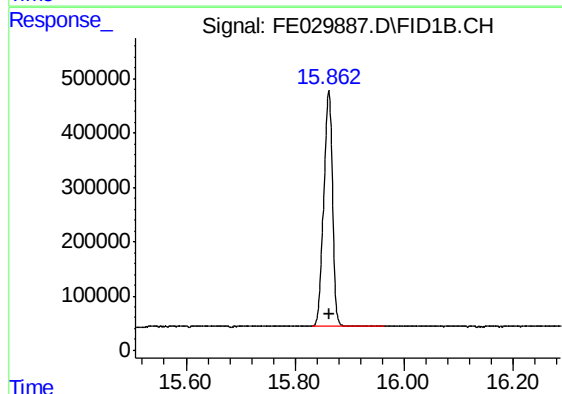

#11 N-HEXACOSANE

R.T.: 15.861 min
Delta R.T.: 0.000 min
Response: 4873130
Conc: 21.13 ug/ml

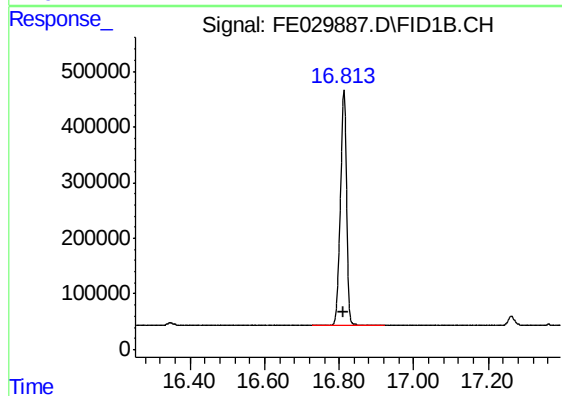

#12 N-OCTACOSANE

R.T.: 16.812 min
Delta R.T.: 0.000 min
Response: 4886930
Conc: 21.22 ug/ml