

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041823AL\
 Data File : FE041399.D
 Signal(s) : FID1B.ch
 Acq On : 18 Apr 2023 08:42
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 18 23:02:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 25 06:32:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) T n-Octacosane (C28)	17.115	9293	0.061 ug/ml
17) T n-Tricontane (C30)	18.005	7812	0.051 ug/ml
18) T n-Dotriacontane (C32)	18.840	41218	0.264 ug/ml
19) T n-Tetratriacontane (C34)	19.626	16249	0.105 ug/ml
21) T n-Octatriacontane (C38)	21.121	89126	0.571 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041823AL\
Data File : FE041399.D
Signal(s) : FID1B.ch
Acq On : 18 Apr 2023 08:42
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 18 23:02:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

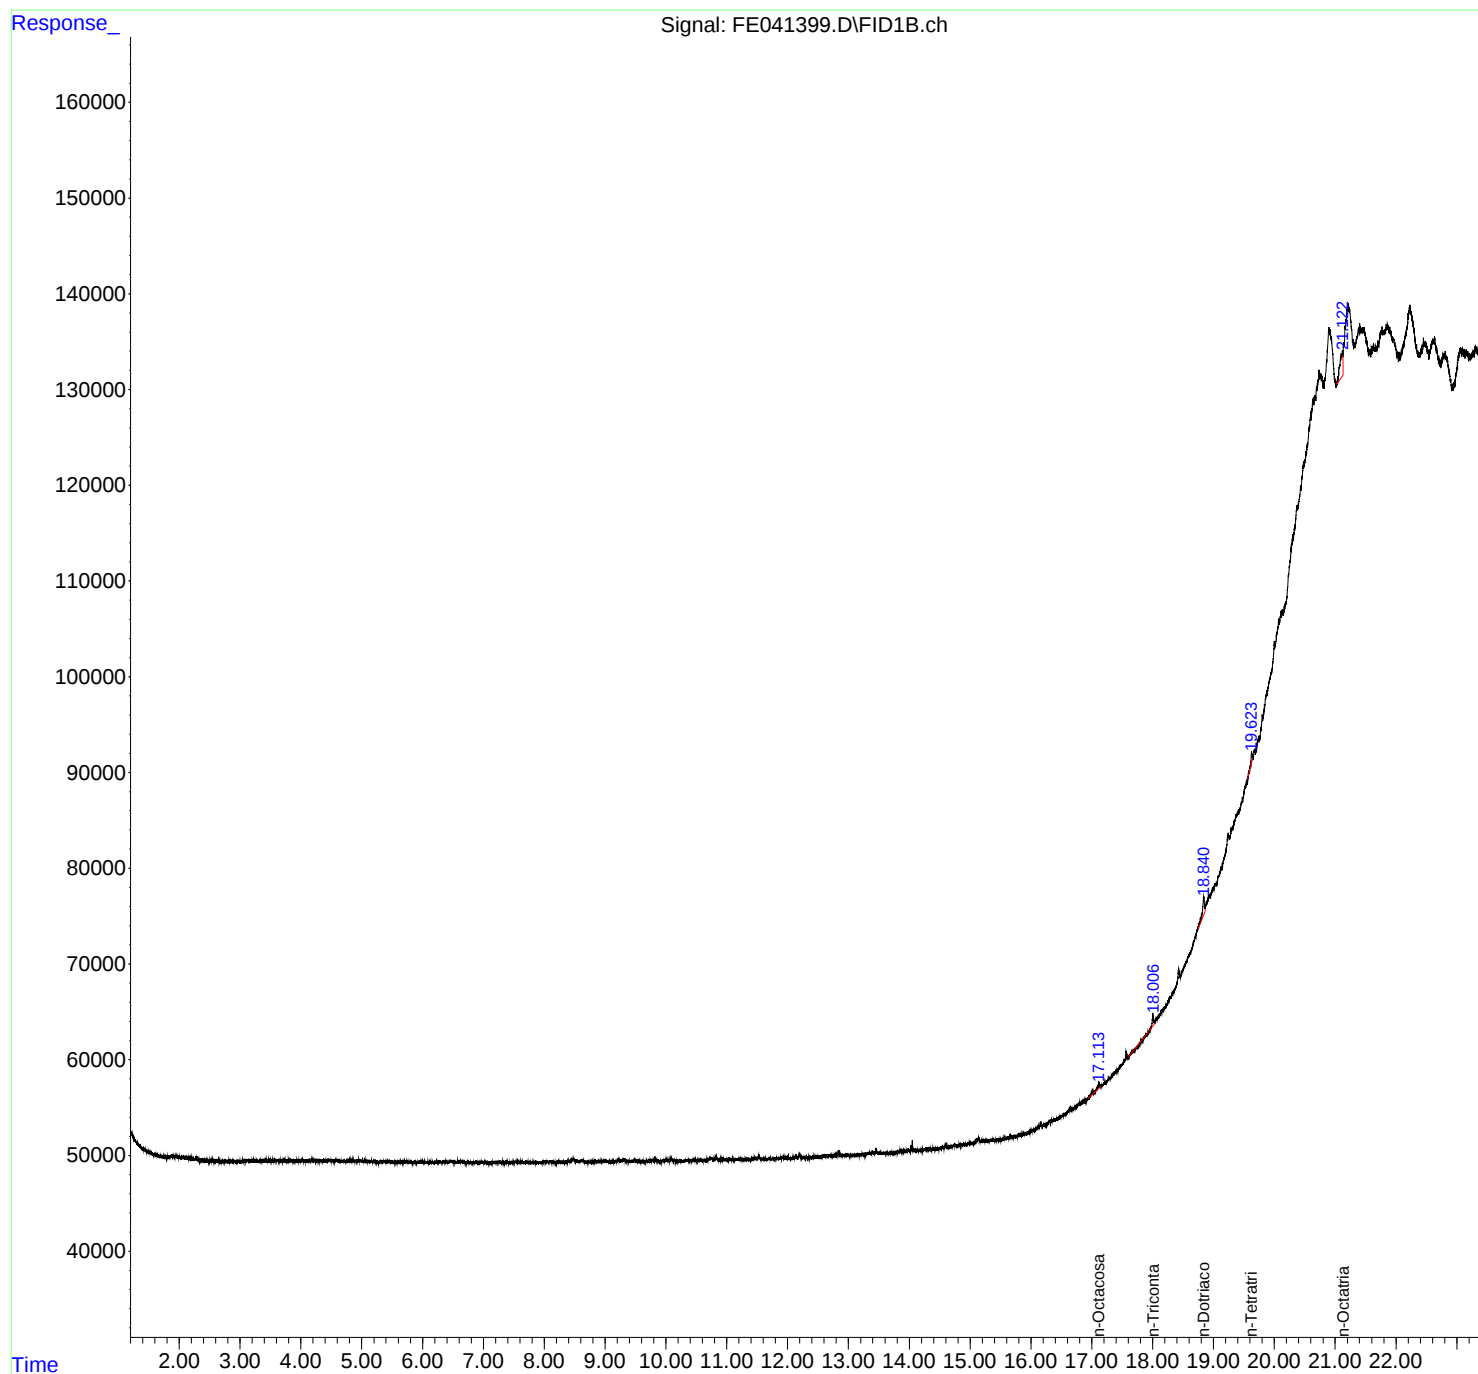


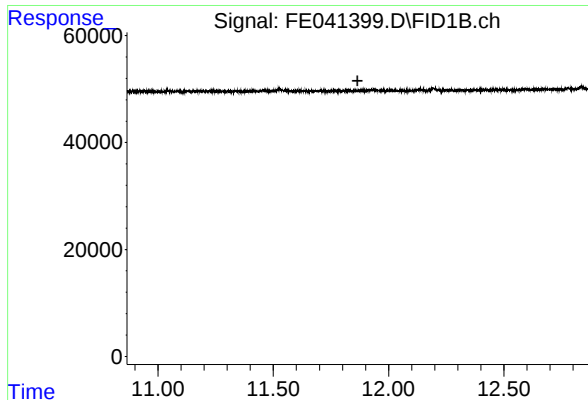

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

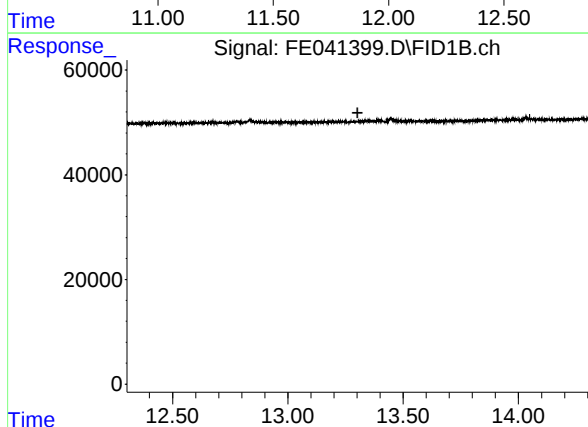


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

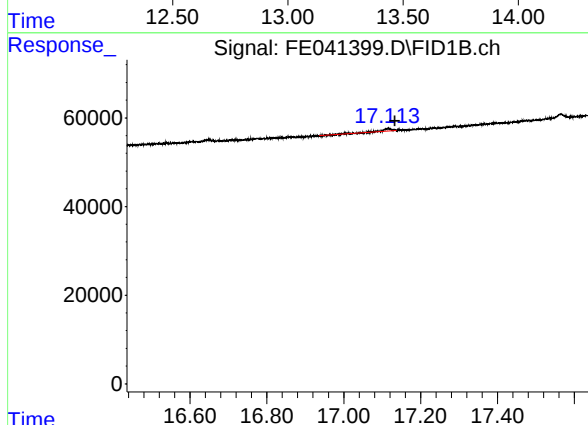


#16 n-Octacosane (C28)

R.T.: 17.115 min
Delta R.T.: -0.018 min
Response: 9293
Conc: 0.06 ug/ml

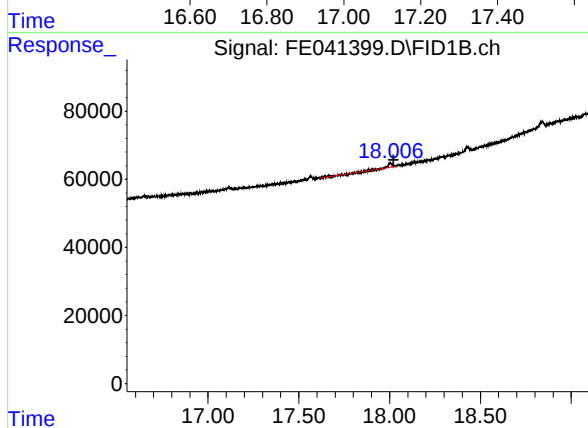

#17 n-Tricontane (C30)

R.T.: 18.005 min
Delta R.T.: -0.017 min
Response: 7812
Conc: 0.05 ug/ml

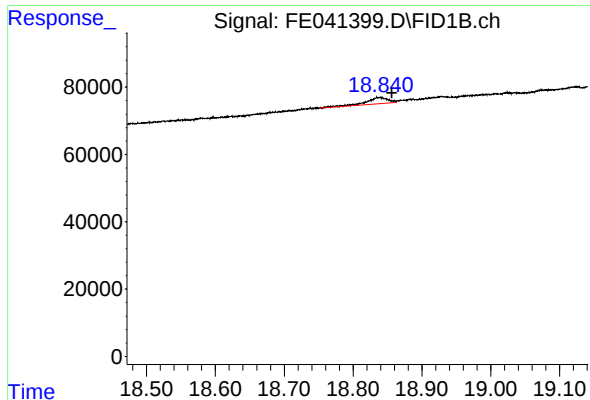


#18 n-Dotriacontane (C32)

R.T.: 18.840 min
Delta R.T.: -0.016 min
Response: 41218
Conc: 0.26 ug/ml

Instrument :


FID_E

ClientSampleId :

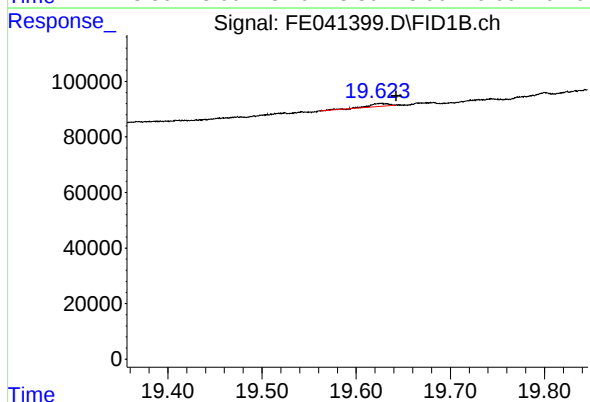

#19 n-Tetratriacontane (C34)

R.T.: 19.626 min
Delta R.T.: -0.017 min
Response: 16249
Conc: 0.10 ug/ml

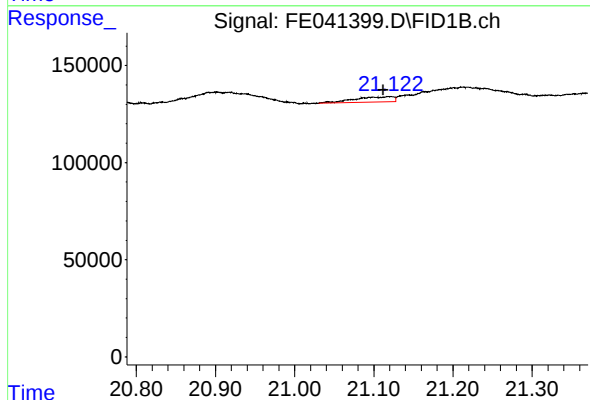

#21 n-Octatriacontane (C38)

R.T.: 21.121 min
Delta R.T.: 0.009 min
Response: 89126
Conc: 0.57 ug/ml