

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE041823AL\  
 Data File : FE041414.D  
 Signal(s) : FID1B.ch  
 Acq On : 18 Apr 2023 17:38  
 Operator : YP\AJ  
 Sample : 02386-14 10X  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 SPA-4WC-23-04

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 04/19/2023  
 Supervised By :Ankita Jodhani 04/19/2023

Integration File: autoint1.e  
 Quant Time: Apr 18 23:04:52 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 032523.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Mar 25 06:32:15 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.847 | 1759587    | 9.362 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 18.72%       |
| 12) S 1-chlorooctadecane (S... | 13.289 | 858562     | 5.967 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 11.93%       |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE041823AL\  
Data File : FE041414.D  
Signal(s) : FID1B.ch  
Acq On : 18 Apr 2023 17:38  
Operator : YP\AJ  
Sample : 02386-14 10X  
Misc :  
ALS Vial : 22 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
SPA-4WC-23-04


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/19/2023  
Supervised By :Ankita Jodhani 04/19/2023

Integration File: autoint1.e  
Quant Time: Apr 18 23:04:52 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 032523.  
Quant Title : GC Extractables  
QLast Update : Sat Mar 25 06:32:15 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

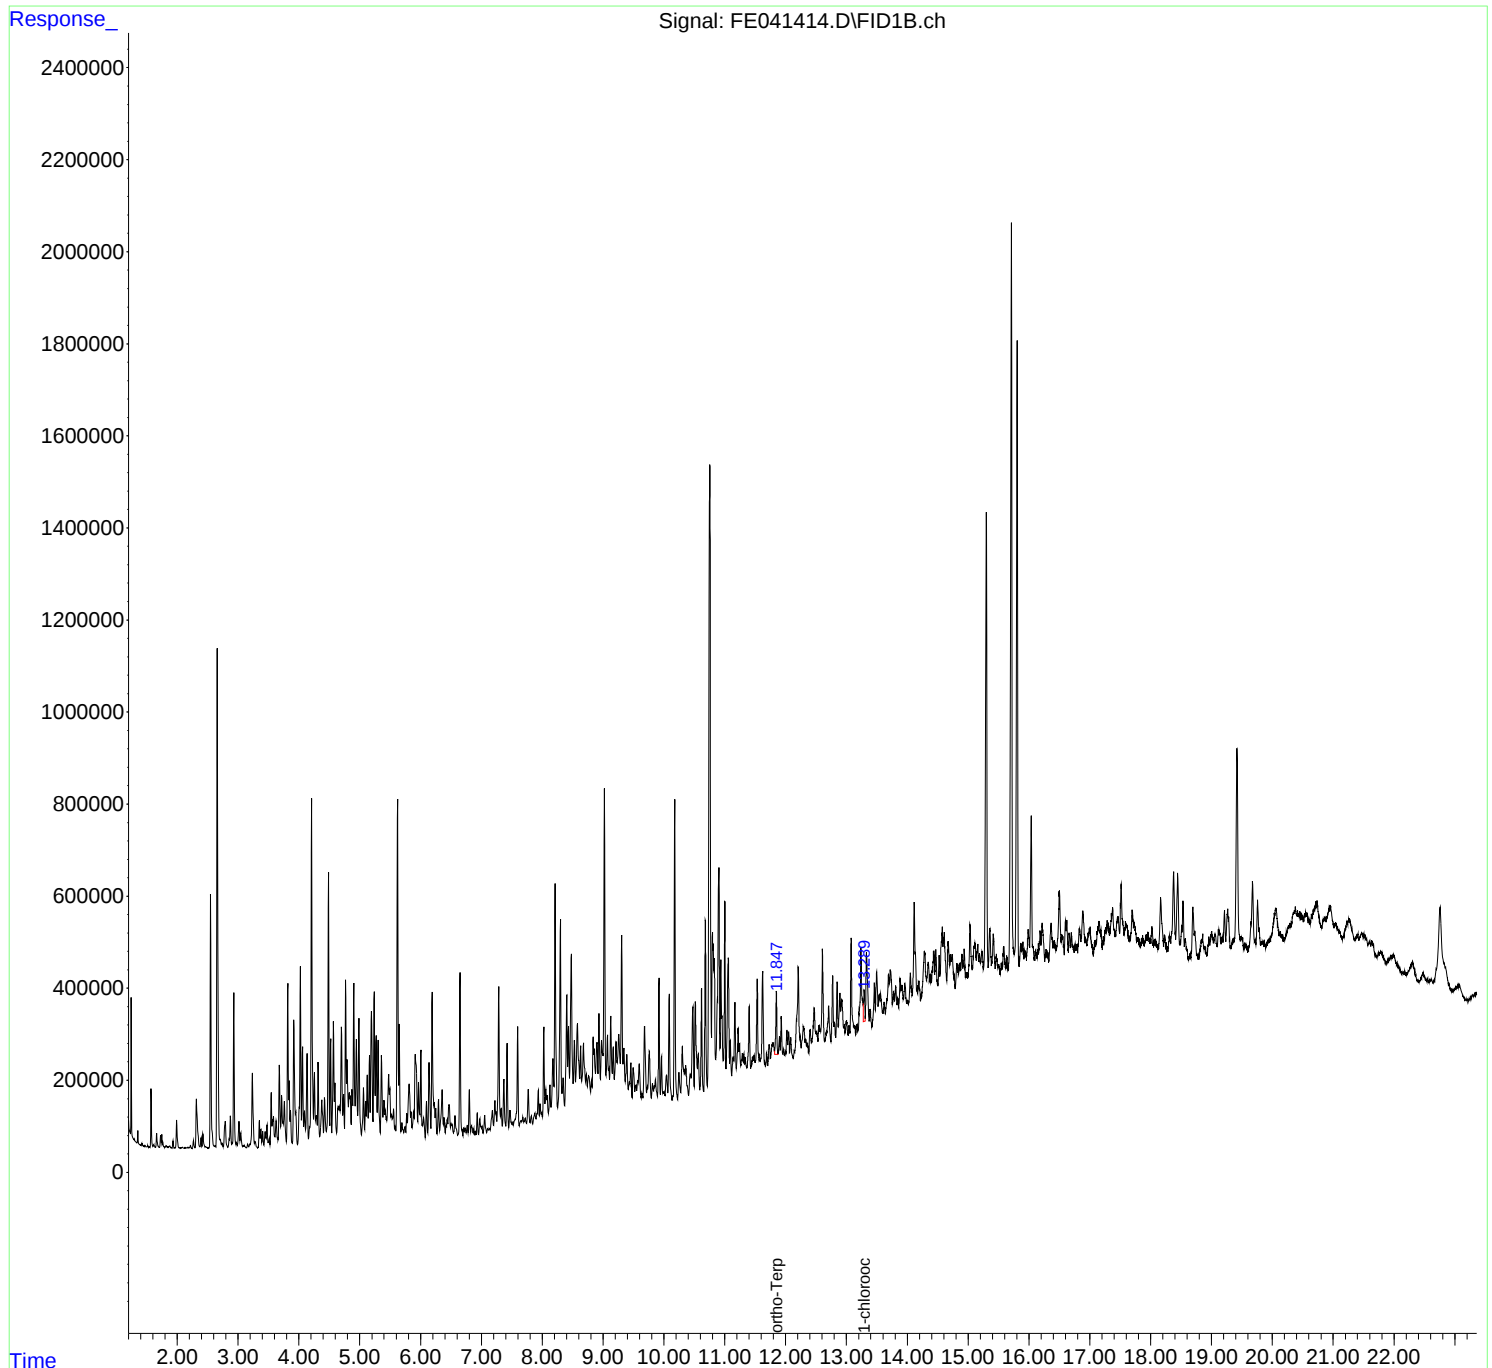

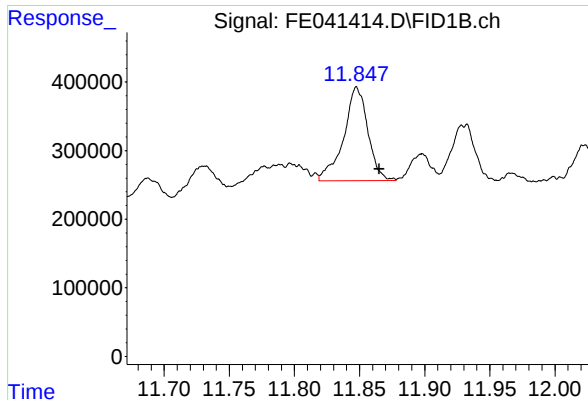


#9 ortho-Terphenyl (SURR)

R.T.: 11.847 min  
Delta R.T.: -0.018 min  
Response: 1759587  
Conc: 9.36 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
SPA-4WC-23-04

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/19/2023  
Supervised By :Ankita Jodhani 04/19/2023

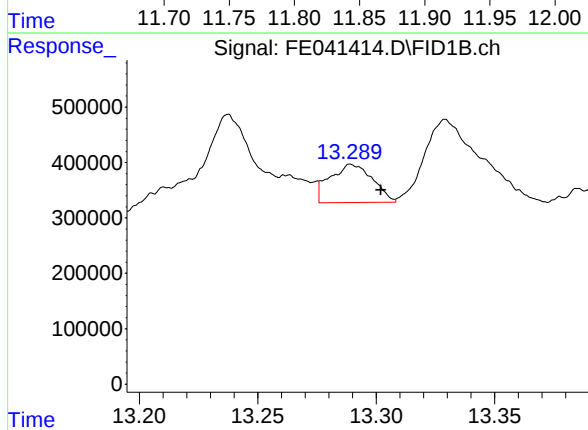

#12 1-chlorooctadecane (SURR)

R.T.: 13.289 min  
Delta R.T.: -0.013 min  
Response: 858562  
Conc: 5.97 ug/ml m