

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041824AL\
 Data File : FE047692.D
 Signal(s) : FID1B.ch
 Acq On : 18 Apr 2024 21:04
 Operator : YP\AJ
 Sample : P2125-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 19 01:25:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 040224.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 02 05:28:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.410	2875177	21.377 ug/ml
Spiked Amount 50.000		Recovery =	42.75%
Target Compounds			
4) T n-Dodecane (C12)	6.775	102160	0.629 ug/ml
6) T n-Tetradecane (C14)	8.603	51529	0.320 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041824AL\
Data File : FE047692.D
Signal(s) : FID1B.ch
Acq On : 18 Apr 2024 21:04
Operator : YP\AJ
Sample : P2125-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 19 01:25:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 040224.M
Quant Title : GC Extractables
QLast Update : Tue Apr 02 05:28:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

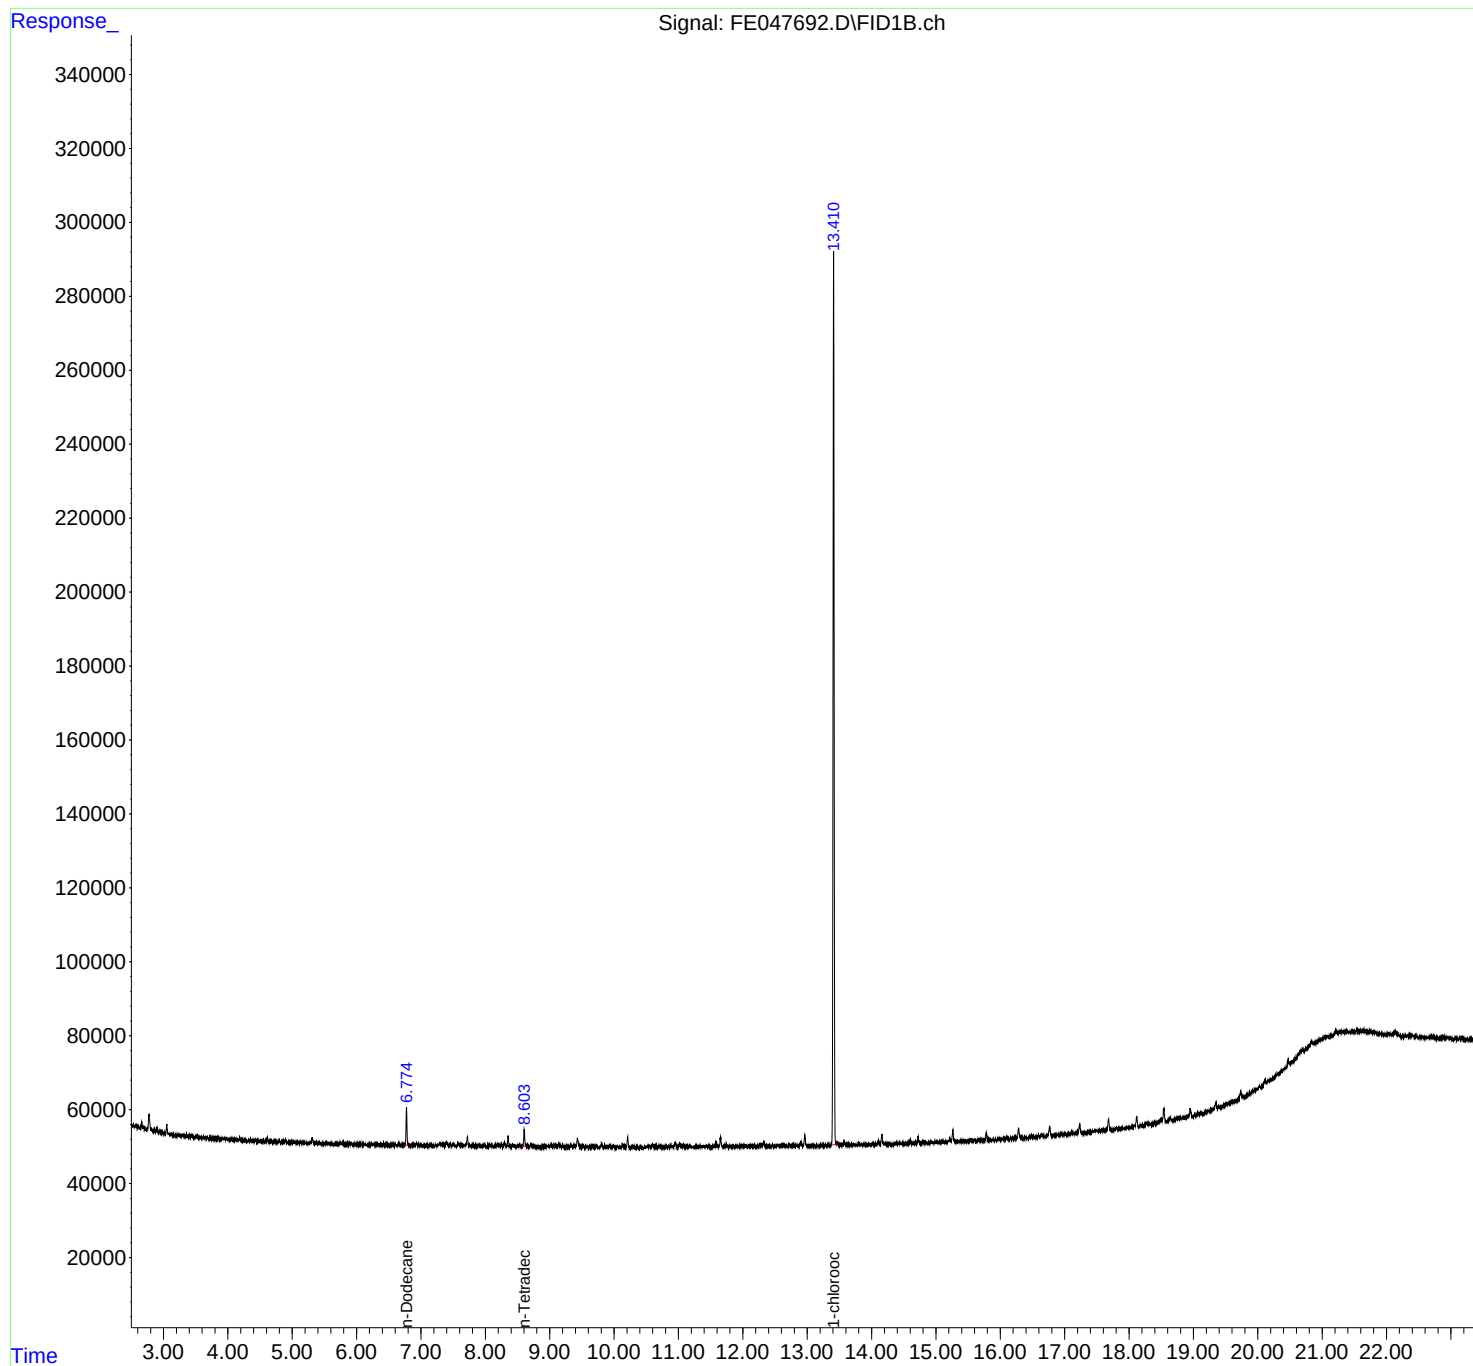


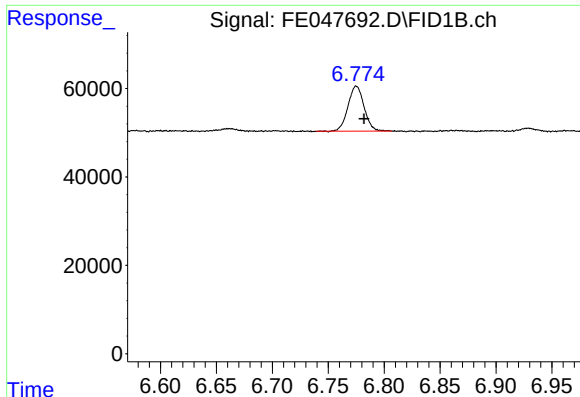

#4 n-Dodecane (C12)


R.T.: 6.775 min
Delta R.T.: -0.007 min
Response: 102160
Conc: 0.63 ug/ml

Instrument :
FID_E
ClientSampleId :

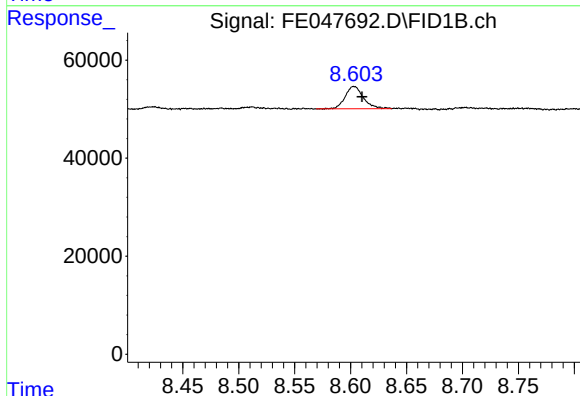


#6 n-Tetradecane (C14)

R.T.: 8.603 min
Delta R.T.: -0.007 min
Response: 51529
Conc: 0.32 ug/ml

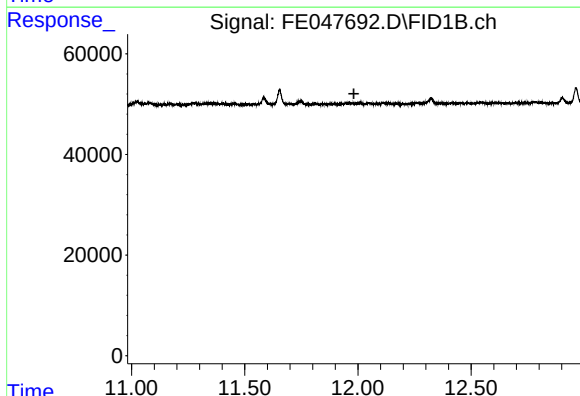

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.982 min
Response: 0
Conc: N.D.

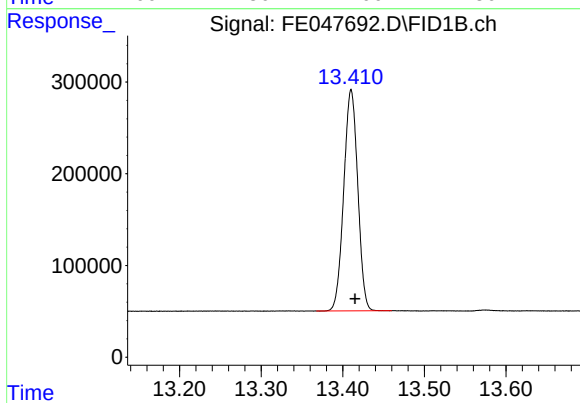

#12 1-chlorooctadecane (SURR)

R.T.: 13.410 min
Delta R.T.: -0.005 min
Response: 2875177
Conc: 21.38 ug/ml