

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041919\
 Data File : FE029922.D
 Signal(s) : FID1B.CH
 Acq On : 19 Apr 2019 13:34
 Operator : AJ\SJ
 Sample : K2475-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 20 00:00:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
 Quant Title :
 QLast Update : Wed Apr 10 08:20:21 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.644	2739602	13.504 ug/ml
Target Compounds			
3) N-DODECANE	6.399	900480	4.020 ug/ml
4) N-TETRADECANE	8.175	619458	2.682 ug/ml
10) N-TETRACOSANE	14.846	879492	3.790 ug/ml
11) N-HEXACOSANE	15.867	401778	1.742 ug/ml
12) N-OCTACOSANE	16.819	365550	1.588 ug/ml
13) N-TRIACONTANE	17.689	710125	3.089 ug/ml
14) N-DOTRIACONTANE	18.542	179450	0.807 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041919\
Data File : FE029922.D
Signal(s) : FID1B.CH
Acq On : 19 Apr 2019 13:34
Operator : AJ\SJ
Sample : K2475-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 20 00:00:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
Quant Title :
QLast Update : Wed Apr 10 08:20:21 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

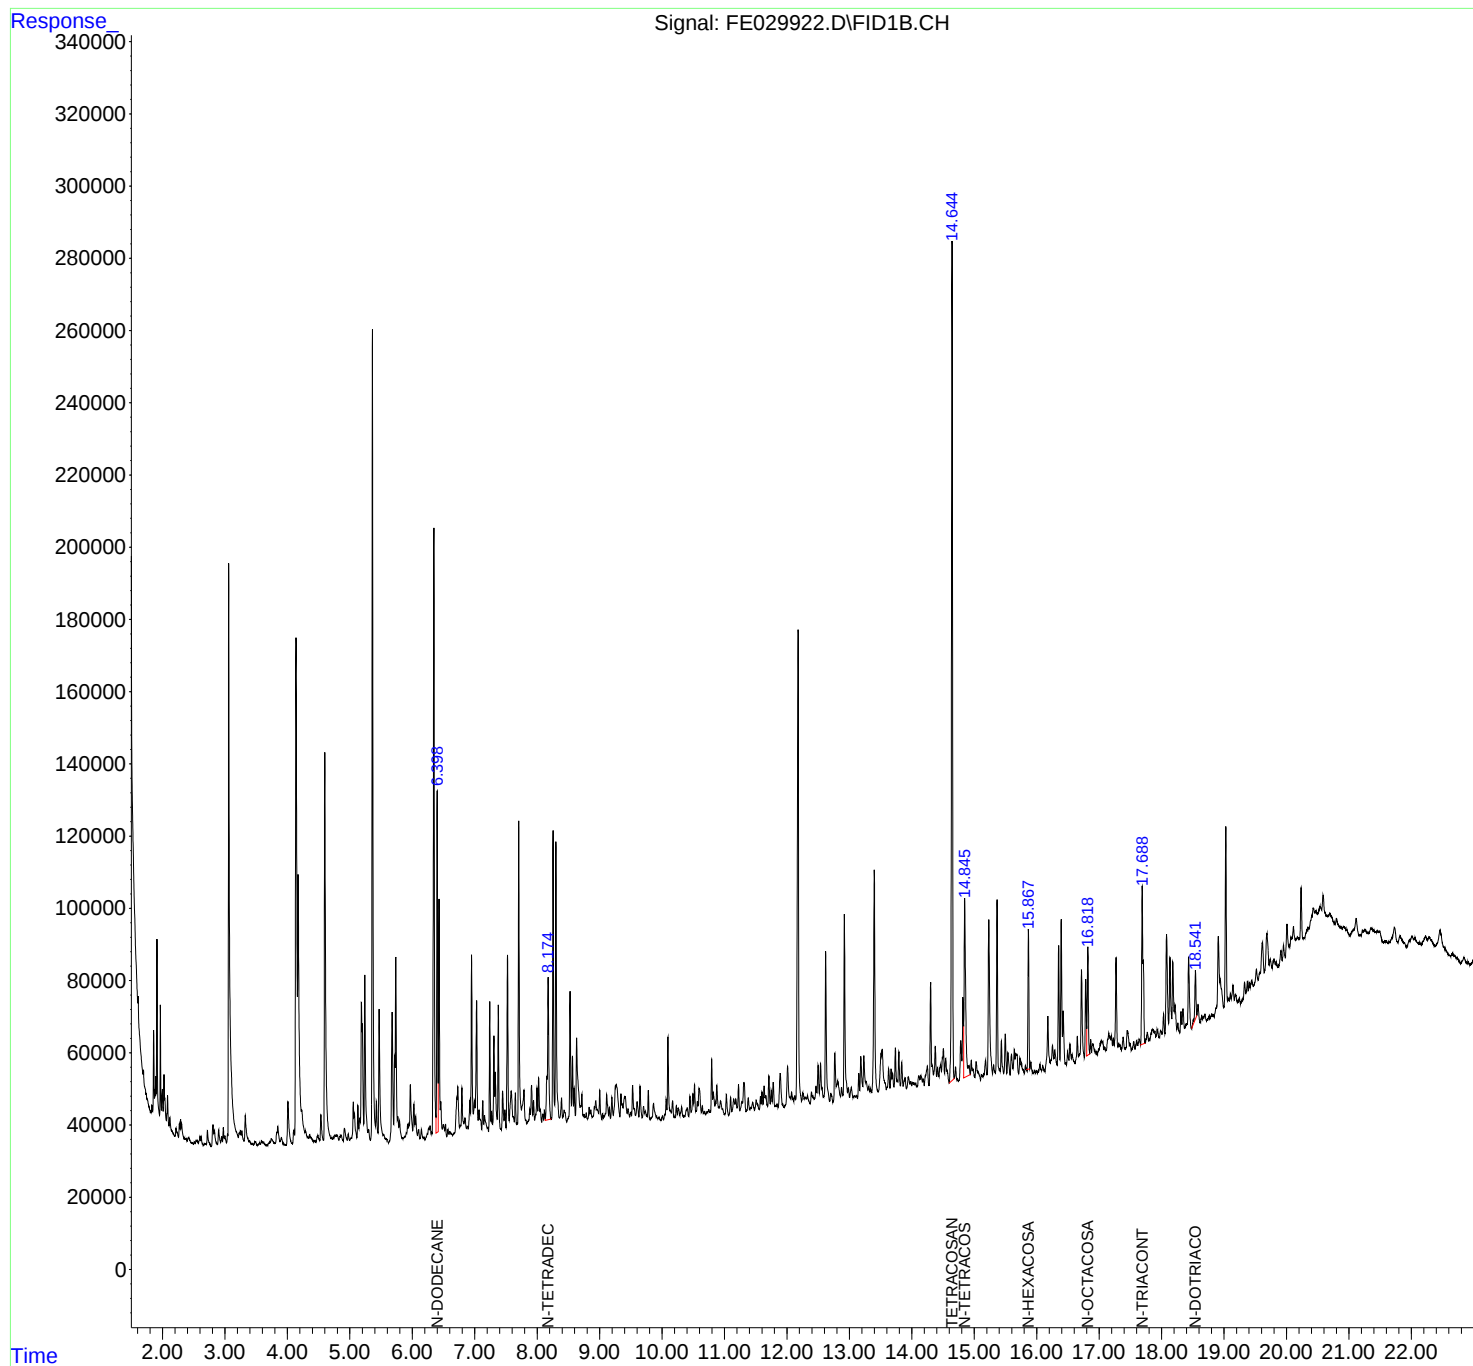

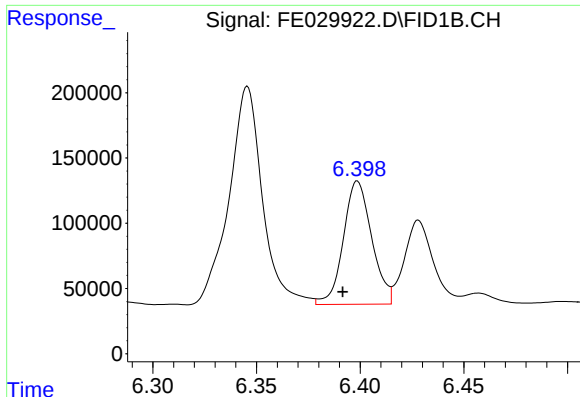


#3 N-DODECANE

R.T.: 6.399 min
Delta R.T.: 0.007 min
Response: 900480
Conc: 4.02 ug/ml

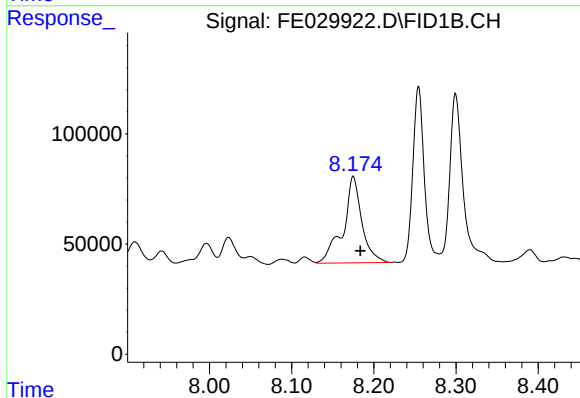


#4 N-TETRADECANE

R.T.: 8.175 min
Delta R.T.: -0.008 min
Response: 619458
Conc: 2.68 ug/ml

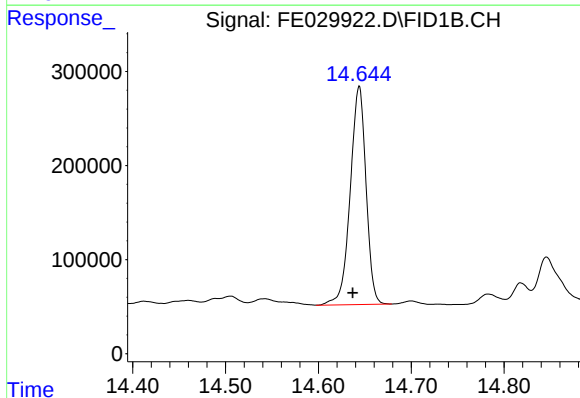


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.644 min
Delta R.T.: 0.007 min
Response: 2739602
Conc: 13.50 ug/ml

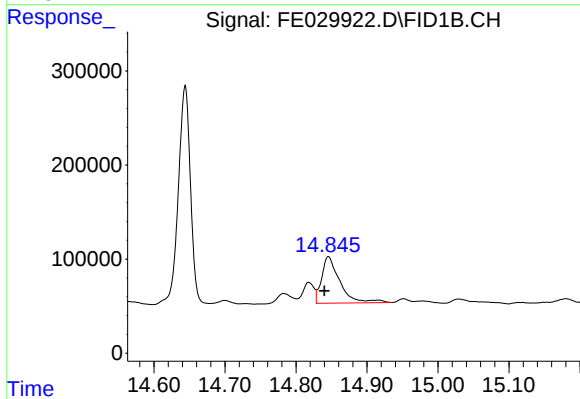


#10 N-TETRACOSANE

R.T.: 14.846 min
Delta R.T.: 0.006 min
Response: 879492
Conc: 3.79 ug/ml

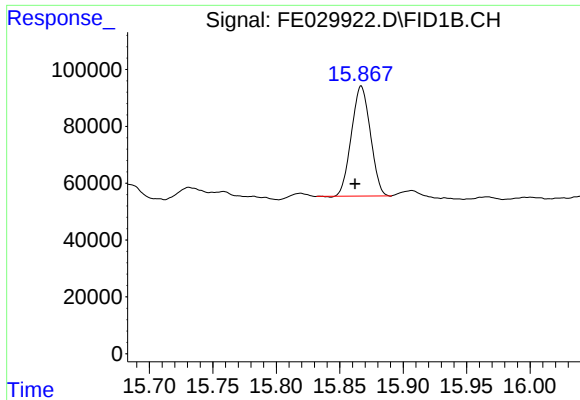


#11 N-HEXACOSANE

R.T.: 15.867 min
Delta R.T.: 0.005 min
Response: 401778
Conc: 1.74 ug/ml

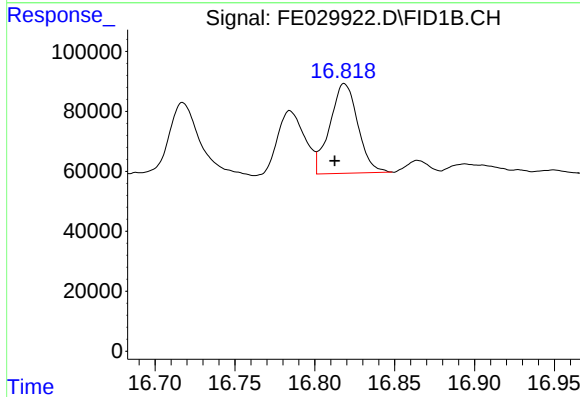


#12 N-OCTACOSANE

R.T.: 16.819 min
Delta R.T.: 0.006 min
Response: 365550
Conc: 1.59 ug/ml

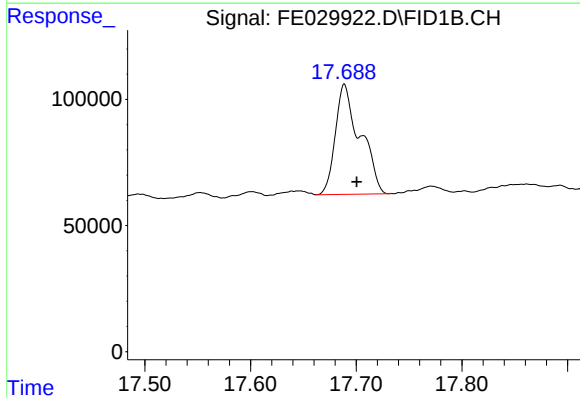

#13 N-TRIACONTANE

R.T.: 17.689 min
Delta R.T.: -0.012 min
Response: 710125
Conc: 3.09 ug/ml

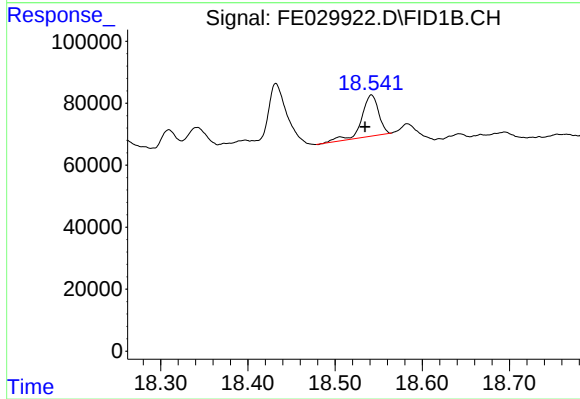

#14 N-DOTRIACONTANE

R.T.: 18.542 min
Delta R.T.: 0.007 min
Response: 179450
Conc: 0.81 ug/ml