

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041923AL\
 Data File : FE041419.D
 Signal(s) : FID1B.ch
 Acq On : 19 Apr 2023 08:30
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 20 01:57:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 25 06:32:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	15.110f	127387	0.787 ug/ml
17) T n-Tricontane (C30)	17.996	9836	0.064 ug/ml
19) T n-Tetratriacontane (C34)	19.620	15120	0.098 ug/ml
20) T n-Hexatriacontane (C36)	20.420	22930	0.151 ug/ml
21) T n-Octatriacontane (C38)	21.157	41122	0.263 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041923AL\
Data File : FE041419.D
Signal(s) : FID1B.ch
Acq On : 19 Apr 2023 08:30
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 20 01:57:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

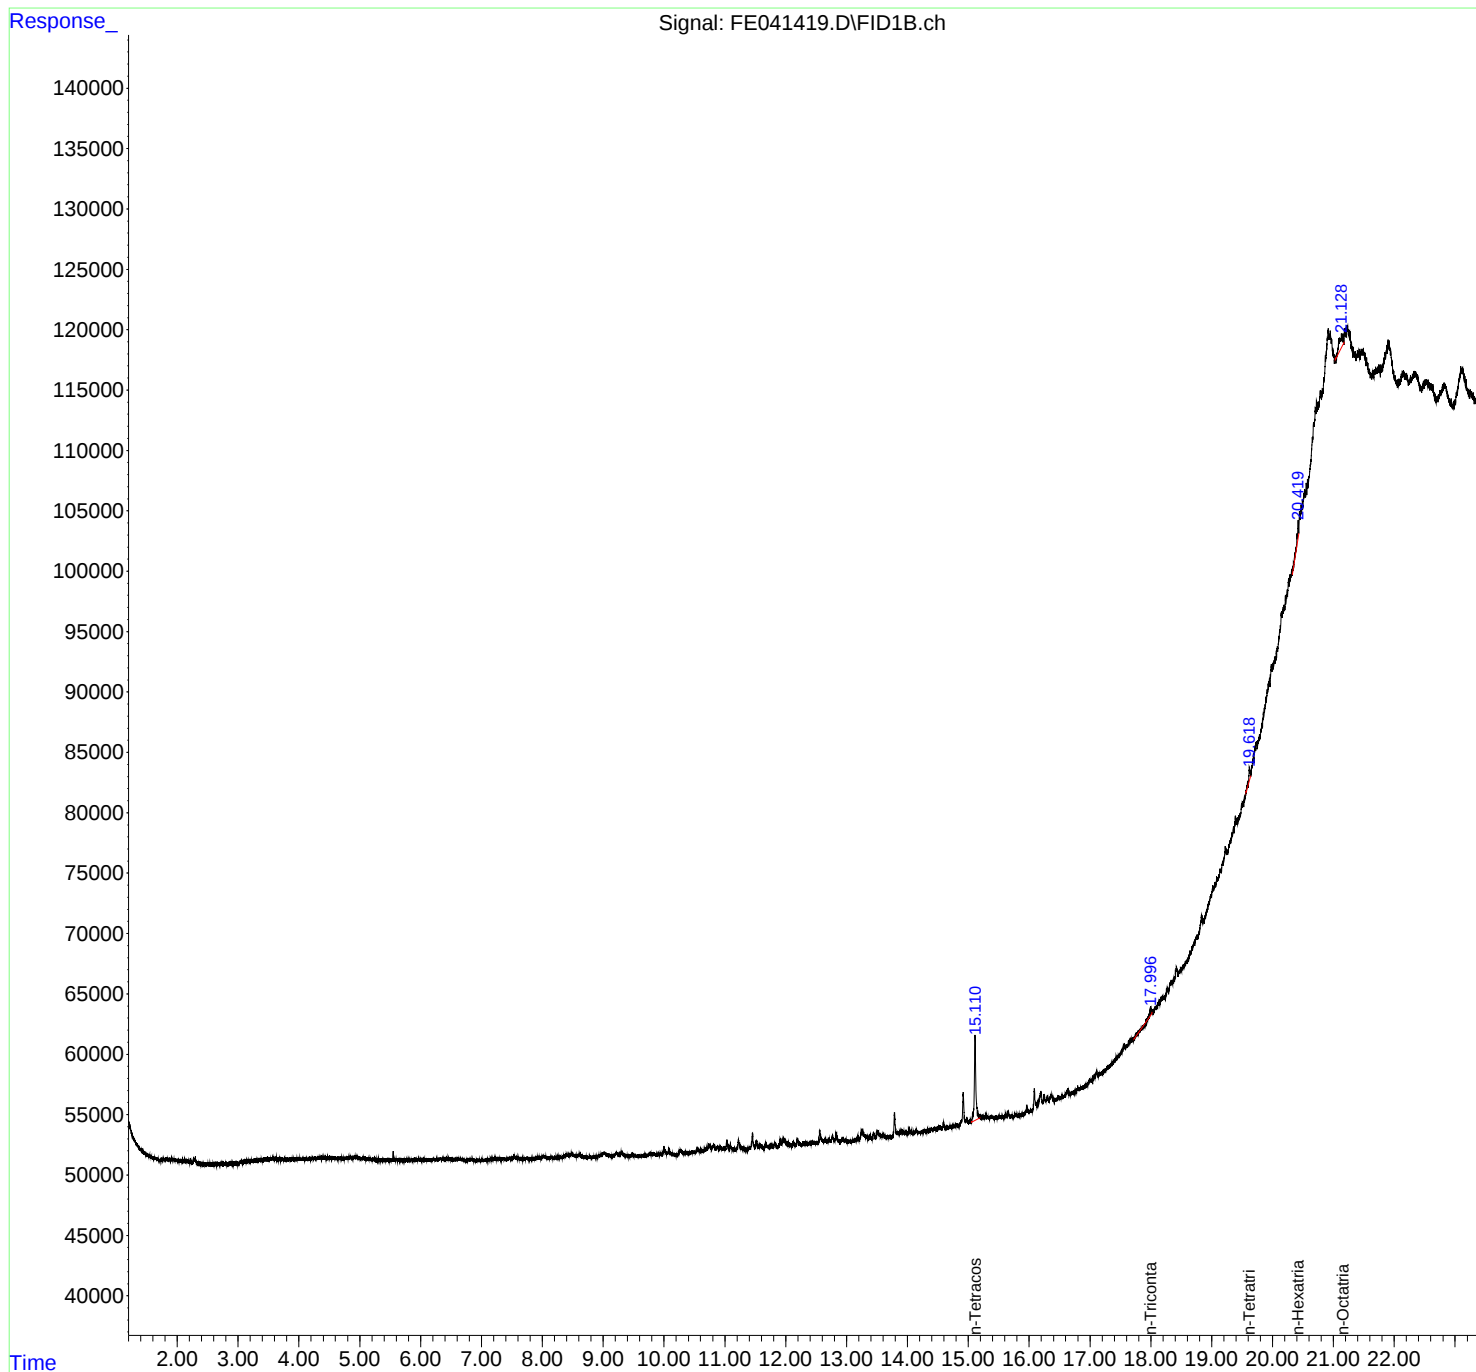


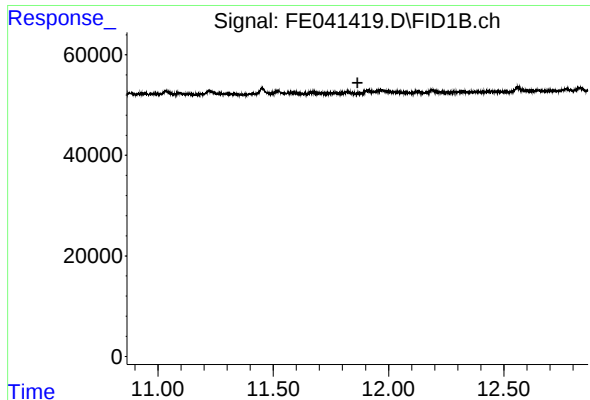

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

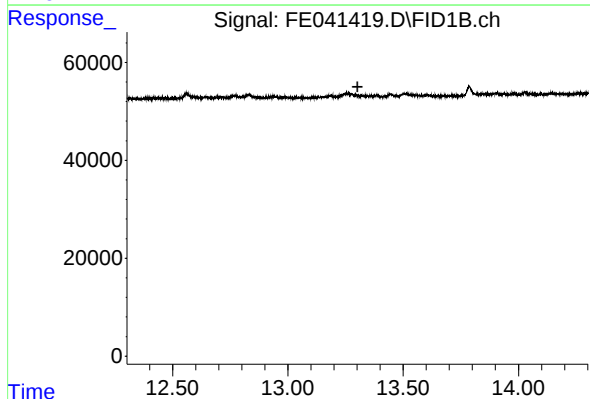


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

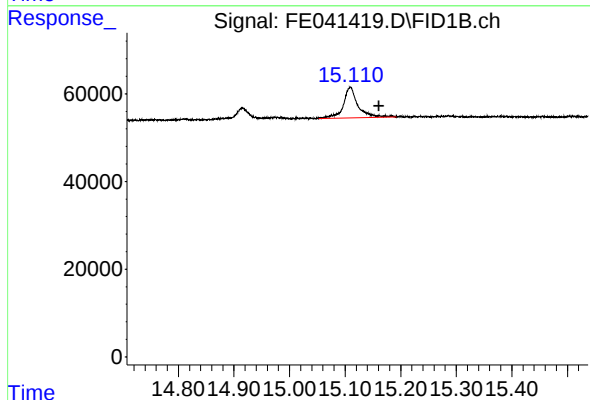


#14 n-Tetracosane (C24)

R.T.: 15.110 min
Delta R.T.: -0.051 min
Response: 127387
Conc: 0.79 ug/ml

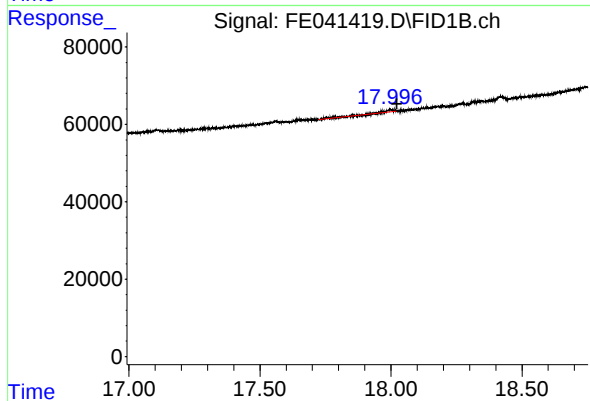

#17 n-Tricontane (C30)


R.T.: 17.996 min
Delta R.T.: -0.026 min
Response: 9836
Conc: 0.06 ug/ml

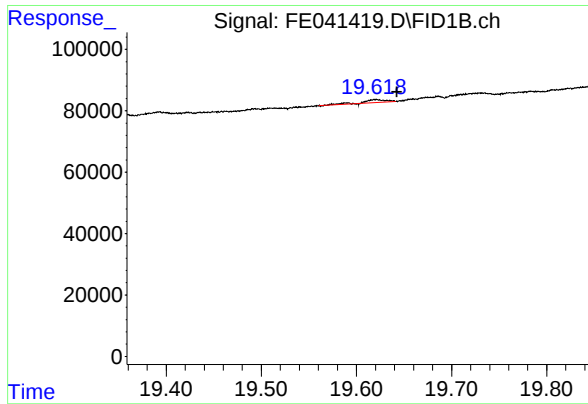

#19 n-Tetratriacontane (C34)


R.T.: 19.620 min
Delta R.T.: -0.022 min
Response: 15120
Conc: 0.10 ug/ml

Instrument :
FID_E
ClientSampleId :

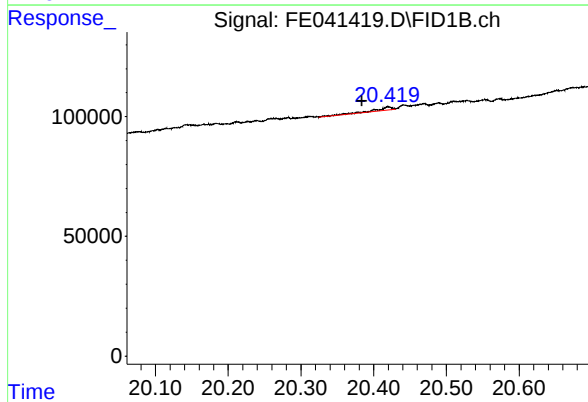

#20 n-Hexatriacontane (C36)

R.T.: 20.420 min
Delta R.T.: 0.036 min
Response: 22930
Conc: 0.15 ug/ml

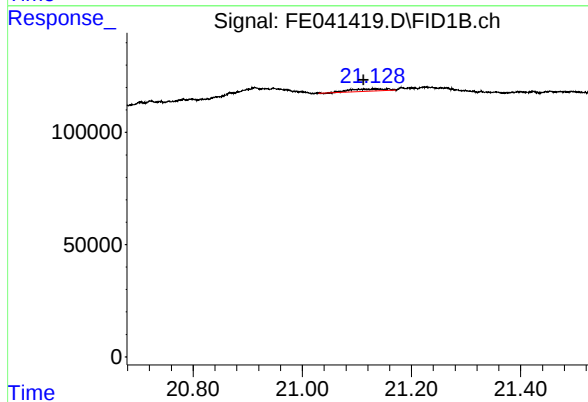

#21 n-Octatriacontane (C38)

R.T.: 21.157 min
Delta R.T.: 0.045 min
Response: 41122
Conc: 0.26 ug/ml