

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041923AL\
Data File : FE041426.D
Signal(s) : FID1B.ch
Acq On : 19 Apr 2023 13:36
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 20 01:58:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	n-Tetracosane (C24)	15.107f	118645	0.733 ug/ml
17) T	n-Tricontane (C30)	17.992	15047	0.098 ug/ml
18) T	n-Dotriacontane (C32)	18.831	27463	0.176 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE041923AL\
Data File : FE041426.D
Signal(s) : FID1B.ch
Acq On : 19 Apr 2023 13:36
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 20 01:58:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 032523.M
Quant Title : GC Extractables
QLast Update : Sat Mar 25 06:32:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

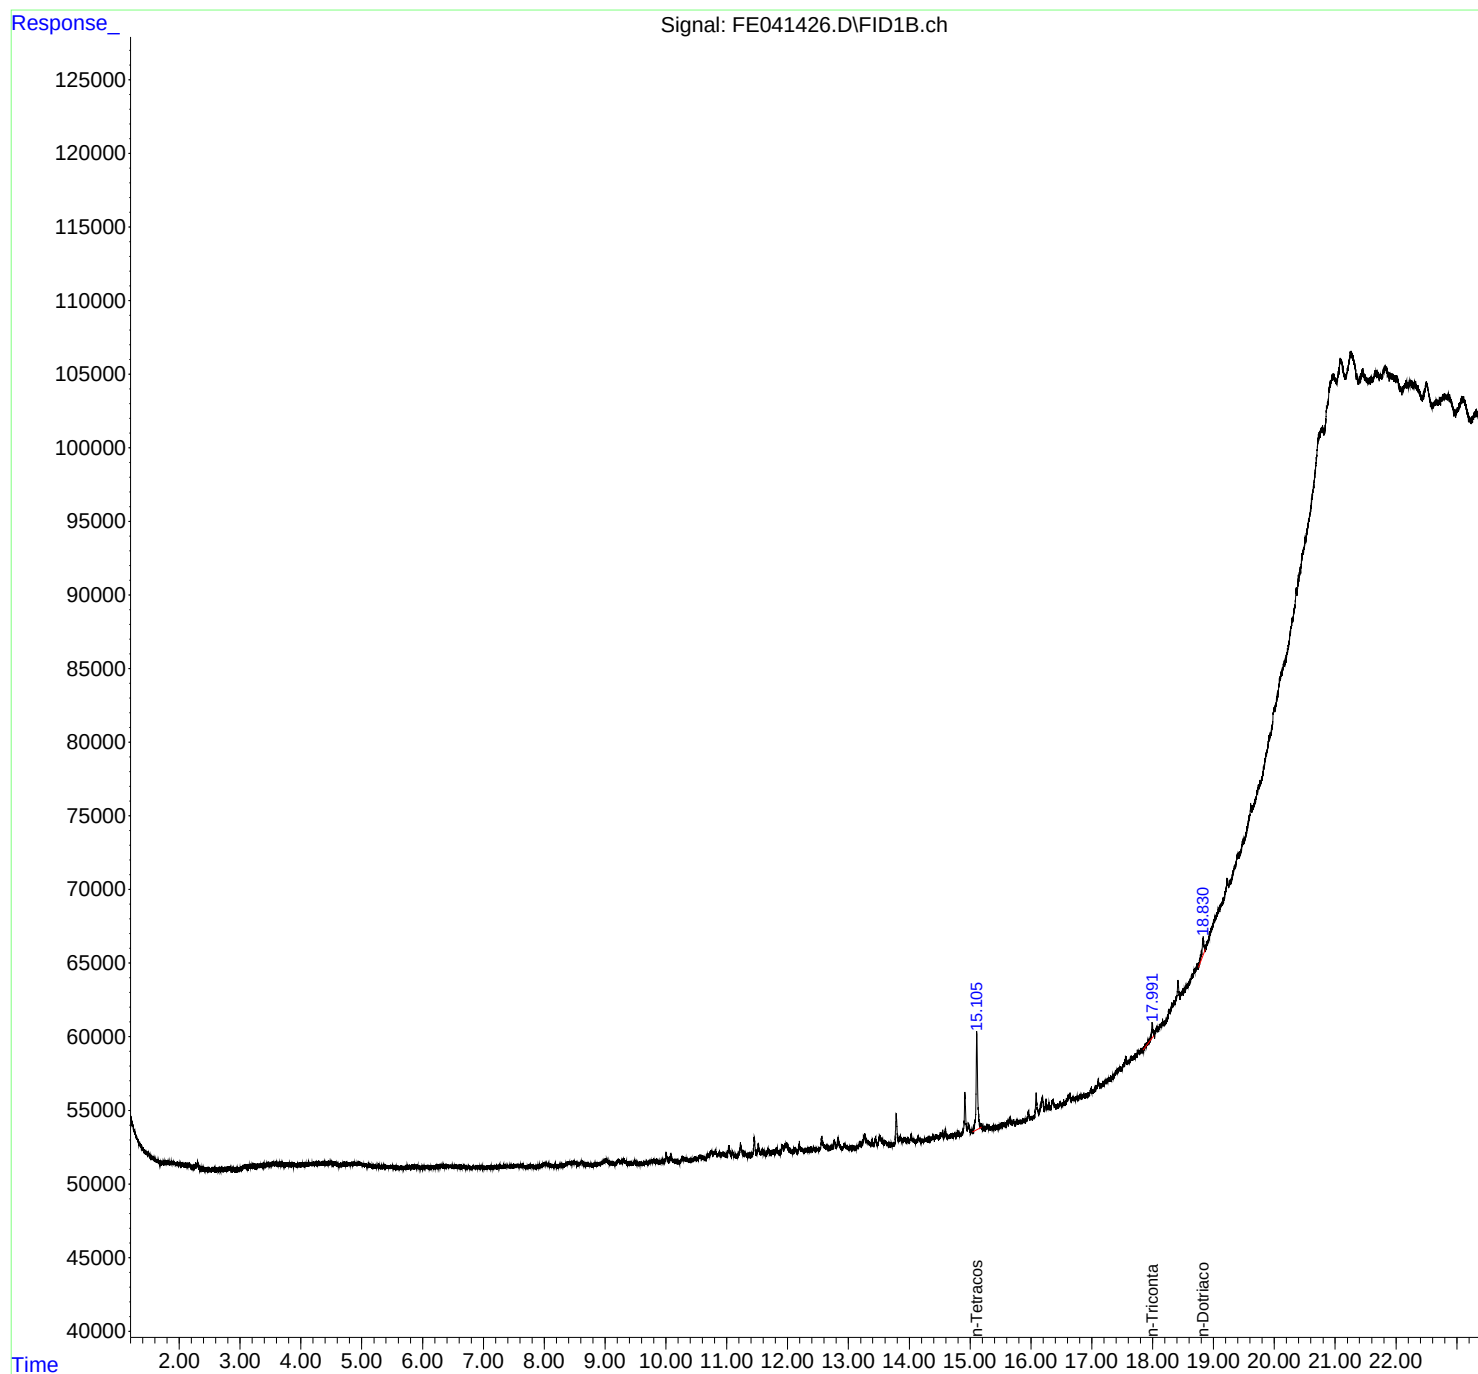


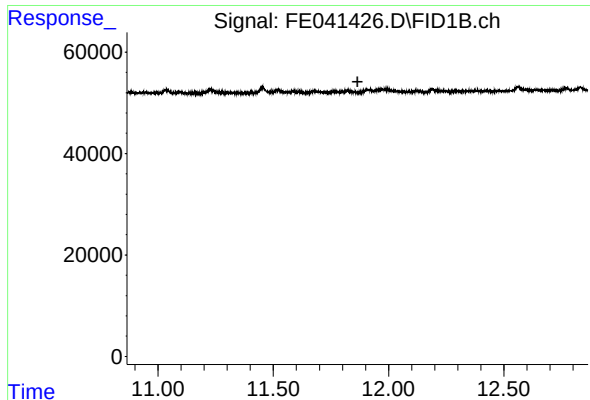

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.865 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

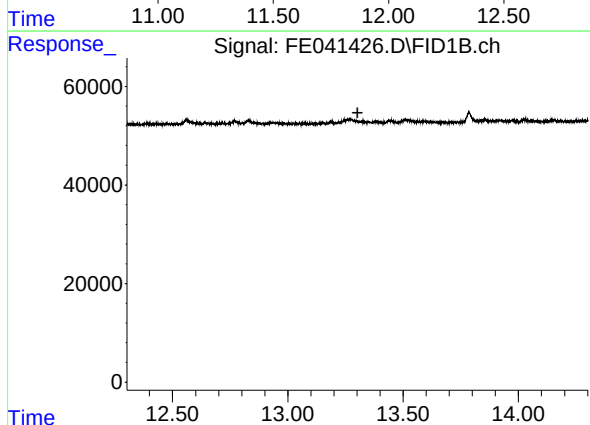


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.302 min
Response: 0
Conc: N.D.

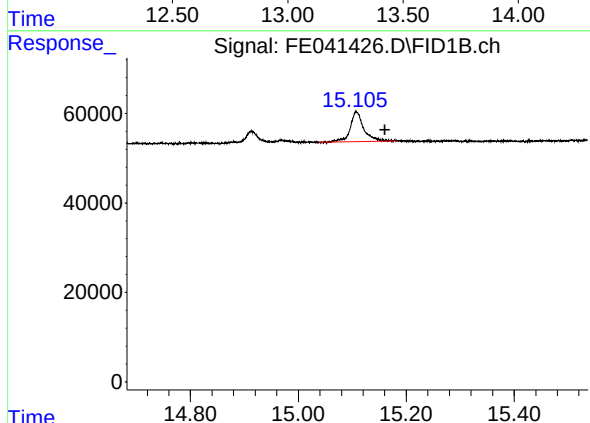


#14 n-Tetracosane (C24)

R.T.: 15.107 min
Delta R.T.: -0.053 min
Response: 118645
Conc: 0.73 ug/ml

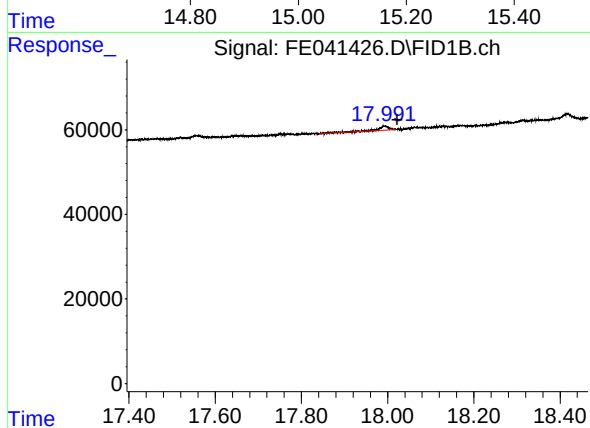

#17 n-Tricontane (C30)

R.T.: 17.992 min
Delta R.T.: -0.030 min
Response: 15047
Conc: 0.10 ug/ml

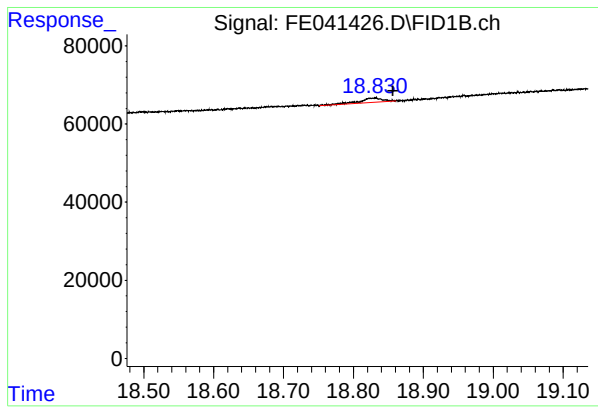

#18 n-Dotriacontane (C32)

R.T.: 18.831 min
Delta R.T.: -0.026 min
Response: 27463
Conc: 0.18 ug/ml

Instrument :

FID_E

ClientSampleId :