

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042021\
Data File : FE033615.D
Signal(s) : FID1B.CH
Acq On : 20 Apr 2021 16:33
Operator : DD\AJ
Sample : M2090-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SEDGWICK-COMP-3

Manual Integrations
APPROVED

Ankita
4/21/2021 1:04:02 PM

Integration File: autoint1.e
Quant Time: Apr 21 01:59:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040521.M
Quant Title :
QLast Update : Tue Apr 06 01:29:58 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.774	5064021	12.885 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042021\
Data File : FE033615.D
Signal(s) : FID1B.CH
Acq On : 20 Apr 2021 16:33
Operator : DD\AJ
Sample : M2090-13
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
SEDGWICK-COMP-3


Manual Integrations
APPROVED

Ankita
4/21/2021 1:04:02 PM

Integration File: autoint1.e
Quant Time: Apr 21 01:59:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040521.M
Quant Title :
QLast Update : Tue Apr 06 01:29:58 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

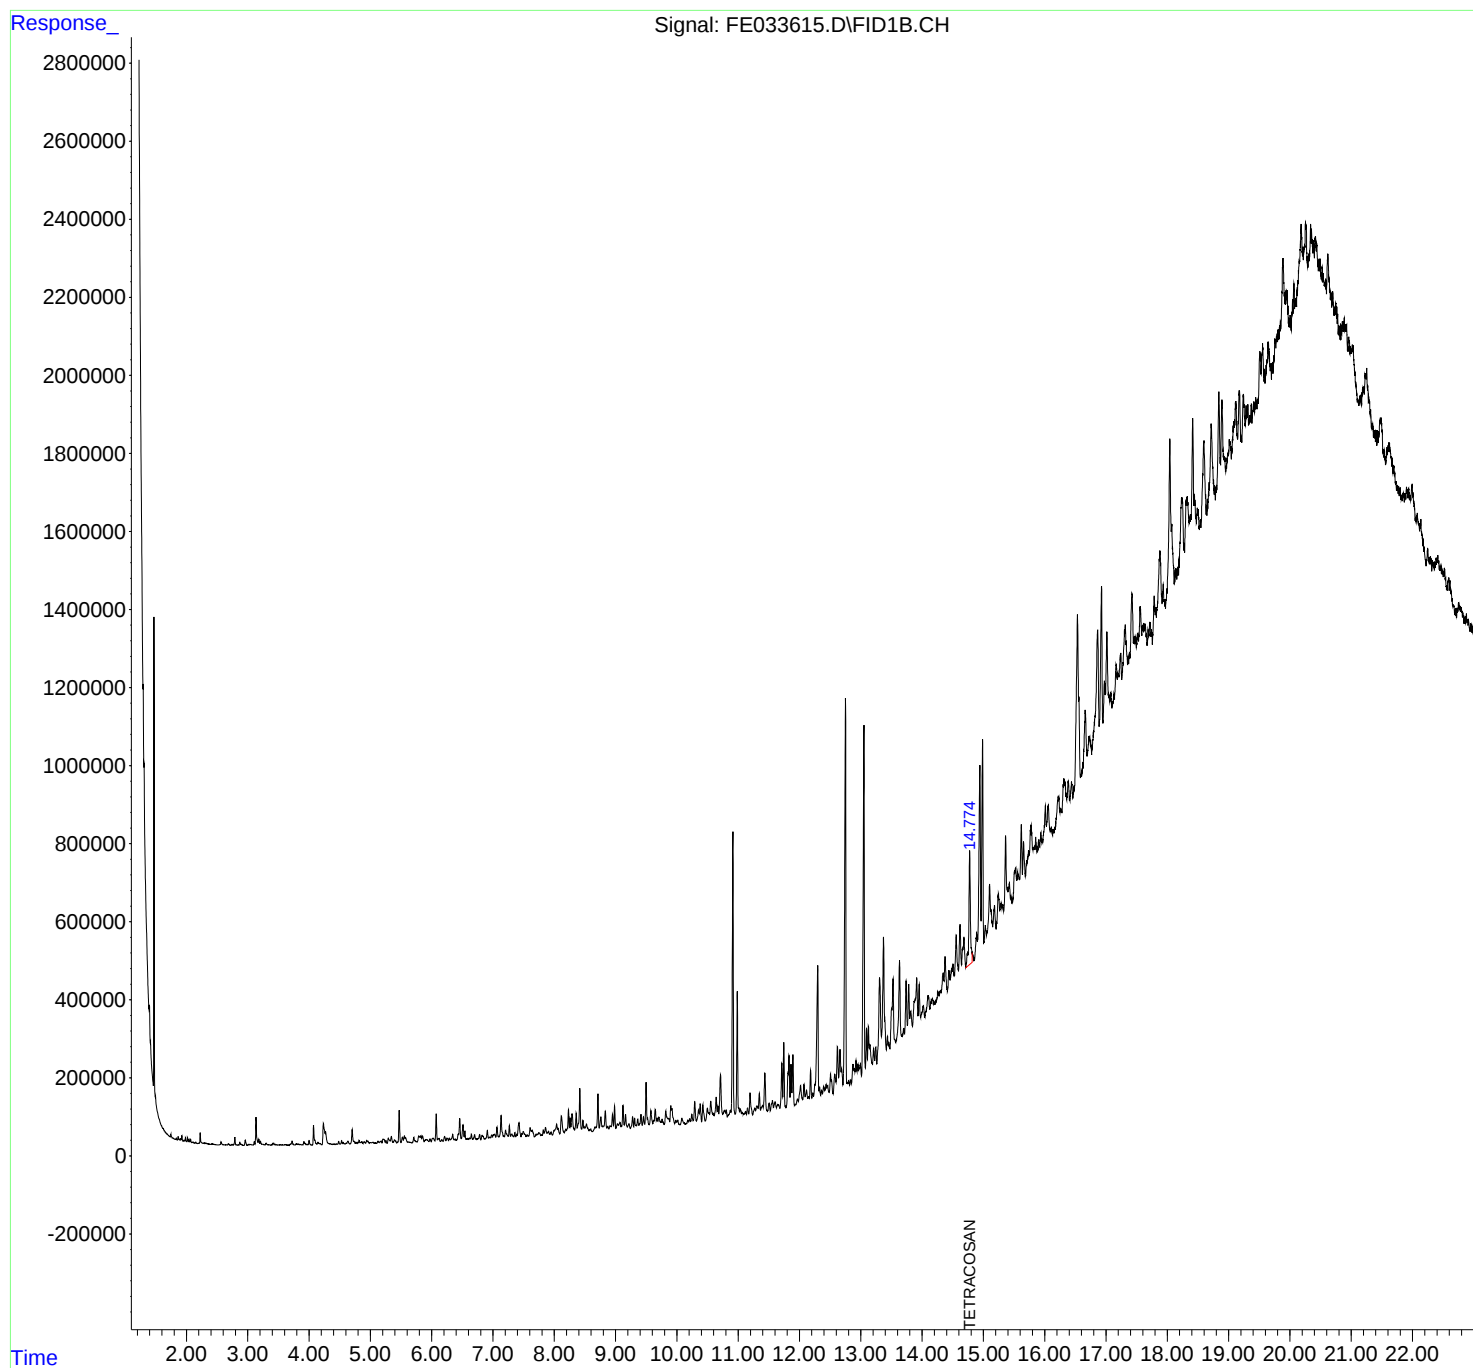

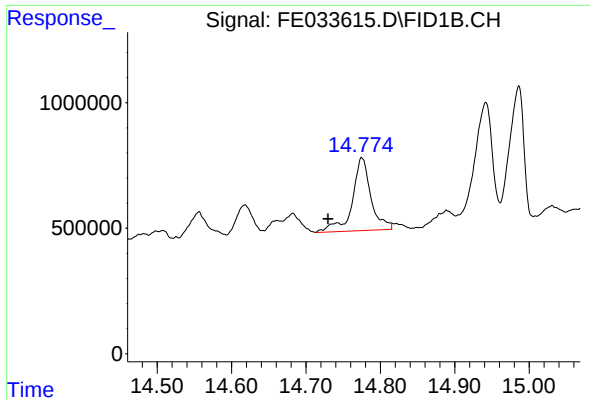

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.774 min
Delta R.T.: 0.044 min
Response: 5064021
Conc: 12.89 ug/ml m

Instrument :
FID_E
ClientSampleId :
SEDGWICK-COMP-3

Manual Integrations
APPROVED

Ankita
4/21/2021 1:04:02 PM