

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042021\
 Data File : FE033621.D
 Signal(s) : FID1B.CH
 Acq On : 20 Apr 2021 21:09
 Operator : DD\AJ
 Sample : M2090-08 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 SEDGWICK-COMP-2

Manual Integrations
 APPROVED

Ankita
 4/21/2021 1:04:09 PM

Integration File: autoint1.e
 Quant Time: Apr 21 02:01:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040521.M
 Quant Title :
 QLast Update : Tue Apr 06 01:29:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.751	618831	1.575 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042021\
Data File : FE033621.D
Signal(s) : FID1B.CH
Acq On : 20 Apr 2021 21:09
Operator : DD\AJ
Sample : M2090-08 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
SEDGWICK-COMP-2


Manual Integrations
APPROVED

Ankita
4/21/2021 1:04:09 PM

Integration File: autoint1.e
Quant Time: Apr 21 02:01:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040521.M
Quant Title :
QLast Update : Tue Apr 06 01:29:58 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

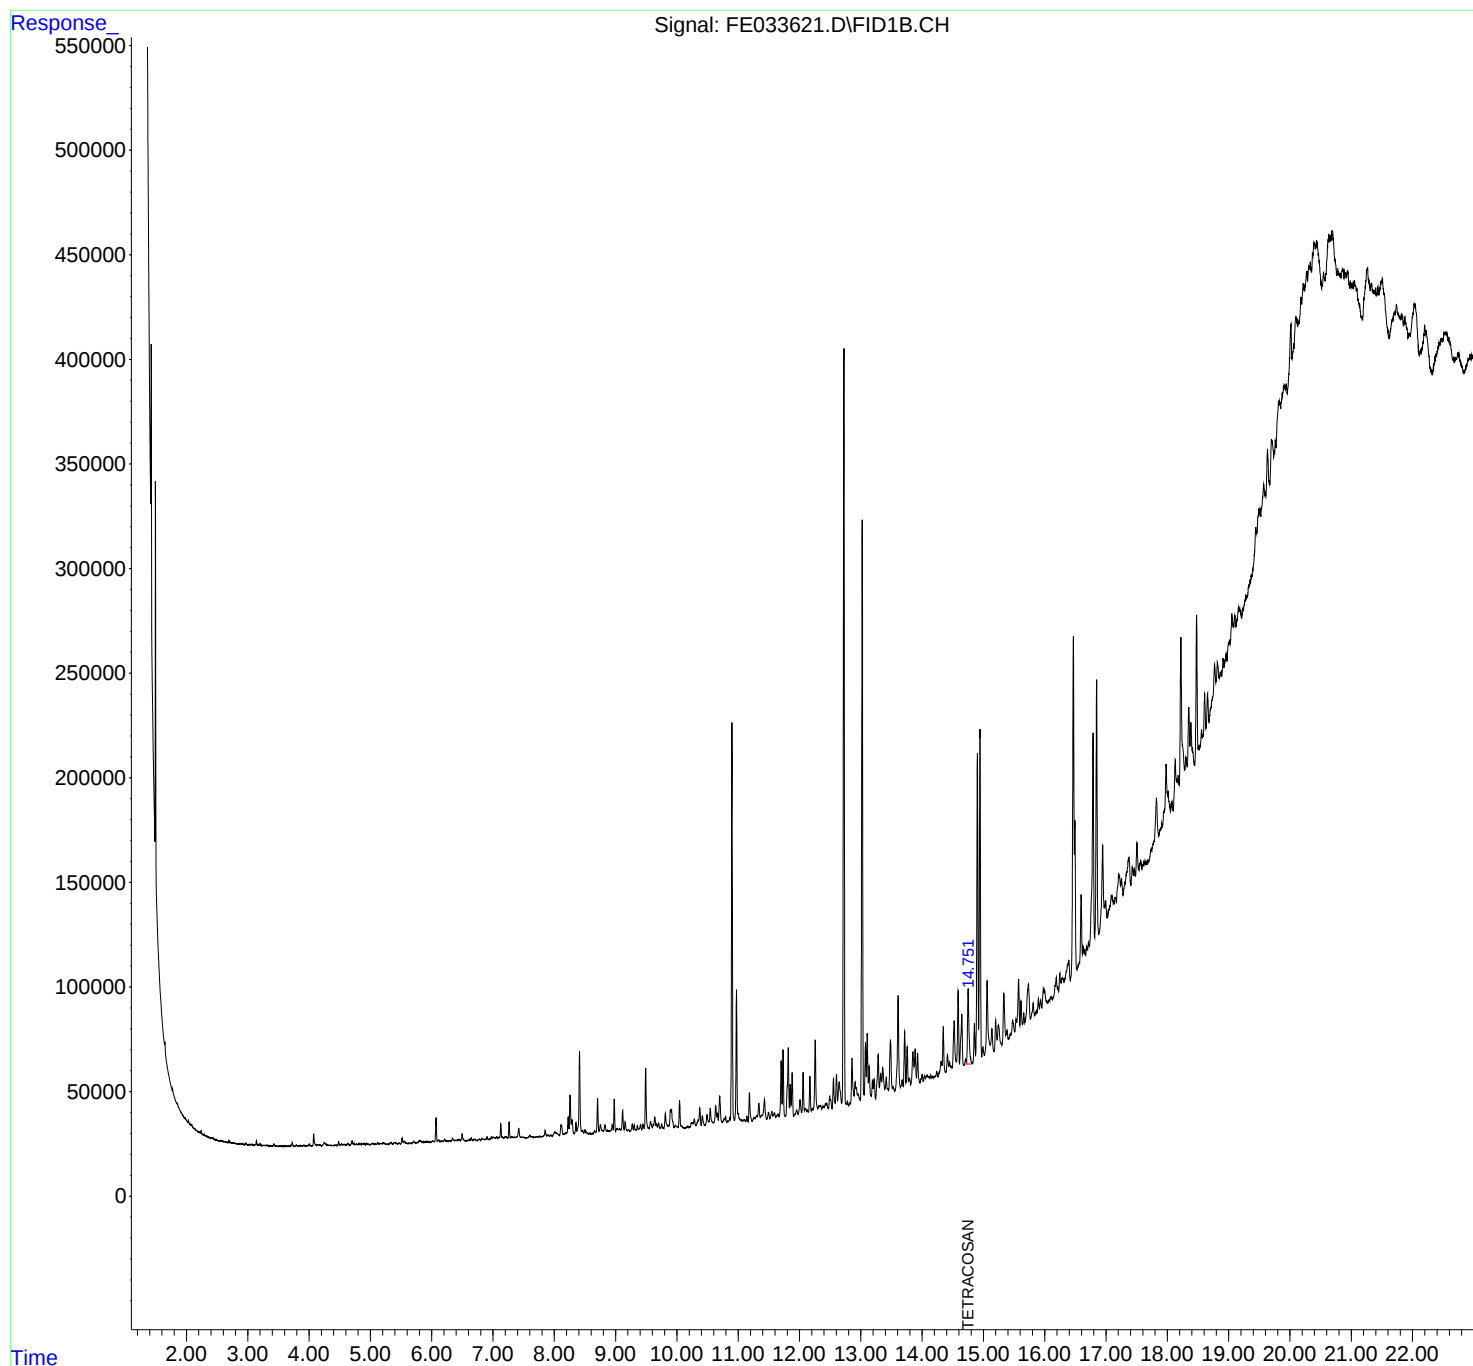

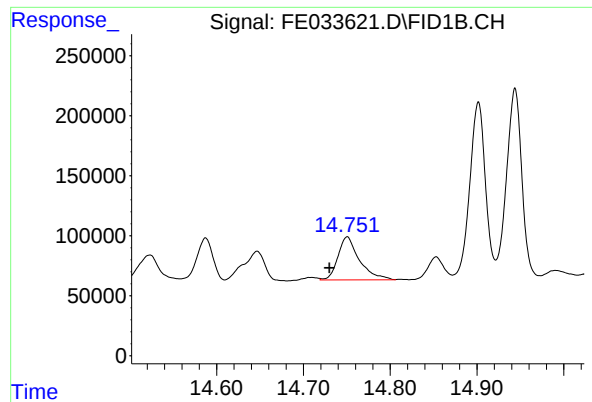

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.751 min
Delta R.T.: 0.021 min
Response: 618831
Conc: 1.57 ug/ml m

Instrument :
FID_E
ClientSampleId :
SEDGWICK-COMP-2

Manual Integrations
APPROVED

Ankita
4/21/2021 1:04:09 PM