

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042120\
 Data File : FE031798.D
 Signal(s) : FID1B.CH
 Acq On : 22 Apr 2020 7:51
 Operator : DD\AJ
 Sample : L2332-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 22 08:52:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
 Quant Title :
 QLast Update : Tue Apr 07 15:06:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.386	8032242	22.055 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.005f	2968690	7.490 ug/ml
8)	N-DOCOSANE	13.479	473094	1.116 ug/ml
10)	N-TETRACOSANE	14.584	361612	0.864 ug/ml
11)	N-HEXACOSANE	15.605	638243	1.540 ug/ml
12)	N-OCTACOSANE	16.557	1906989	4.635 ug/ml
13)	N-TRIACONTANE	17.447	3839154	9.335 ug/ml
14)	N-DOTRIACONTANE	18.280	2711131	6.895 ug/ml
15)	N-TETRATRIACONTANE	19.065	2161616	5.838 ug/ml
16)	N-HEXATRIACONTANE	19.809	1933882	5.609 ug/ml
17)	N-OCTATRIACONTANE	20.499	4729287	15.293 ug/ml
18)	N-TETRACONTANE	21.334	300872	0.952 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042120\
Data File : FE031798.D
Signal(s) : FID1B.CH
Acq On : 22 Apr 2020 7:51
Operator : DD\AJ
Sample : L2332-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 22 08:52:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
Quant Title :
QLast Update : Tue Apr 07 15:06:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

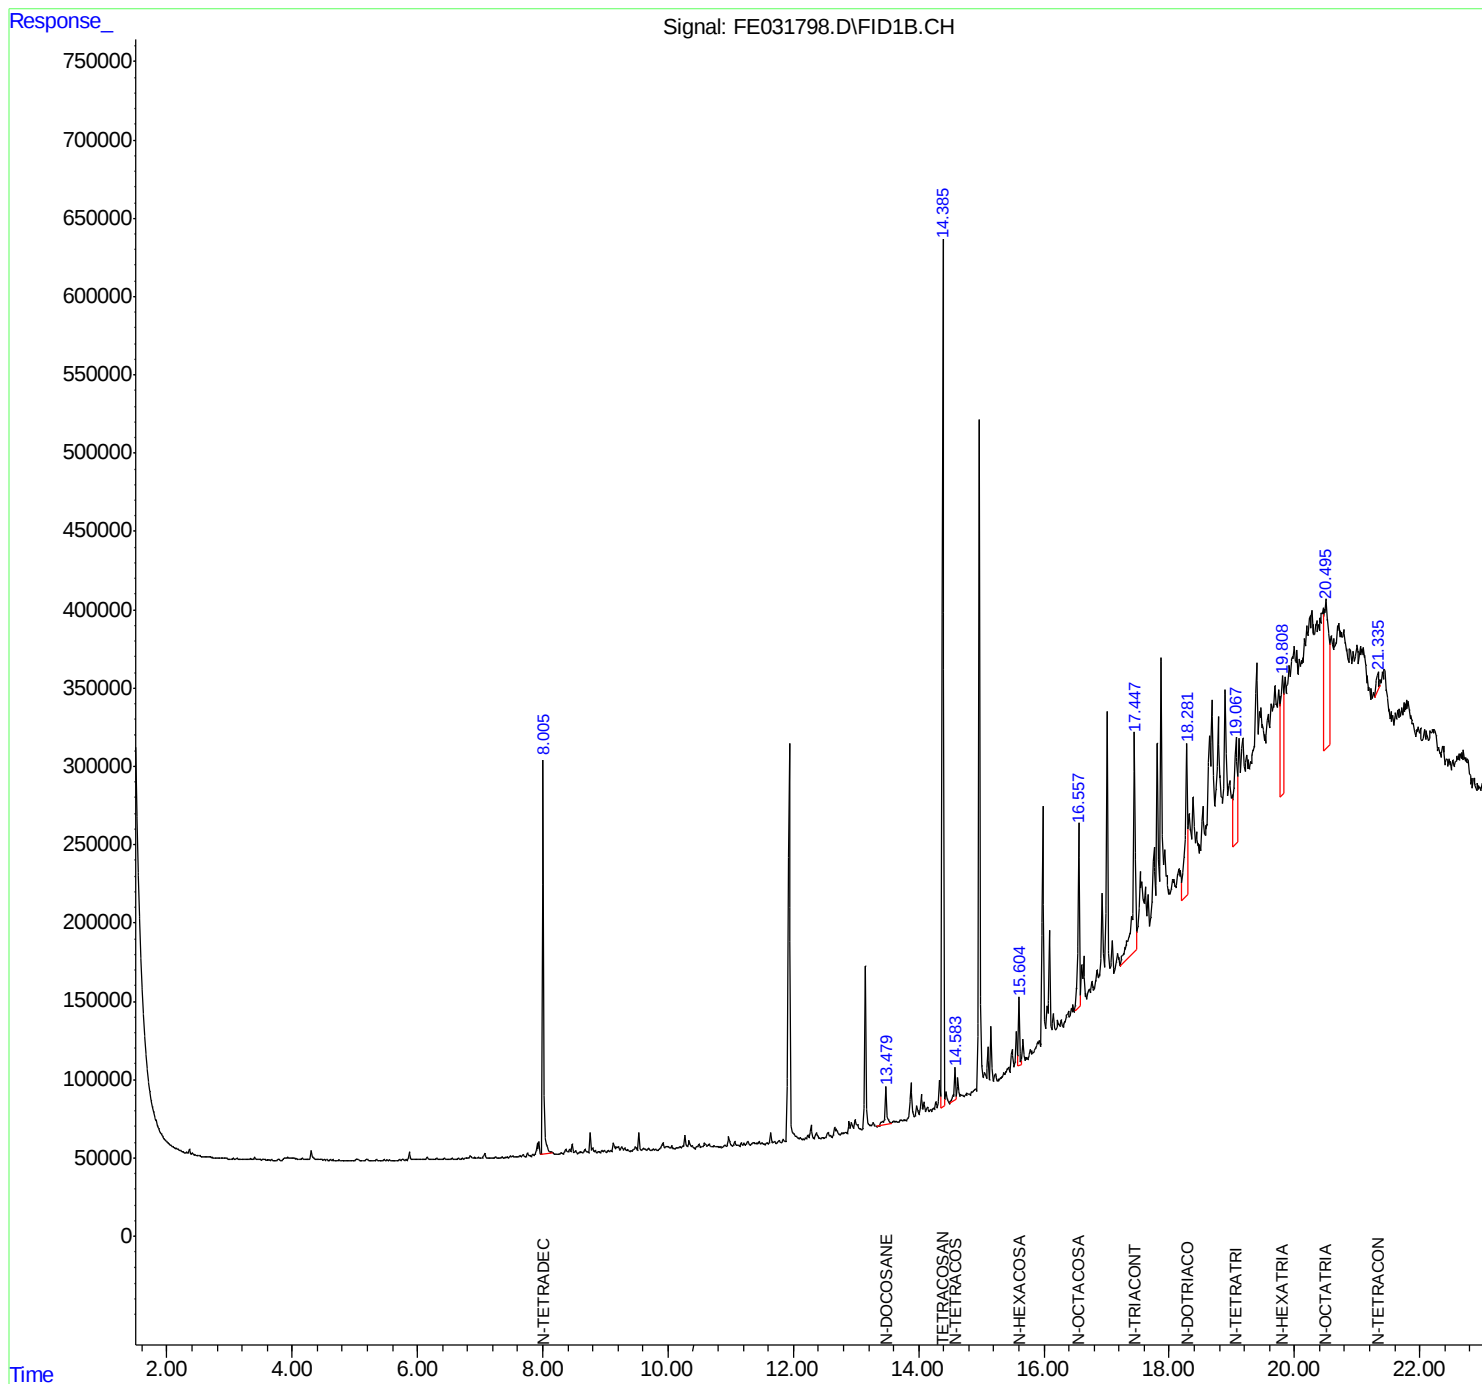

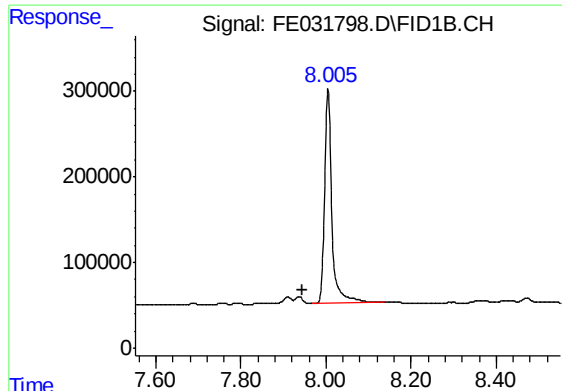


#4 N-TETRADECANE

R.T.: 8.005 min
Delta R.T.: 0.061 min
Response: 2968690
Conc: 7.49 ug/ml

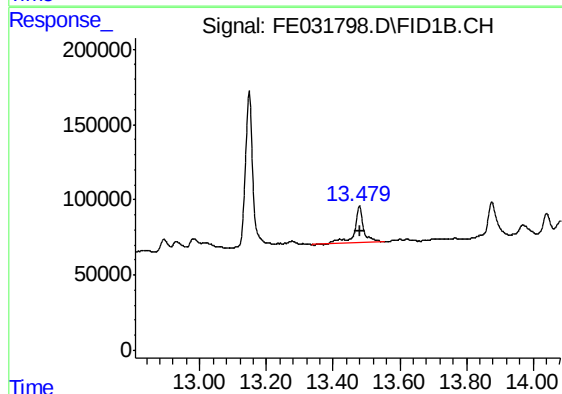


#8 N-DOCOSANE

R.T.: 13.479 min
Delta R.T.: -0.003 min
Response: 473094
Conc: 1.12 ug/ml

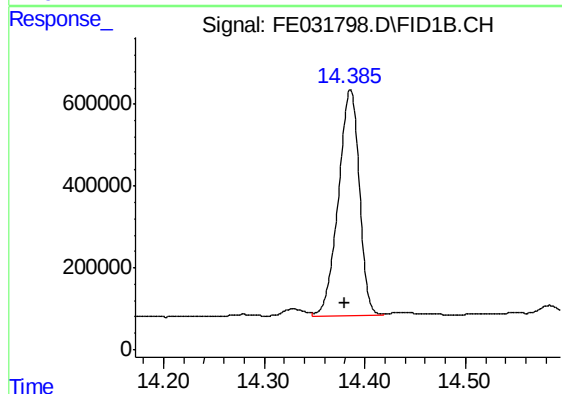


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.386 min
Delta R.T.: 0.006 min
Response: 8032242
Conc: 22.05 ug/ml

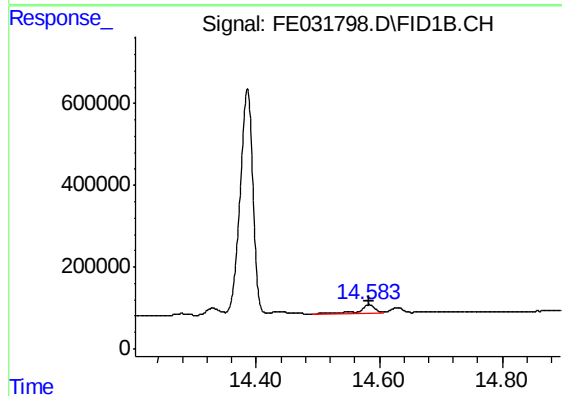


#10 N-TETRACOSANE

R.T.: 14.584 min
Delta R.T.: 0.000 min
Response: 361612
Conc: 0.86 ug/ml

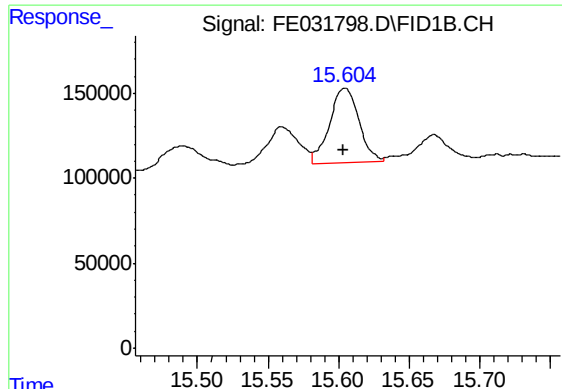


#11 N-HEXACOSANE

R.T.: 15.605 min
Delta R.T.: 0.001 min
Response: 638243
Conc: 1.54 ug/ml

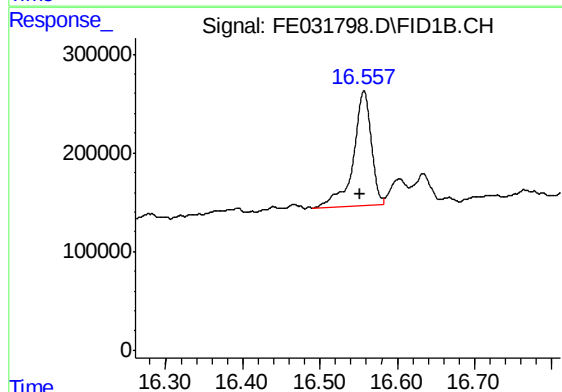


#12 N-OCTACOSANE

R.T.: 16.557 min
Delta R.T.: 0.004 min
Response: 1906989
Conc: 4.64 ug/ml

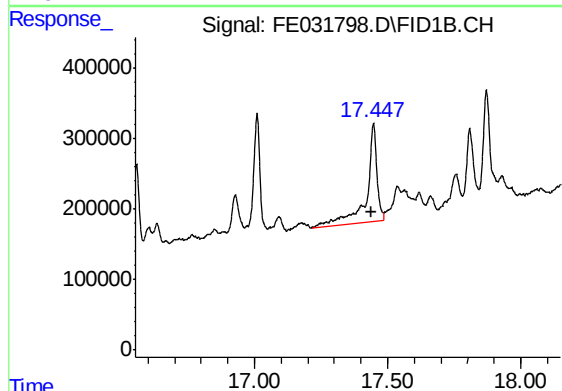


#13 N-TRIACONTANE

R.T.: 17.447 min
Delta R.T.: 0.008 min
Response: 3839154
Conc: 9.33 ug/ml

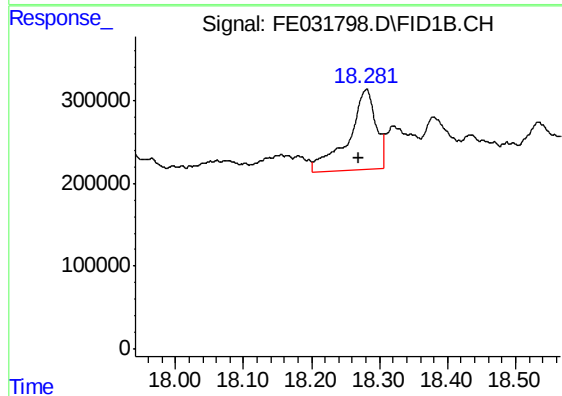


#14 N-DOTRIACONTANE

R.T.: 18.280 min
Delta R.T.: 0.011 min
Response: 2711131
Conc: 6.89 ug/ml

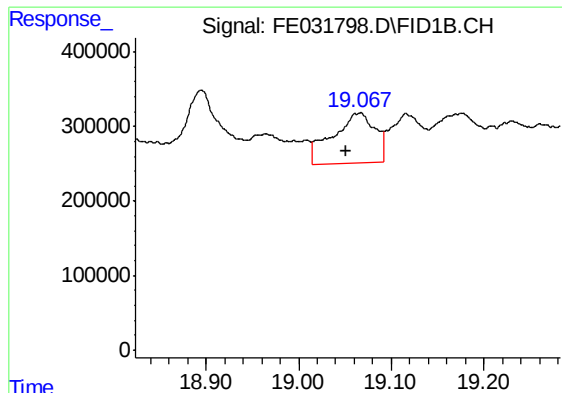


#15 N-TETRATRIACONTANE

R.T.: 19.065 min
Delta R.T.: 0.014 min
Response: 2161616
Conc: 5.84 ug/ml

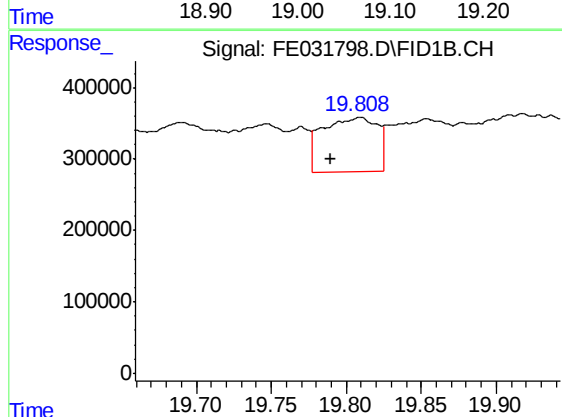


#16 N-HEXATRIACONTANE

R.T.: 19.809 min
Delta R.T.: 0.019 min
Response: 1933882
Conc: 5.61 ug/ml

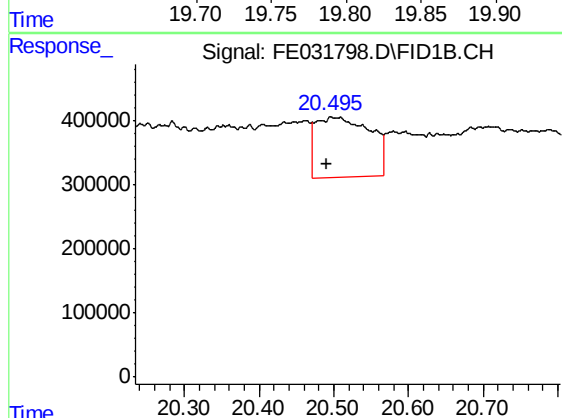

#17 N-OCTATRIACONTANE

R.T.: 20.499 min
Delta R.T.: 0.008 min
Response: 4729287
Conc: 15.29 ug/ml

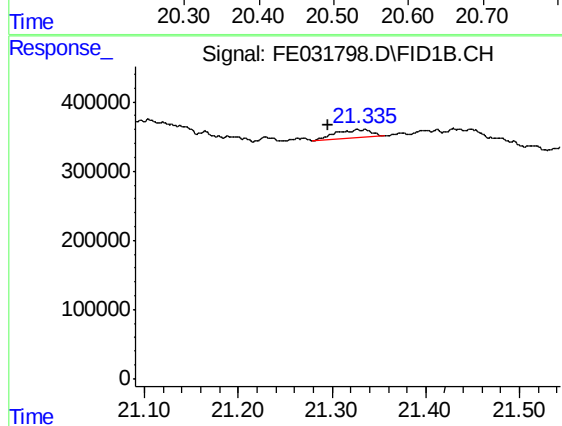

#18 N-TETRACONTANE

R.T.: 21.334 min
Delta R.T.: 0.038 min
Response: 300872
Conc: 0.95 ug/ml