

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042219\
 Data File : FE029935.D
 Signal(s) : FID1B.CH
 Acq On : 22 Apr 2019 11:35
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Apr 22 22:48:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE040919.M
 Quant Title :
 QLast Update : Wed Apr 10 07:42:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
5) N-DODECANE	6.385	4333020	21.123 ug/ml
11) N-OCTACOSANE	16.818	4063389	19.997 ug/ml
12) N-DOTRIACONTANE	18.534	130941	0.663 ug/ml
14) N-HEXATRIACONTANE	20.060	53113	0.292 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042219\
Data File : FE029935.D
Signal(s) : FID1B.CH
Acq On : 22 Apr 2019 11:35
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 22 22:48:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE040919.M
Quant Title :
QLast Update : Wed Apr 10 07:42:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

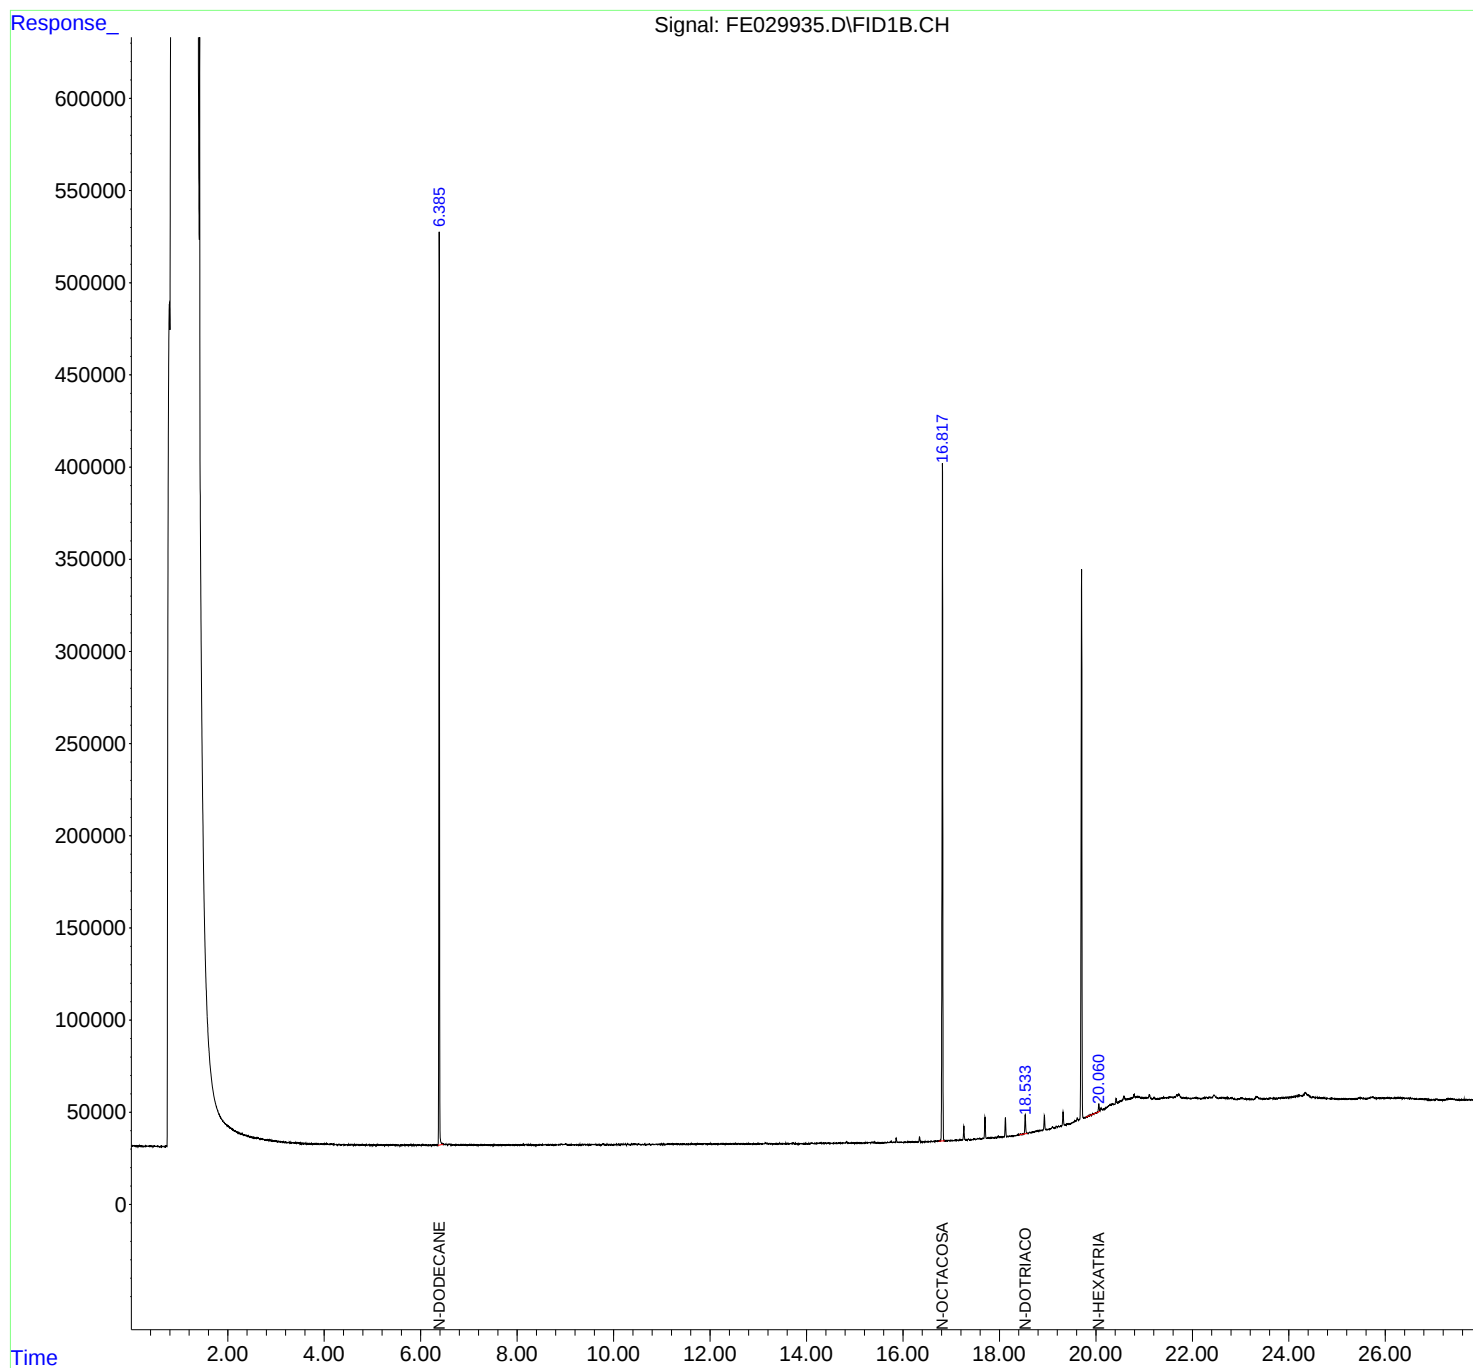


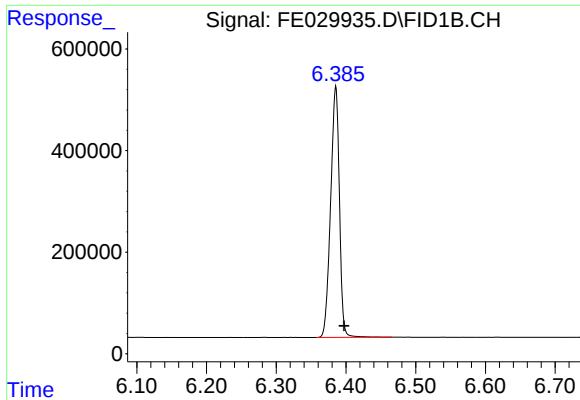

#5 N-DODECANE


R.T.: 6.385 min
Delta R.T.: -0.012 min
Response: 4333020
Conc: 21.12 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

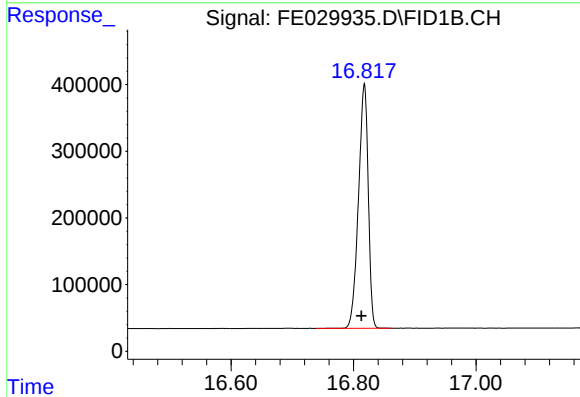


#11 N-OCTACOSANE

R.T.: 16.818 min
Delta R.T.: 0.005 min
Response: 4063389
Conc: 20.00 ug/ml

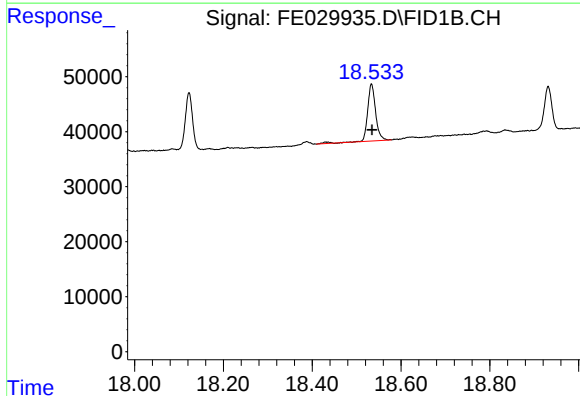


#12 N-DOTRIACONTANE

R.T.: 18.534 min
Delta R.T.: -0.001 min
Response: 130941
Conc: 0.66 ug/ml

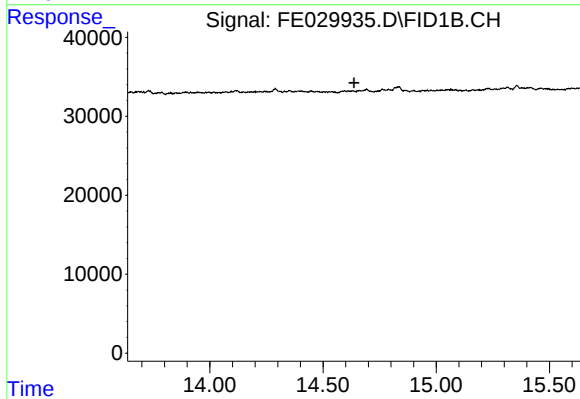

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.637 min
Response: 0
Conc: N.D.

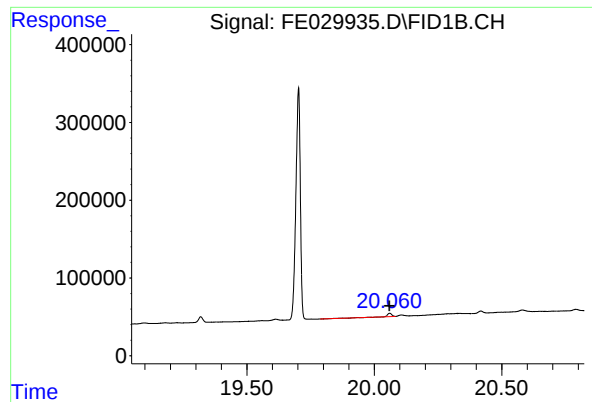

#14 N-HEXATRIACONTANE

R.T.: 20.060 min
Delta R.T.: 0.000 min
Response: 53113
Conc: 0.29 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER