

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042223AL\
 Data File : FE041494.D
 Signal(s) : FID1B.ch
 Acq On : 22 Apr 2023 00:49
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 22 04:06:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 07:33:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.599	66613	0.418 ug/ml
14) T n-Tetracosane (C24)	15.262	58285	0.362 ug/ml
15) T n-Hexacosane (C26)	16.300	20278	0.128 ug/ml
16) T n-Octacosane (C28)	17.250	29452	0.191 ug/ml
20) T n-Hexatriacontane (C36)	20.478	175507	1.312 ug/ml
21) T n-Octatriacontane (C38)	21.230	195499	1.480 ug/ml
22) T n-Tetracontane (C40)	22.208	285290	2.253 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042223AL\
Data File : FE041494.D
Signal(s) : FID1B.ch
Acq On : 22 Apr 2023 00:49
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 22 04:06:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

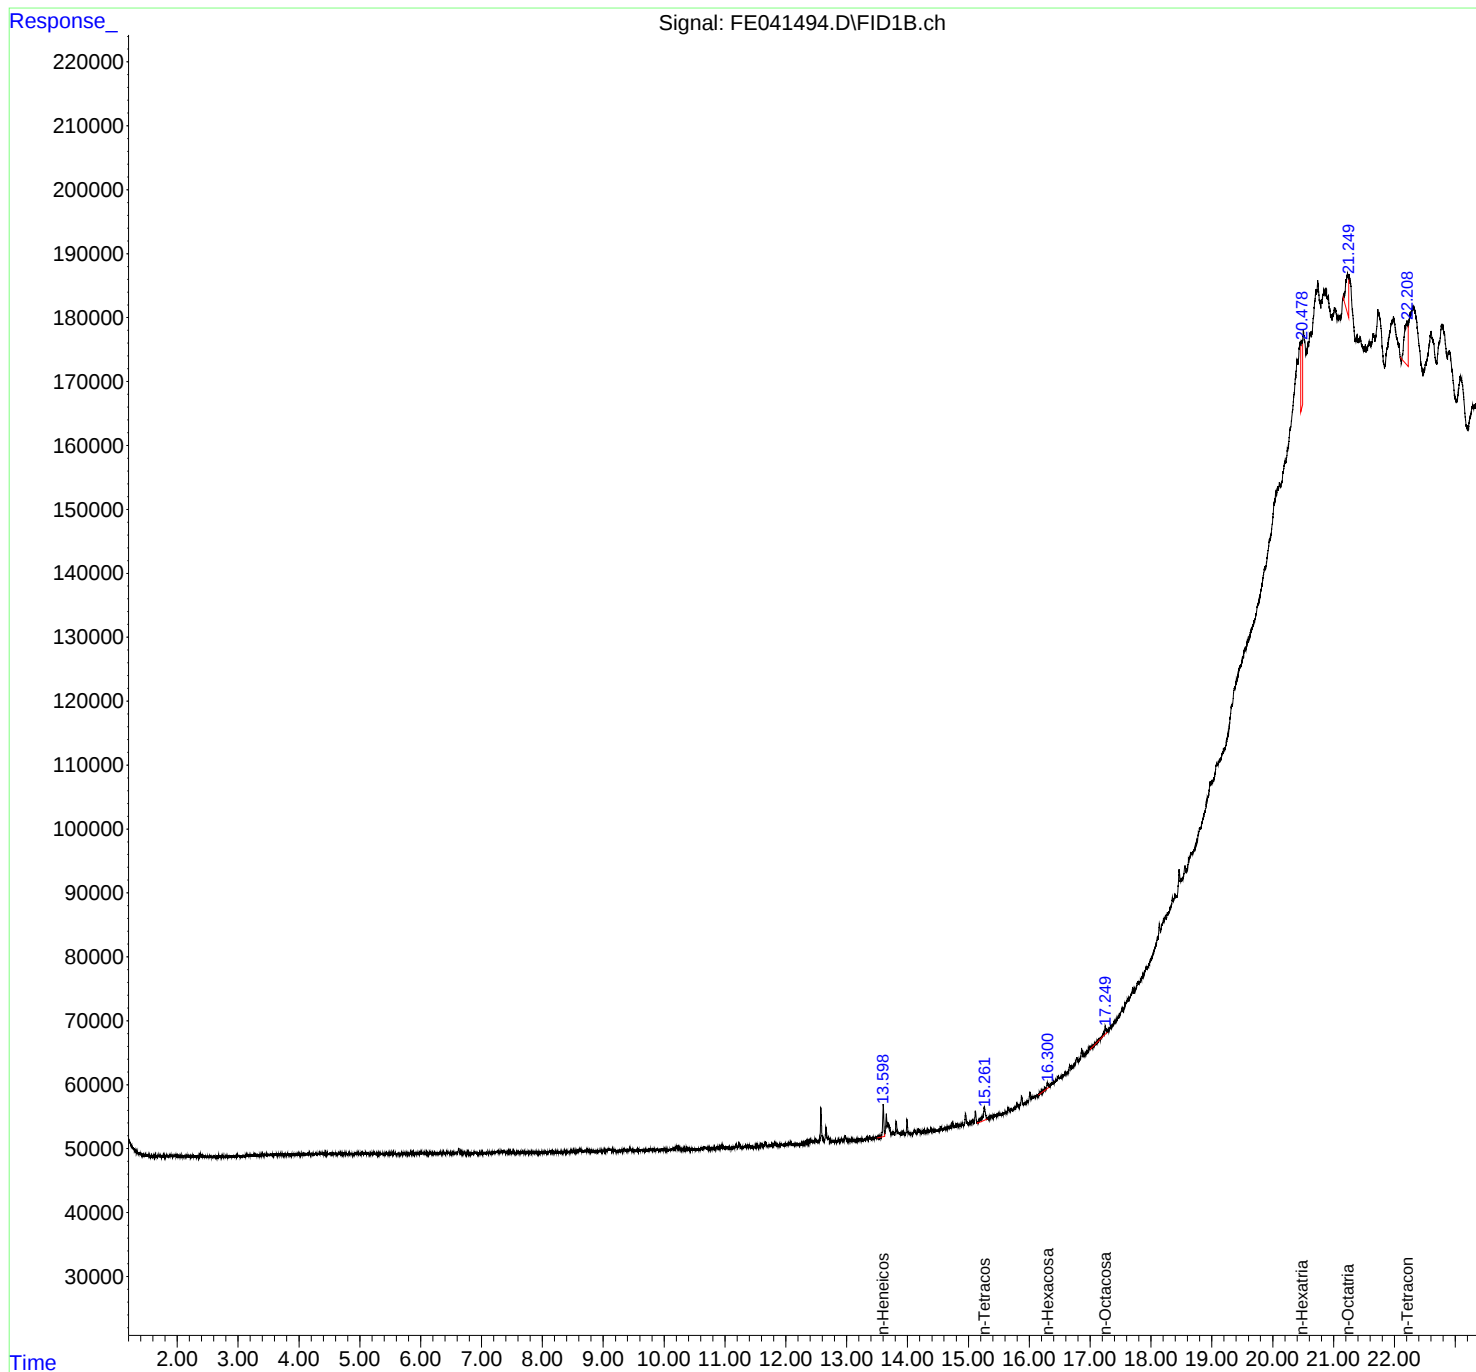


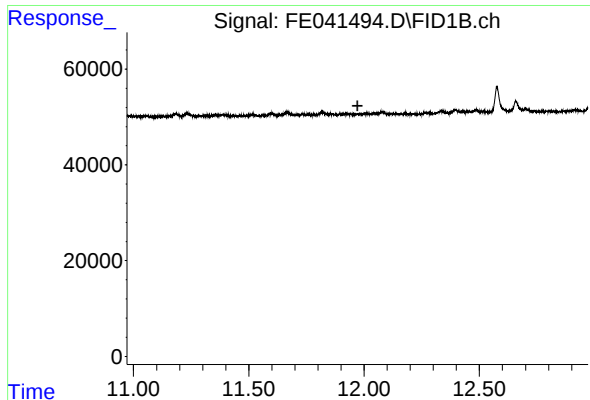

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.972 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

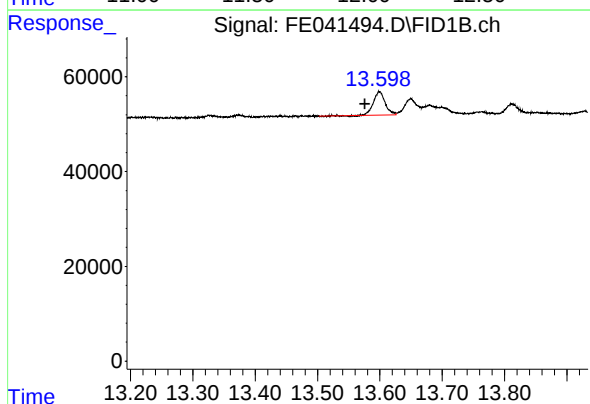


#11 n-Heneicosane (C21)

R.T.: 13.599 min
Delta R.T.: 0.023 min
Response: 66613
Conc: 0.42 ug/ml

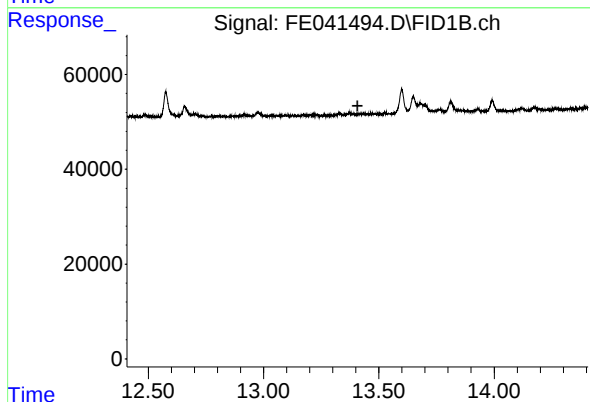


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.408 min
Response: 0
Conc: N.D.

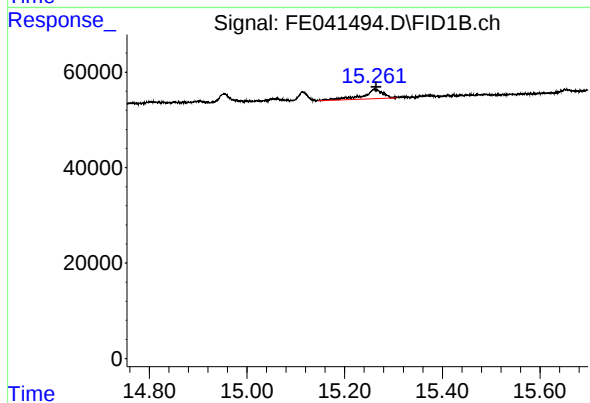

#14 n-Tetracosane (C24)


R.T.: 15.262 min
Delta R.T.: -0.003 min
Response: 58285
Conc: 0.36 ug/ml

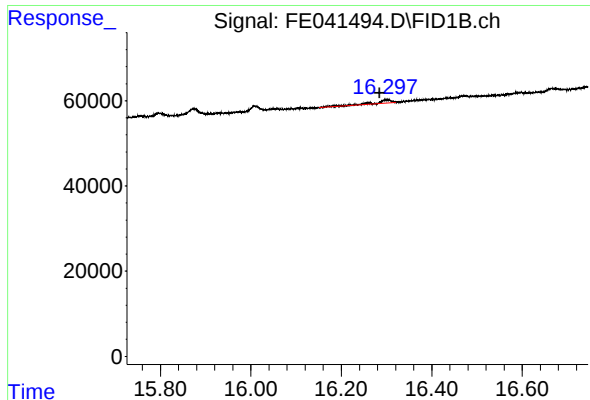

#15 n-Hexacosane (C26)


R.T.: 16.300 min
Delta R.T.: 0.015 min
Response: 20278
Conc: 0.13 ug/ml

Instrument :
FID_E
ClientSampleId :

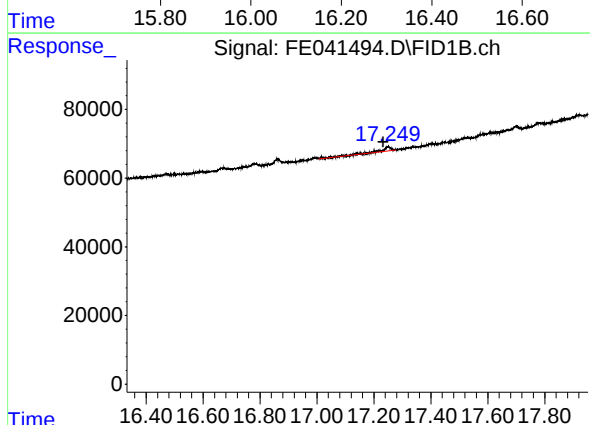


#16 n-Octacosane (C28)

R.T.: 17.250 min
Delta R.T.: 0.015 min
Response: 29452
Conc: 0.19 ug/ml

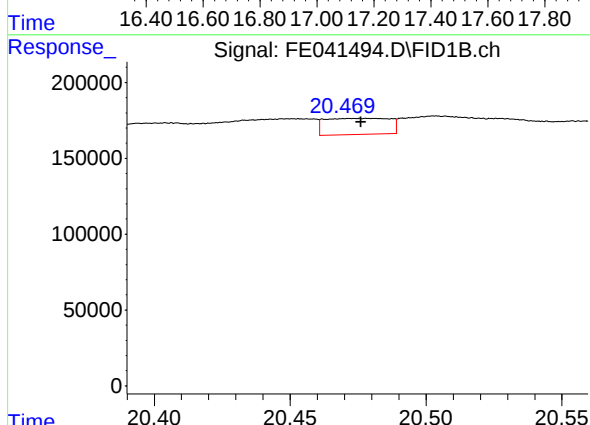


#20 n-Hexatriacontane (C36)

R.T.: 20.478 min
Delta R.T.: 0.002 min
Response: 175507
Conc: 1.31 ug/ml

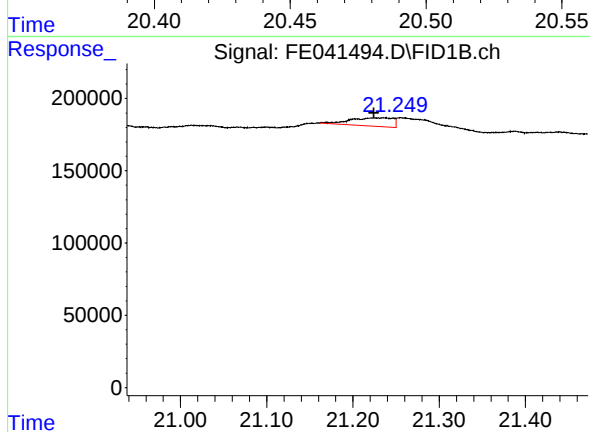

#21 n-Octatriacontane (C38)

R.T.: 21.230 min
Delta R.T.: 0.005 min
Response: 195499
Conc: 1.48 ug/ml

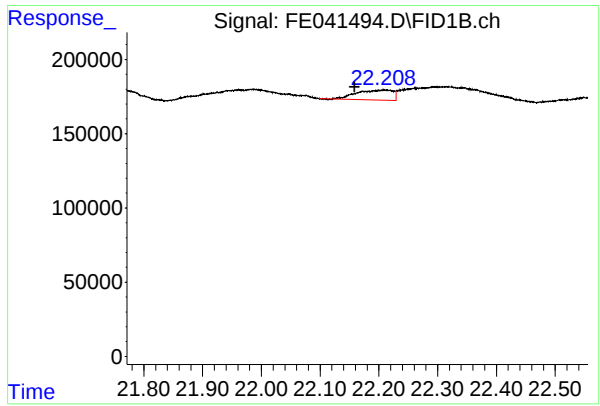

#22 n-Tetracontane (C40)

R.T.: 22.208 min
Delta R.T.: 0.050 min
Response: 285290
Conc: 2.25 ug/ml

Instrument :
FID_E
ClientSampleId :