

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042423AL\
Data File : FE041505.D
Signal(s) : FID1B.ch
Acq On : 24 Apr 2023 08:18
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 24 10:51:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	18.137	18401	0.121 ug/ml
18) T	n-Dotriacontane (C32)	18.998	31693	0.213 ug/ml
19) T	n-Tetratriacontane (C34)	19.743	17248	0.122 ug/ml
20) T	n-Hexatriacontane (C36)	20.486	28329	0.212 ug/ml
22) T	n-Tetracontane (C40)	22.172	163864	1.294 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042423AL\
Data File : FE041505.D
Signal(s) : FID1B.ch
Acq On : 24 Apr 2023 08:18
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 24 10:51:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

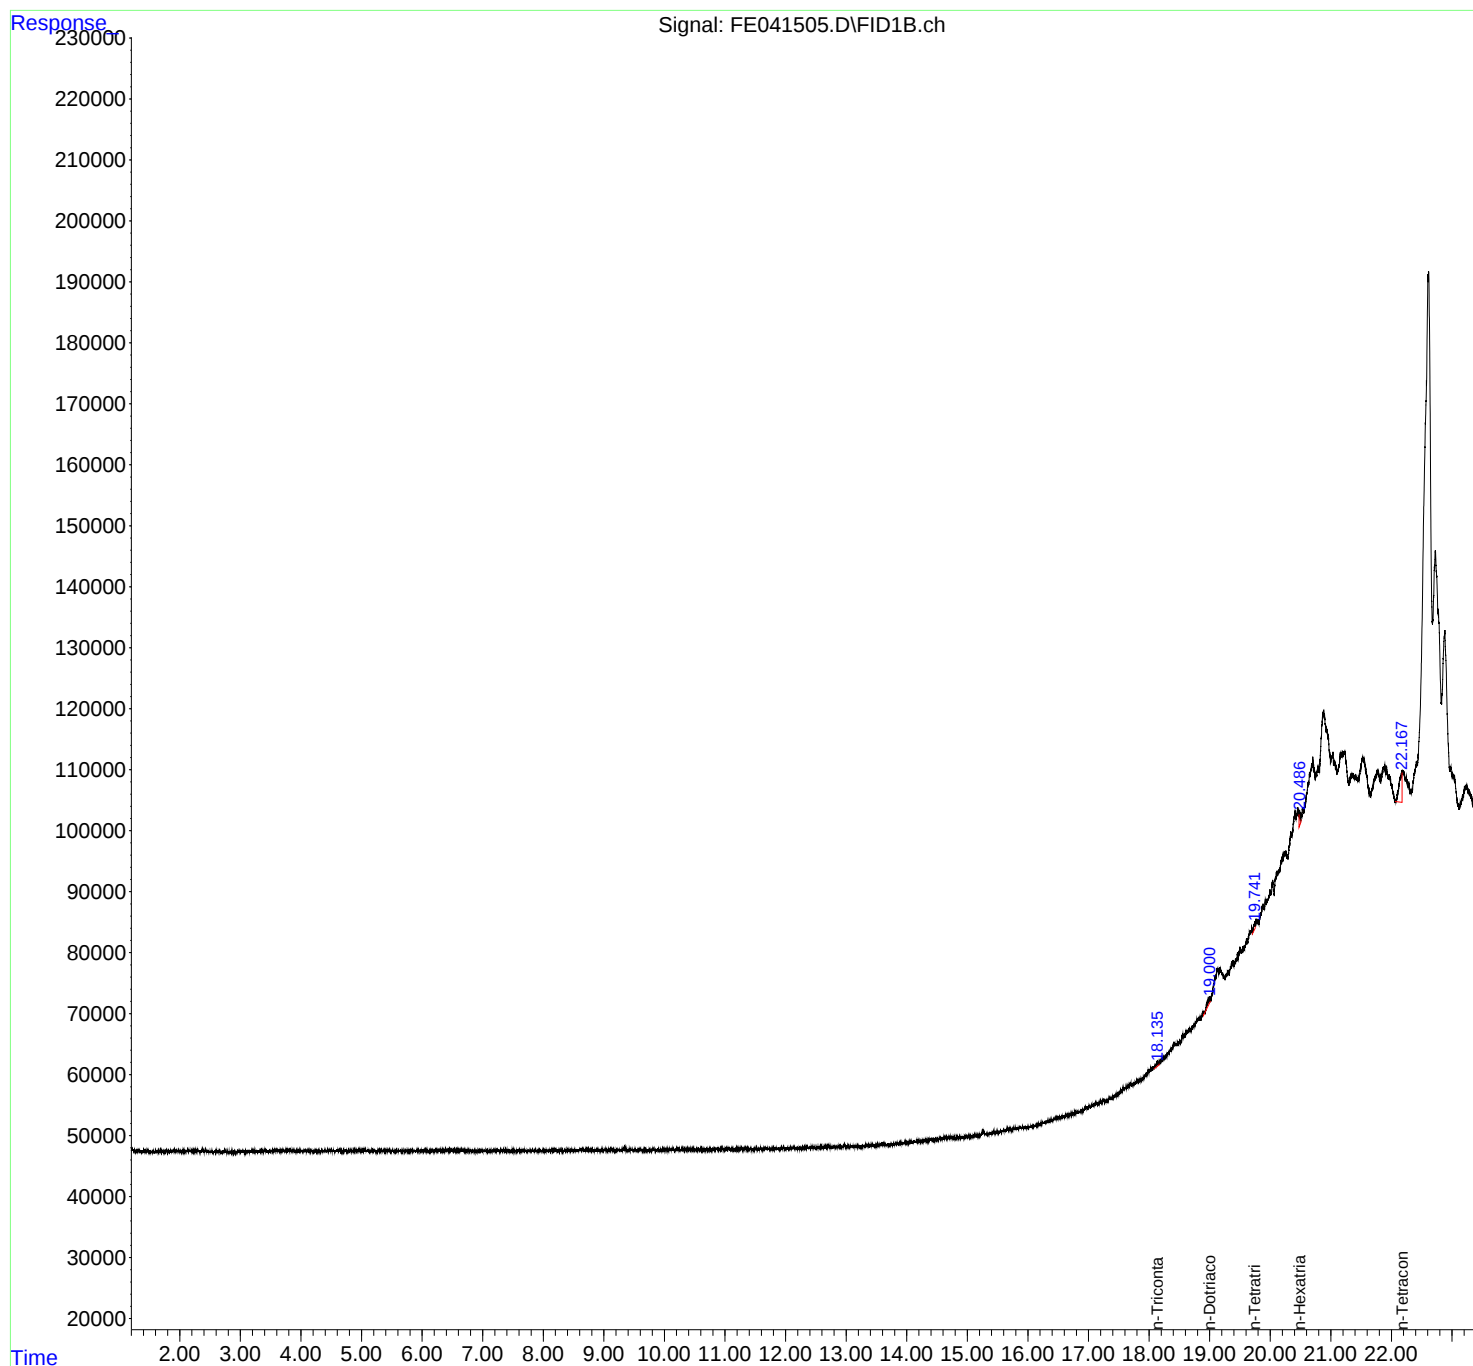


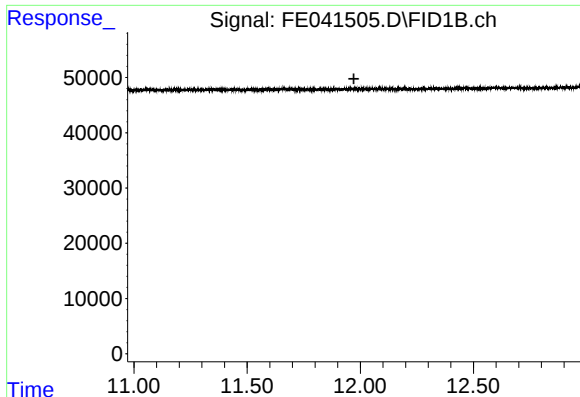

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.972 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

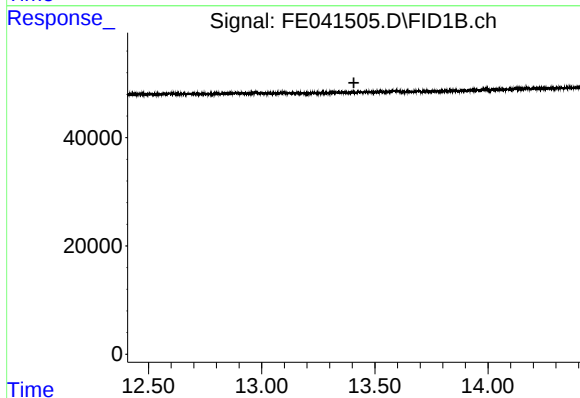


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.408 min
Response: 0
Conc: N.D.

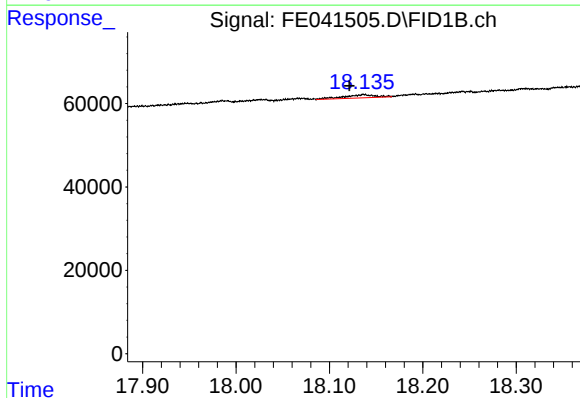


#17 n-Tricontane (C30)

R.T.: 18.137 min
Delta R.T.: 0.015 min
Response: 18401
Conc: 0.12 ug/ml

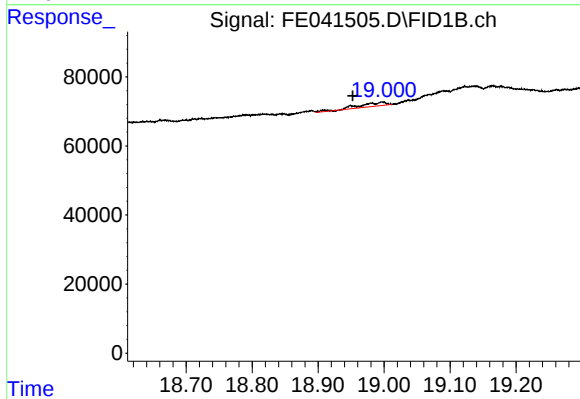

#18 n-Dotriacontane (C32)


R.T.: 18.998 min
Delta R.T.: 0.046 min
Response: 31693
Conc: 0.21 ug/ml

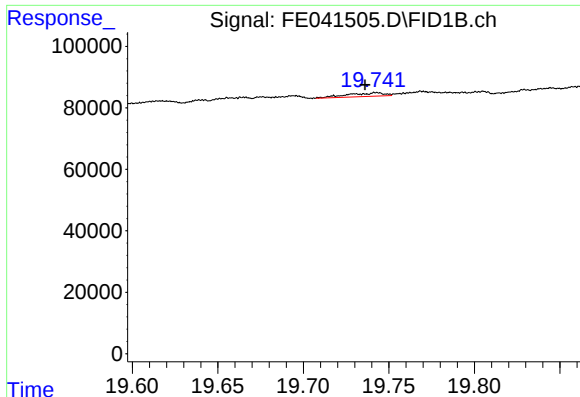

#19 n-Tetratriacontane (C34)


R.T.: 19.743 min
Delta R.T.: 0.007 min
Response: 17248
Conc: 0.12 ug/ml

Instrument :
FID_E
ClientSampleId :

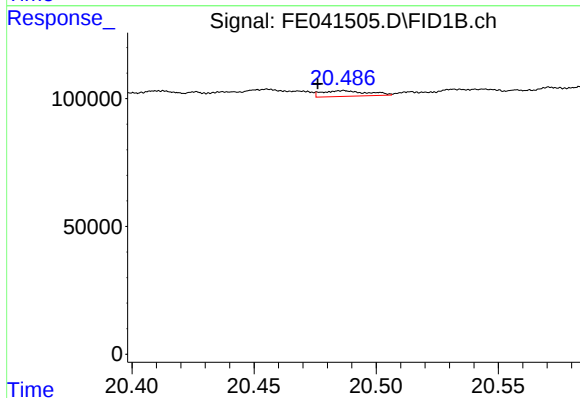

#20 n-Hexatriacontane (C36)

R.T.: 20.486 min
Delta R.T.: 0.010 min
Response: 28329
Conc: 0.21 ug/ml

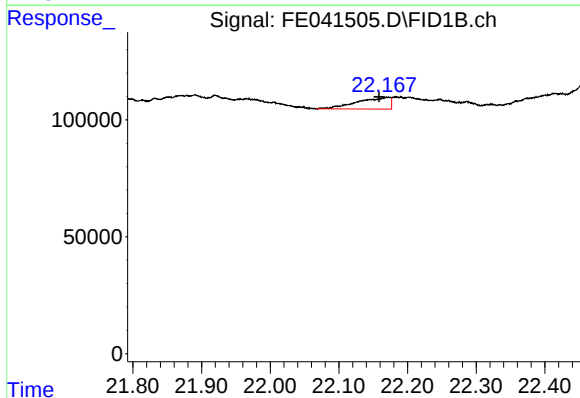

#22 n-Tetracontane (C40)

R.T.: 22.172 min
Delta R.T.: 0.013 min
Response: 163864
Conc: 1.29 ug/ml