

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042423AL\
 Data File : FE041520.D
 Signal(s) : FID1B.ch
 Acq On : 24 Apr 2023 15:50
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 25 01:36:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 07:33:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	n-Tetracosane (C24)	15.262	36501	0.226 ug/ml
17) T	n-Tricontane (C30)	18.148	59675	0.392 ug/ml
18) T	n-Dotriacontane (C32)	18.950	46940	0.315 ug/ml
19) T	n-Tetratriacontane (C34)	19.736	65597	0.466 ug/ml
20) T	n-Hexatriacontane (C36)	20.484	103159	0.771 ug/ml
21) T	n-Octatriacontane (C38)	21.185	72794	0.551 ug/ml
22) T	n-Tetracontane (C40)	22.155	219572	1.734 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042423AL\
Data File : FE041520.D
Signal(s) : FID1B.ch
Acq On : 24 Apr 2023 15:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 25 01:36:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

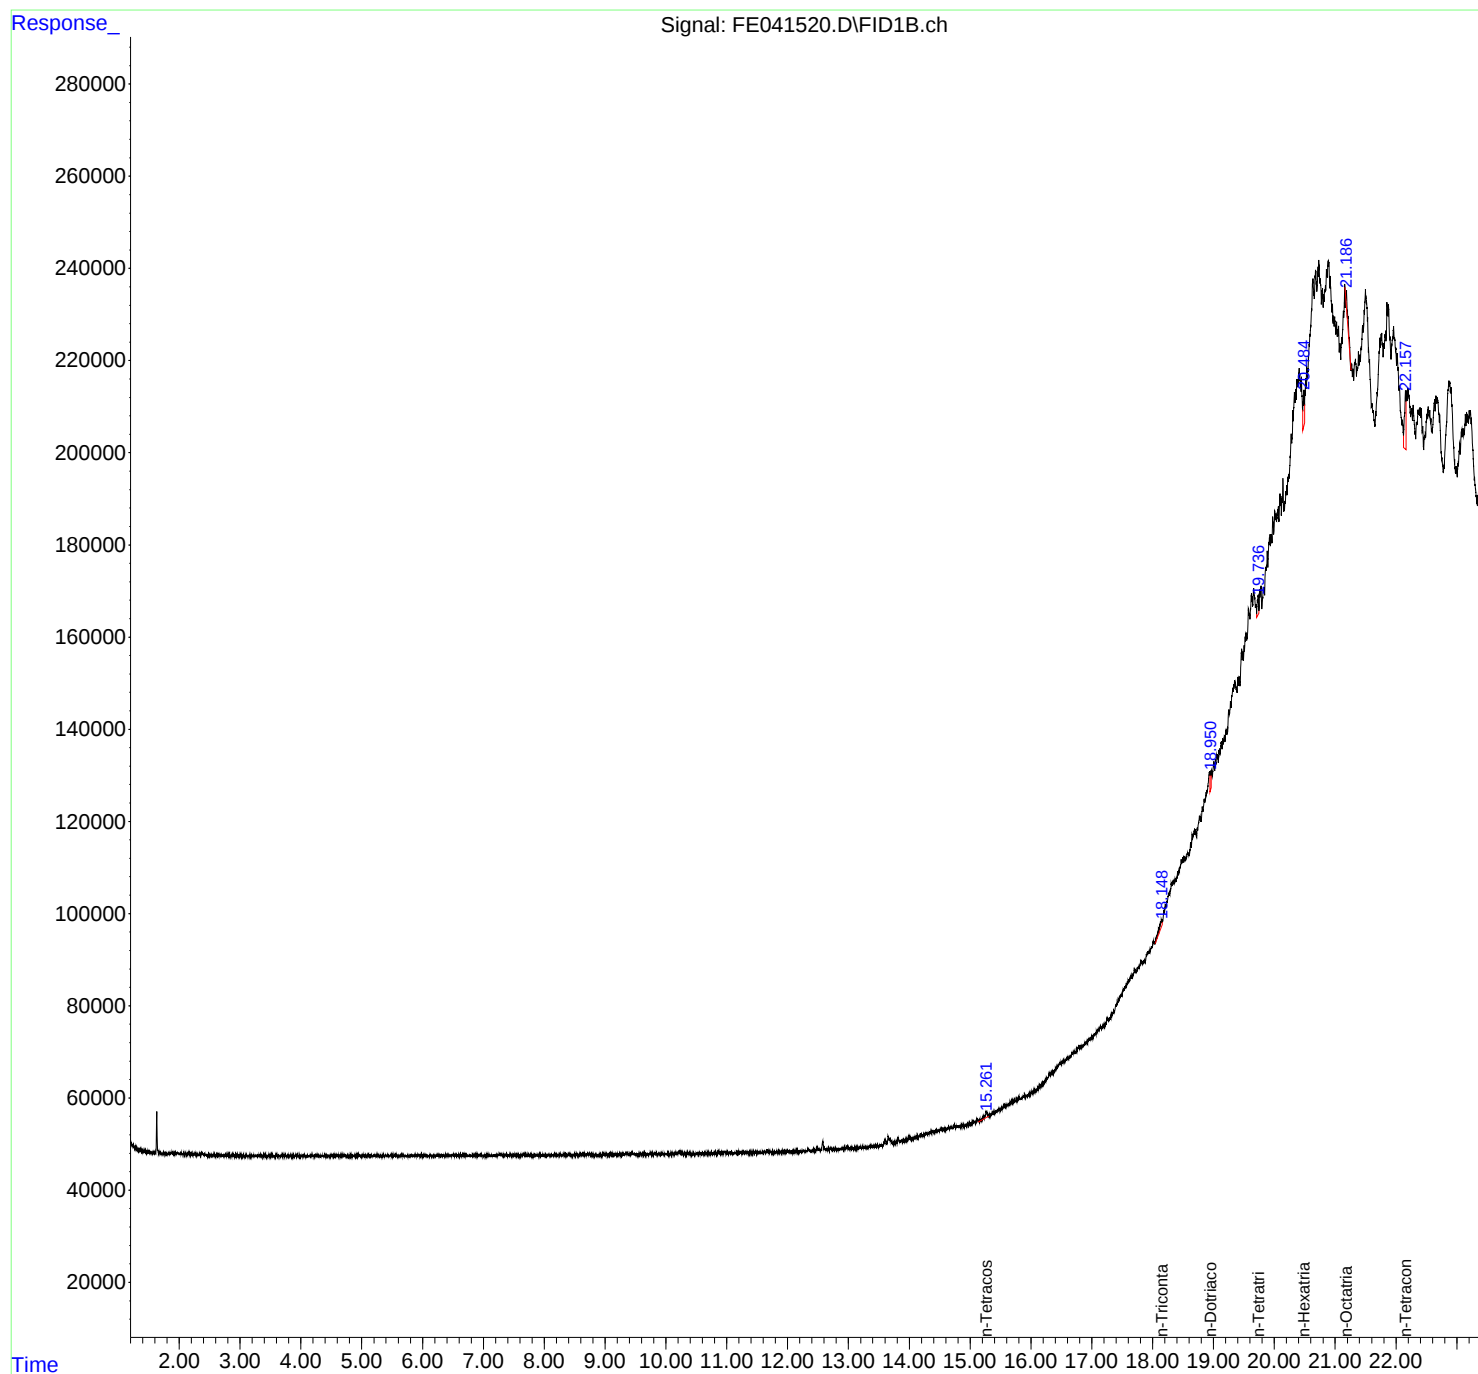


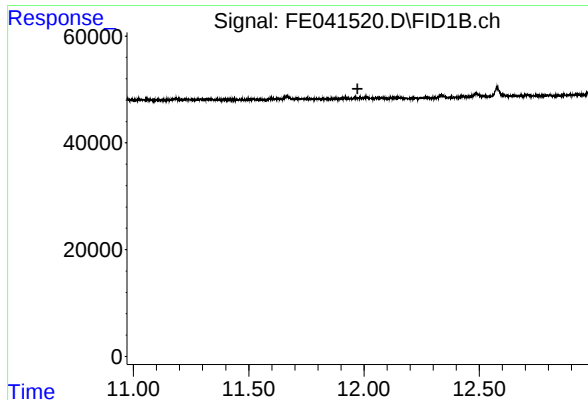

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.972 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

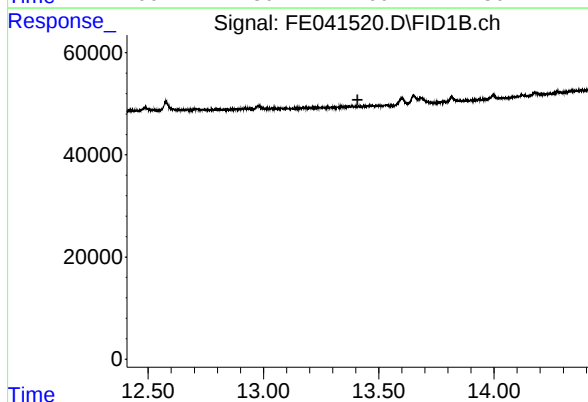


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.408 min
Response: 0
Conc: N.D.

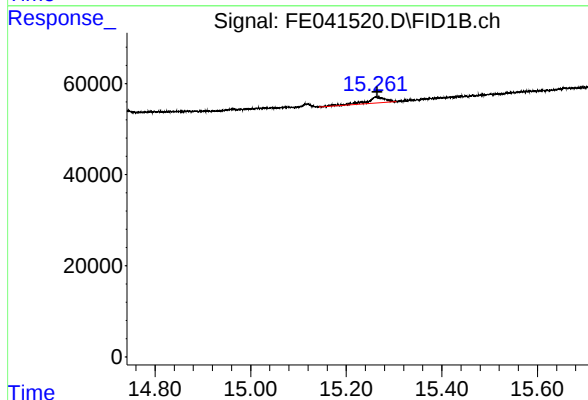


#14 n-Tetracosane (C24)

R.T.: 15.262 min
Delta R.T.: -0.003 min
Response: 36501
Conc: 0.23 ug/ml

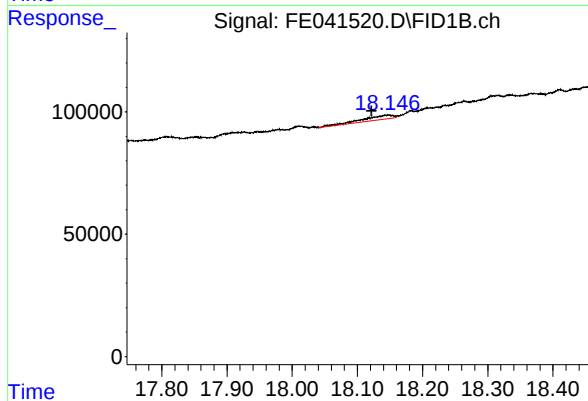

#17 n-Tricontane (C30)


R.T.: 18.148 min
Delta R.T.: 0.026 min
Response: 59675
Conc: 0.39 ug/ml

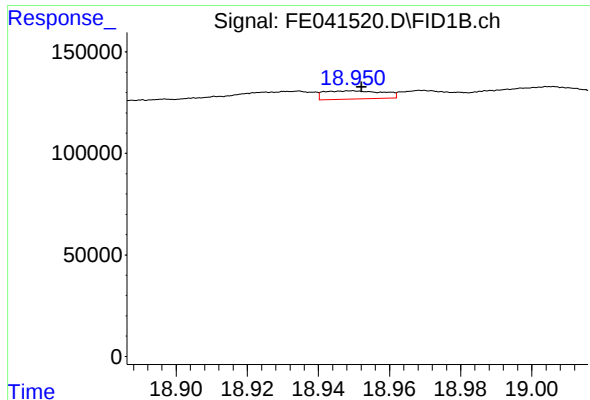

#18 n-Dotriacontane (C32)


R.T.: 18.950 min
Delta R.T.: -0.003 min
Response: 46940
Conc: 0.32 ug/ml

Instrument :
FID_E
ClientSampleId :

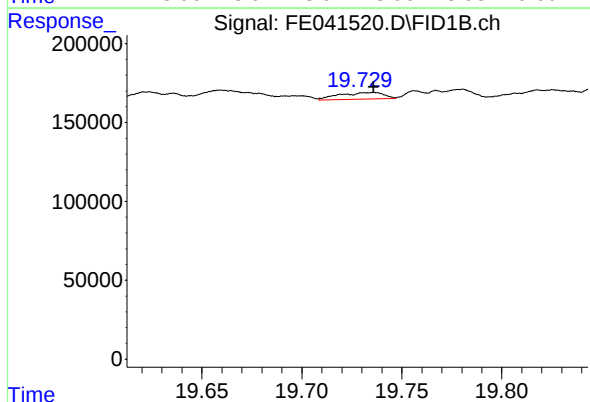


#19 n-Tetratriacontane (C34)

R.T.: 19.736 min
Delta R.T.: 0.000 min
Response: 65597
Conc: 0.47 ug/ml

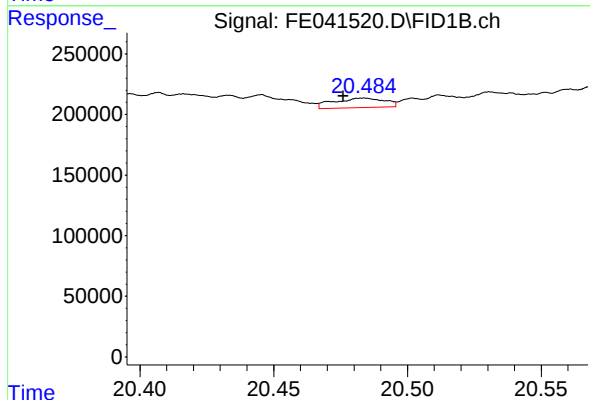


#20 n-Hexatriacontane (C36)

R.T.: 20.484 min
Delta R.T.: 0.007 min
Response: 103159
Conc: 0.77 ug/ml

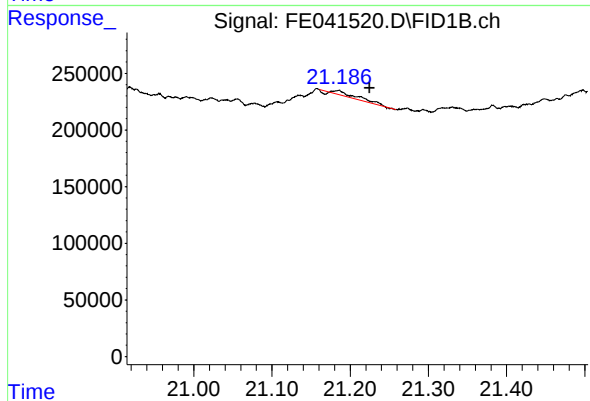

#21 n-Octatriacontane (C38)

R.T.: 21.185 min
Delta R.T.: -0.040 min
Response: 72794
Conc: 0.55 ug/ml

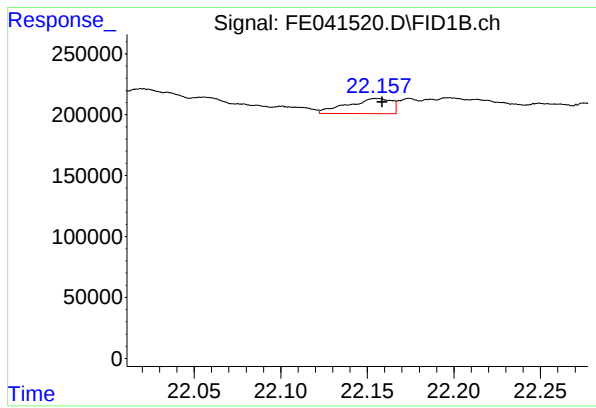

#22 n-Tetracontane (C40)

R.T.: 22.155 min
Delta R.T.: -0.003 min
Response: 219572
Conc: 1.73 ug/ml

Instrument :
FID_E
ClientSampleId :