

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042424AL\
 Data File : FE047751.D
 Signal(s) : FID1B.ch
 Acq On : 24 Apr 2024 08:27
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 25 03:37:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 040224.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 02 05:28:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.956	53111	0.328 ug/ml
11) T n-Heneicosane (C21)	13.571	53798	0.339 ug/ml
13) T n-Docosane (C22)	14.158	49051	0.306 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042424AL\
Data File : FE047751.D
Signal(s) : FID1B.ch
Acq On : 24 Apr 2024 08:27
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 25 03:37:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 040224.M
Quant Title : GC Extractables
QLast Update : Tue Apr 02 05:28:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

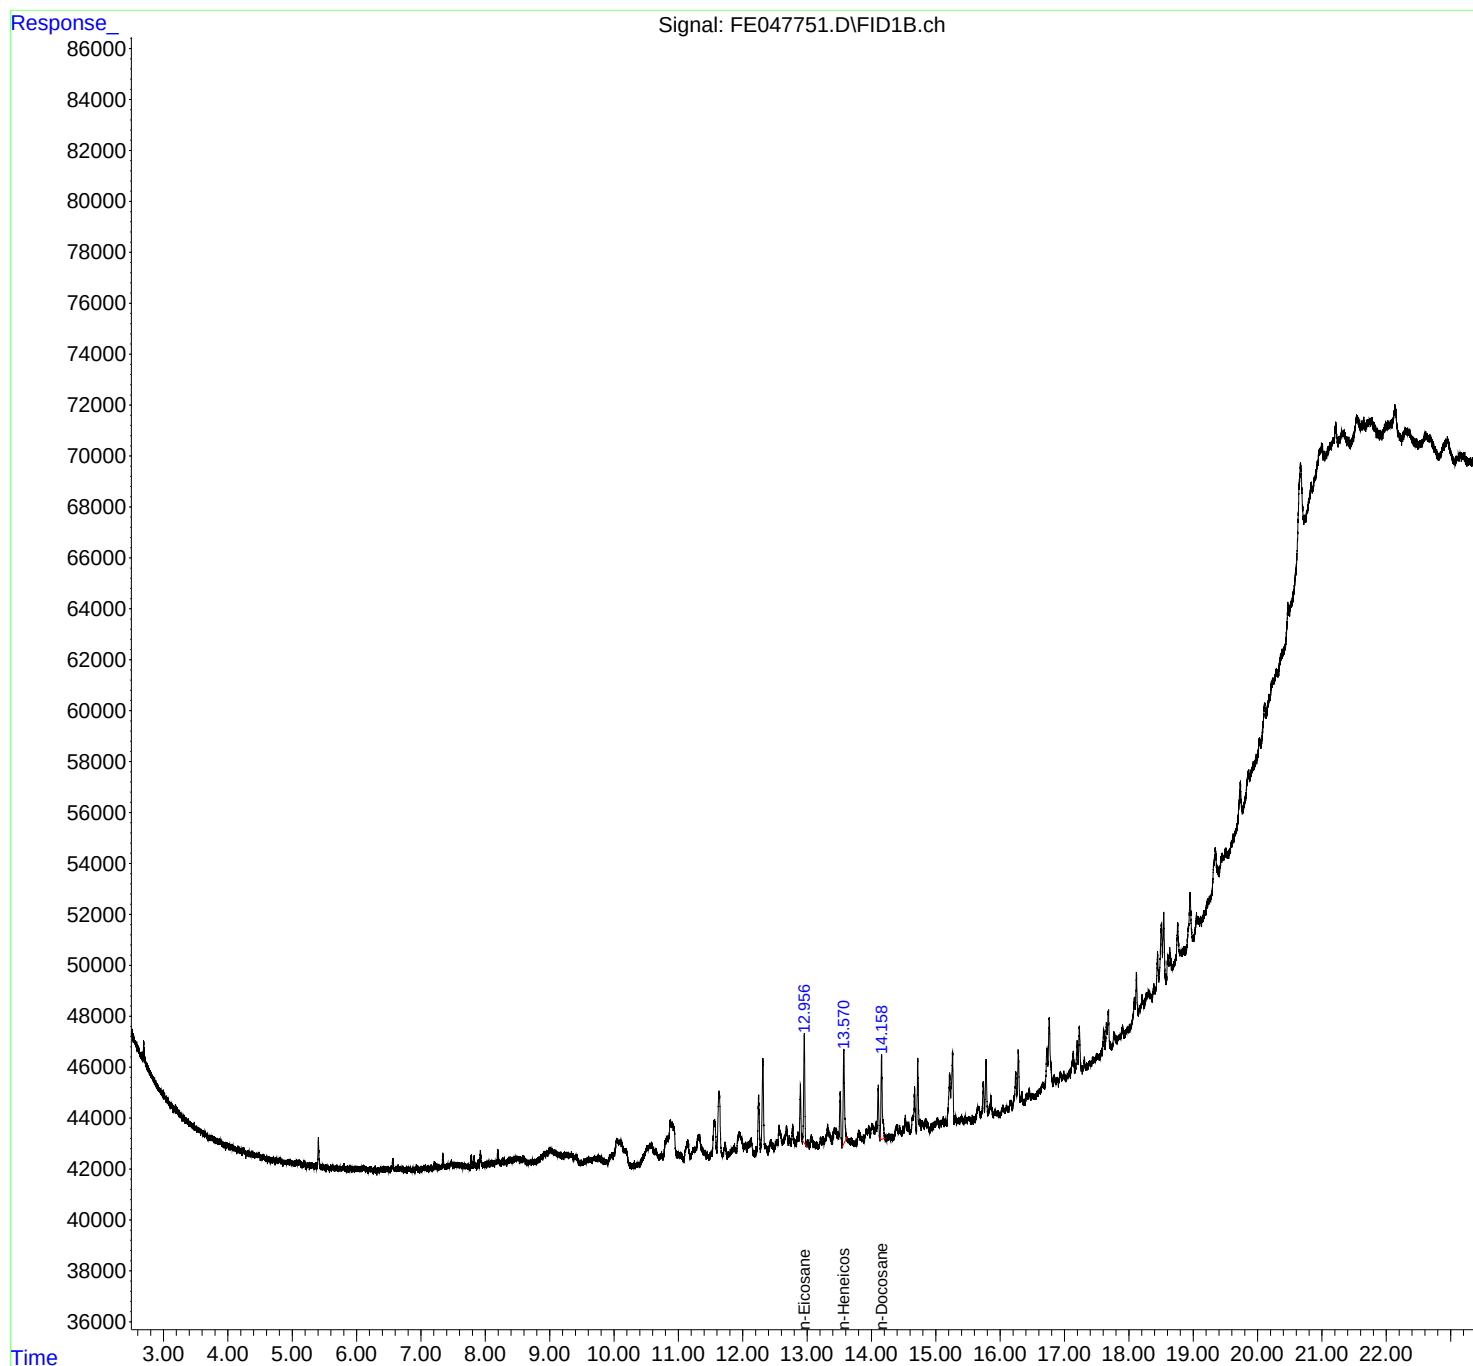


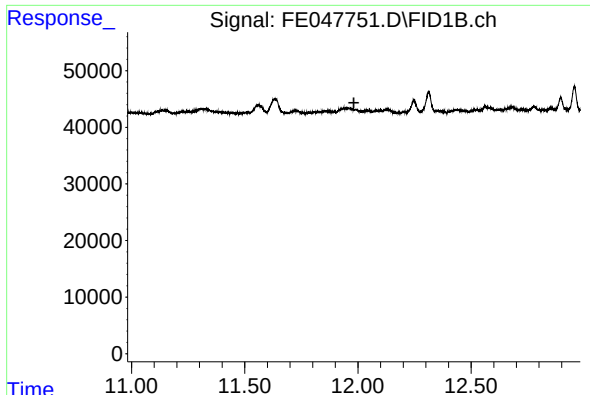

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.982 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

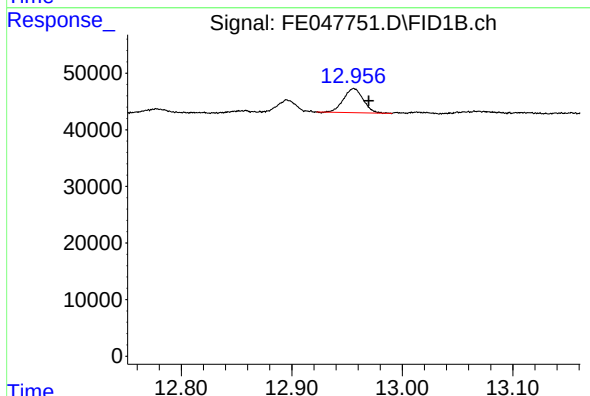


#10 n-Eicosane (C20)

R.T.: 12.956 min
Delta R.T.: -0.013 min
Response: 53111
Conc: 0.33 ug/ml

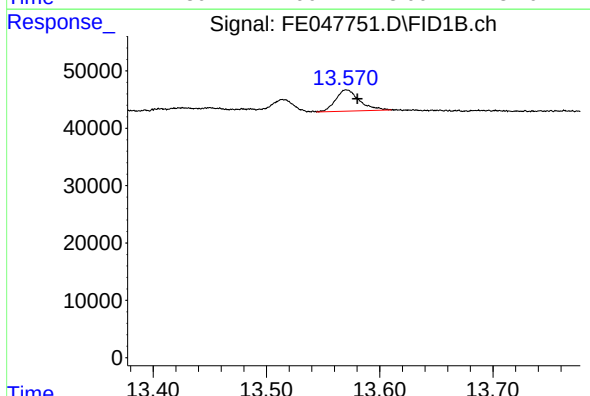


#11 n-Heneicosane (C21)

R.T.: 13.571 min
Delta R.T.: -0.010 min
Response: 53798
Conc: 0.34 ug/ml

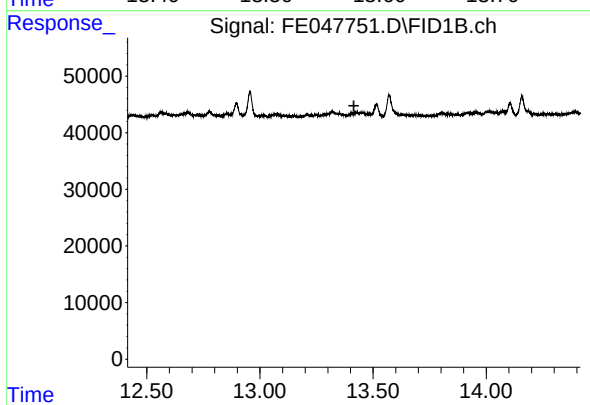

#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.415 min
Response: 0
Conc: N.D.

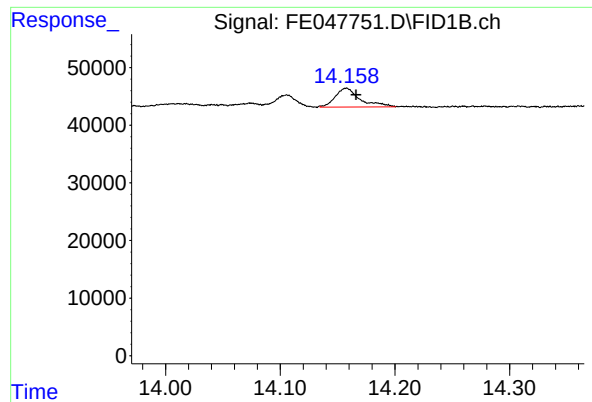

#13 n-Docosane (C22)

R.T.: 14.158 min
Delta R.T.: -0.009 min
Response: 49051
Conc: 0.31 ug/ml

Instrument :

FID_E

ClientSampleId :