

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE042424AL\  
 Data File : FE047770.D  
 Signal(s) : FID1B.ch  
 Acq On : 24 Apr 2024 22:18  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Apr 25 03:42:17 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 040224.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Apr 02 05:28:28 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

#### System Monitoring Compounds

##### Target Compounds

|       |                          |         |        |             |
|-------|--------------------------|---------|--------|-------------|
| 18) T | n-Dotriacontane (C32)    | 18.962  | 33473  | 0.201 ug/ml |
| 19) T | n-Tetratriacontane (C34) | 19.673f | 105510 | 0.658 ug/ml |
| 20) T | n-Hexatriacontane (C36)  | 20.444  | 43279  | 0.271 ug/ml |
| 21) T | n-Octatriacontane (C38)  | 21.239  | 64336  | 0.396 ug/ml |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE042424AL\  
Data File : FE047770.D  
Signal(s) : FID1B.ch  
Acq On : 24 Apr 2024 22:18  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Apr 25 03:42:17 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 040224.M  
Quant Title : GC Extractables  
QLast Update : Tue Apr 02 05:28:28 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

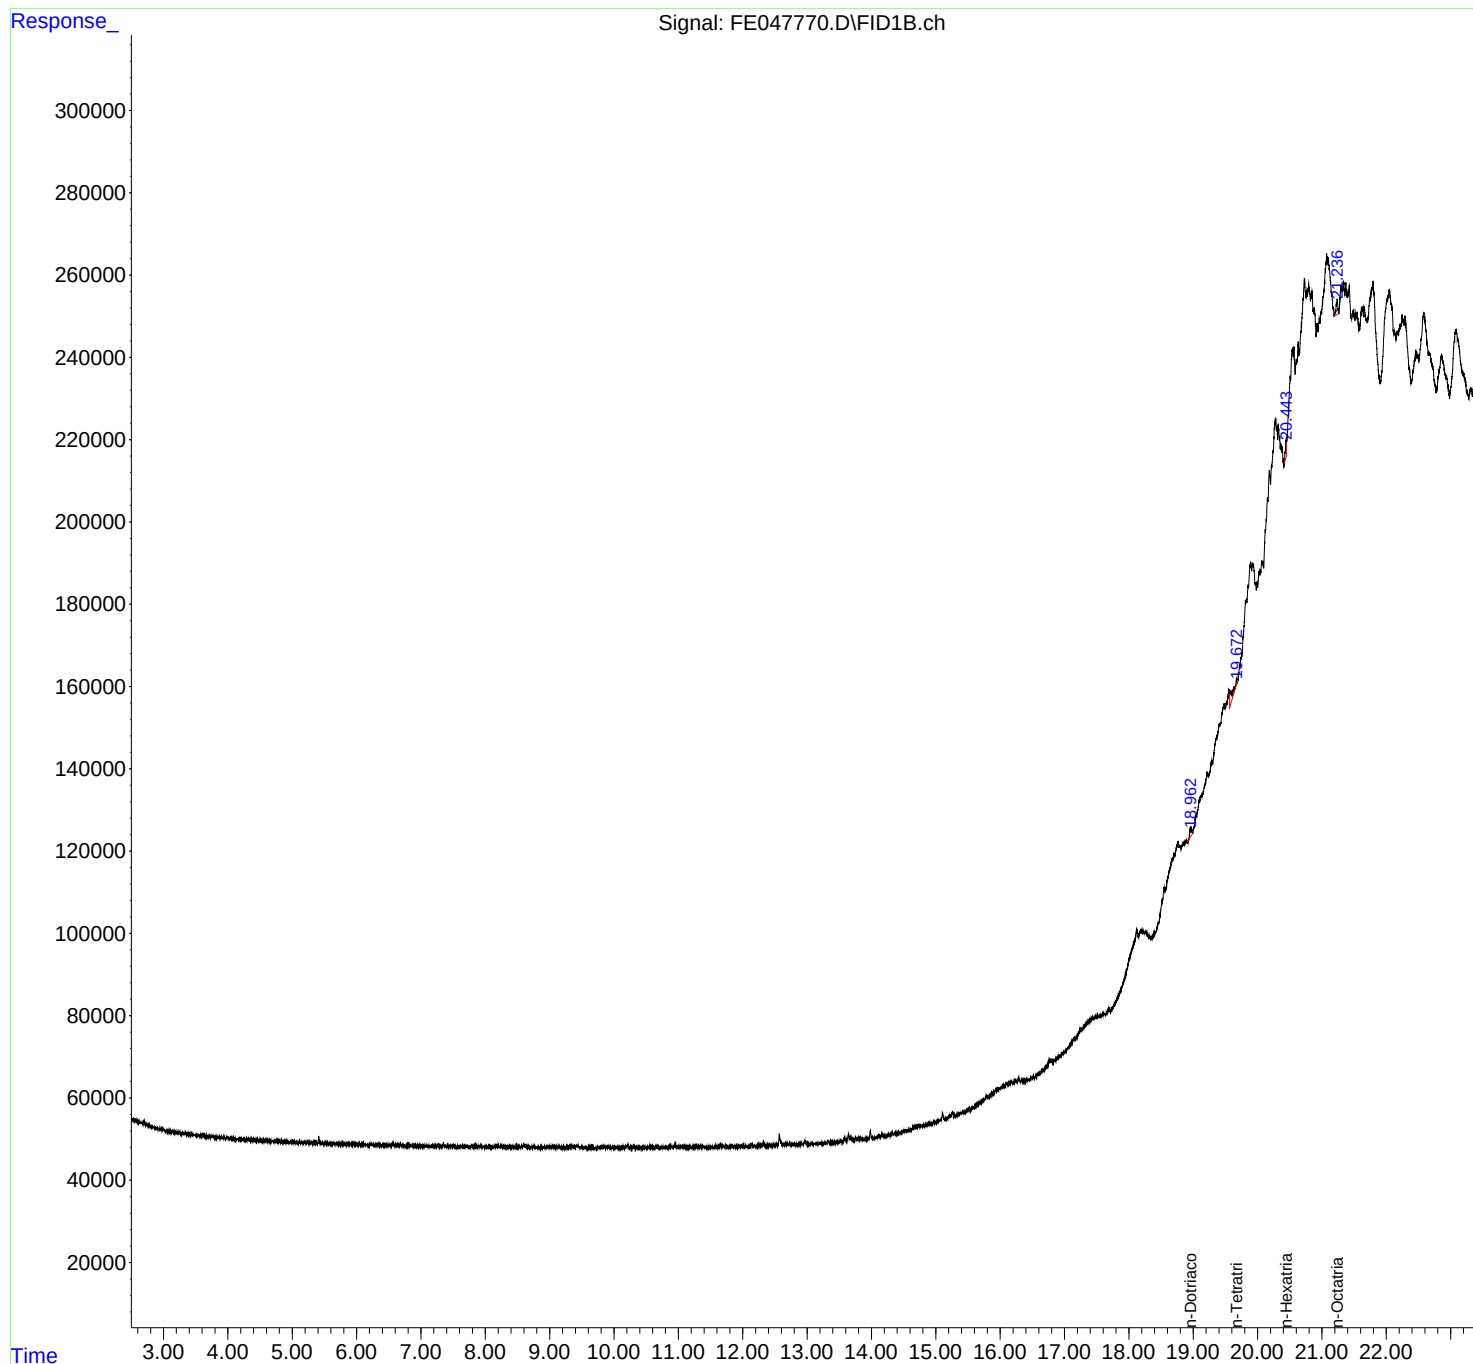


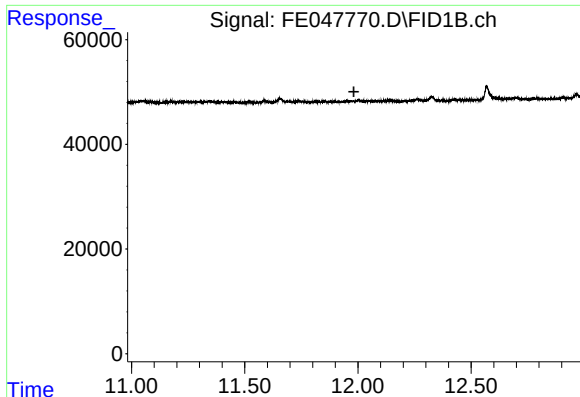

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min  
Exp R.T.: 11.982 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :

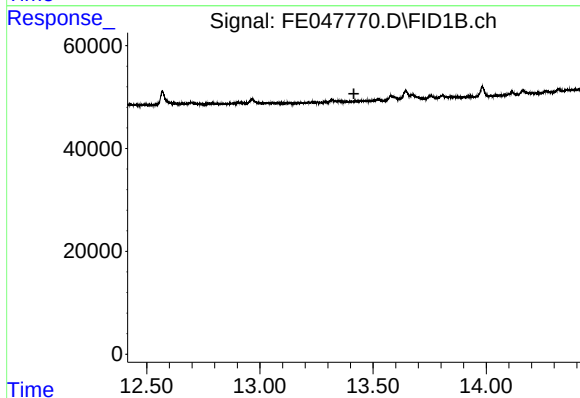


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min  
Exp R.T.: 13.415 min  
Response: 0  
Conc: N.D.

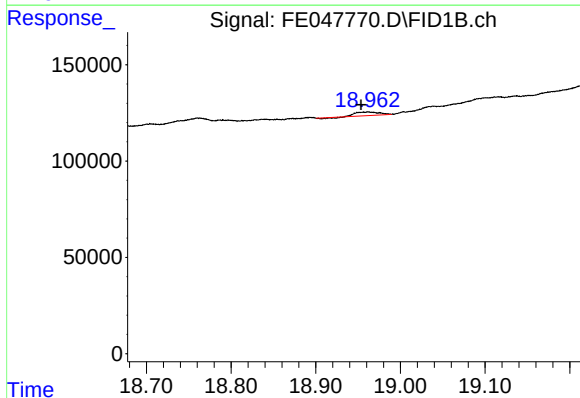


#18 n-Dotriacontane (C32)

R.T.: 18.962 min  
Delta R.T.: 0.008 min  
Response: 33473  
Conc: 0.20 ug/ml

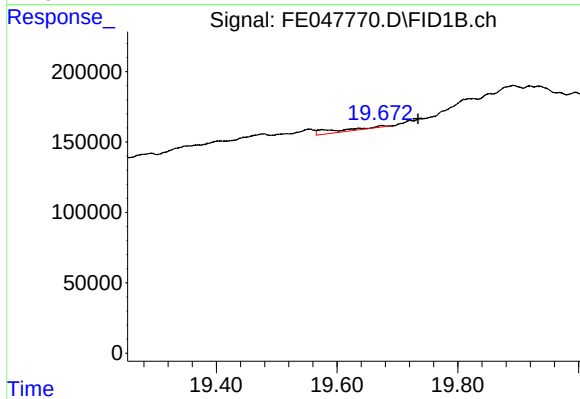

#19 n-Tetratriacontane (C34)


R.T.: 19.673 min  
Delta R.T.: -0.061 min  
Response: 105510  
Conc: 0.66 ug/ml

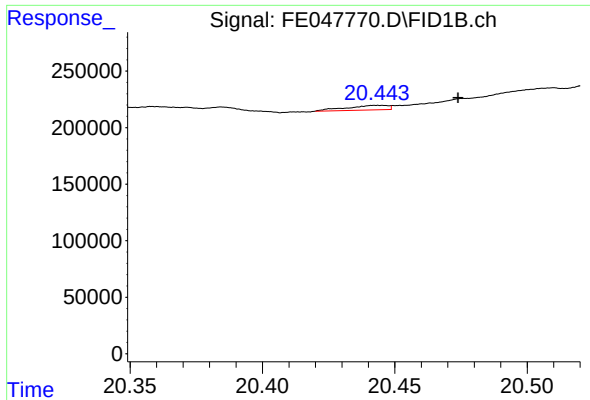

#20 n-Hexatriacontane (C36)

R.T.: 20.444 min  
Delta R.T.: -0.030 min  
Response: 43279  
Conc: 0.27 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

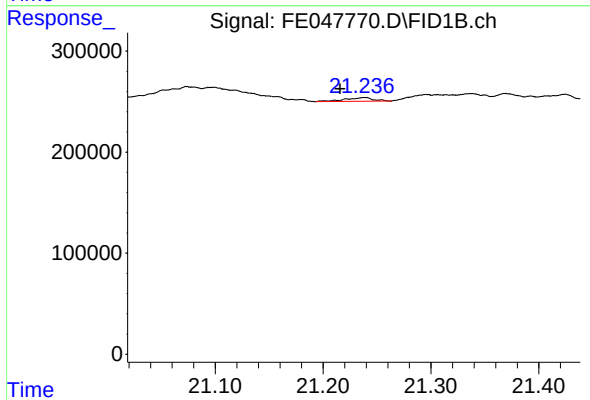

#21 n-Octatriacontane (C38)

R.T.: 21.239 min  
Delta R.T.: 0.023 min  
Response: 64336  
Conc: 0.40 ug/ml