

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042520\
 Data File : FE031833.D
 Signal(s) : FID1B.CH
 Acq On : 25 Apr 2020 11:56
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Apr 27 03:45:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
 Quant Title :
 QLast Update : Tue Apr 07 15:06:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.150	7085251	18.913 ug/ml
12) N-OCTACOSANE	16.557	7608378	18.494 ug/ml
13) N-TRIACONTANE	17.438	299220	0.728 ug/ml
14) N-DOTRIACONTANE	18.272	274784	0.699 ug/ml
15) N-TETRATRIACONTANE	19.057	249791	0.675 ug/ml
16) N-HEXATRIACONTANE	19.799	1716467	4.978 ug/ml
17) N-OCTATRIACONTANE	20.502	3229977	10.444 ug/ml
18) N-TETRACONTANE	21.310	533096	1.687 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042520\
Data File : FE031833.D
Signal(s) : FID1B.CH
Acq On : 25 Apr 2020 11:56
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 27 03:45:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
Quant Title :
QLast Update : Tue Apr 07 15:06:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

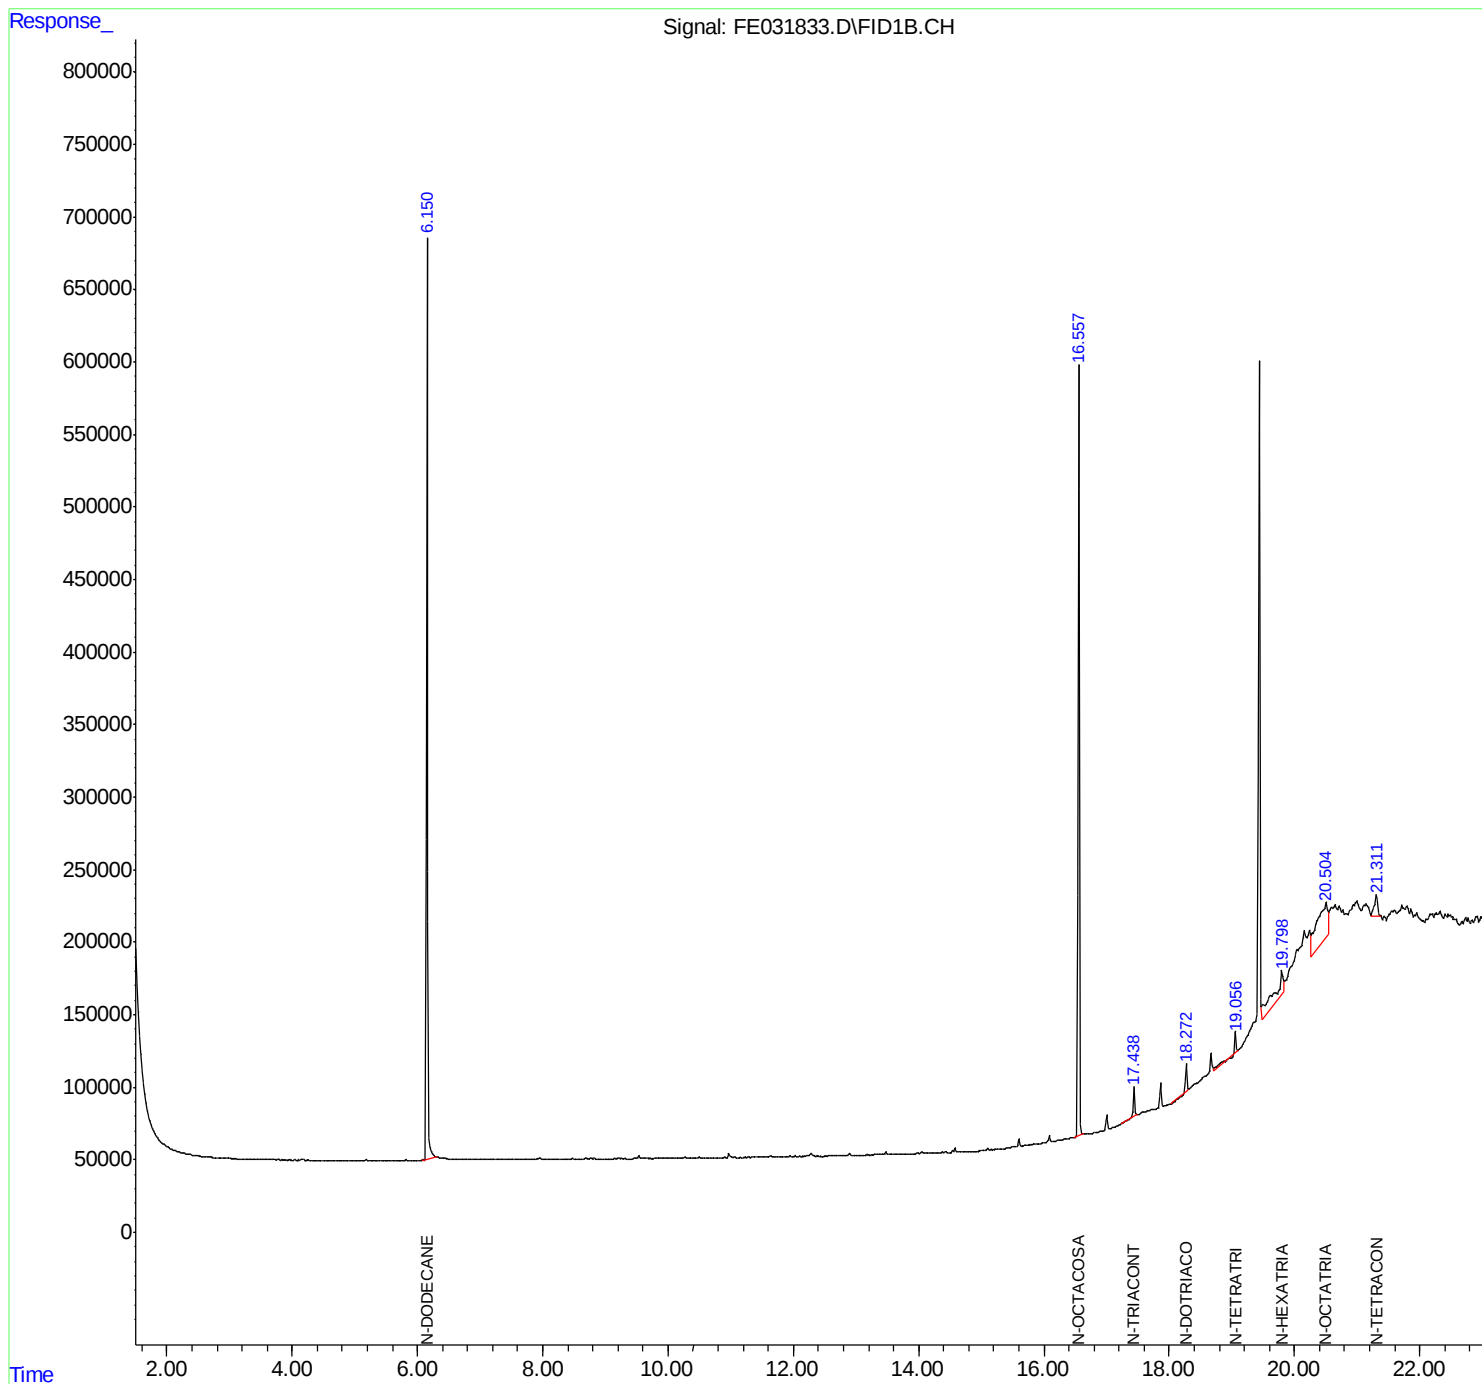


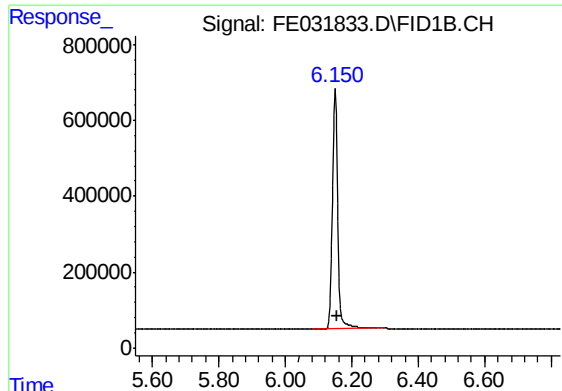

#3 N-DODECANE


R.T.: 6.150 min
Delta R.T.: -0.004 min
Response: 7085251
Conc: 18.91 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

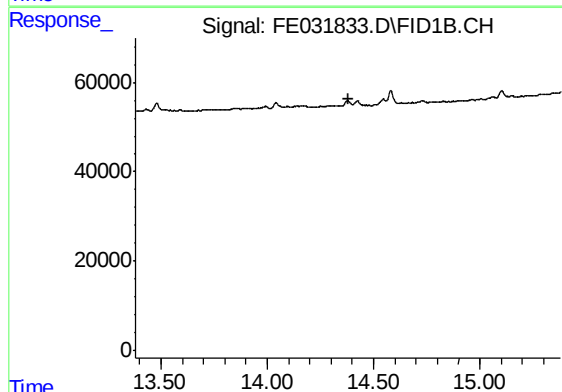


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.379 min
Response: 0
Conc: N.D.

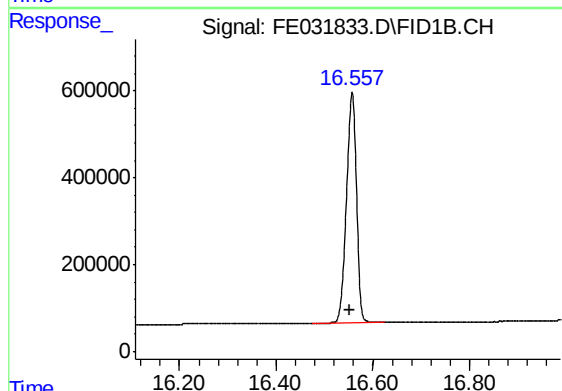


#12 N-OCTACOSANE

R.T.: 16.557 min
Delta R.T.: 0.005 min
Response: 7608378
Conc: 18.49 ug/ml

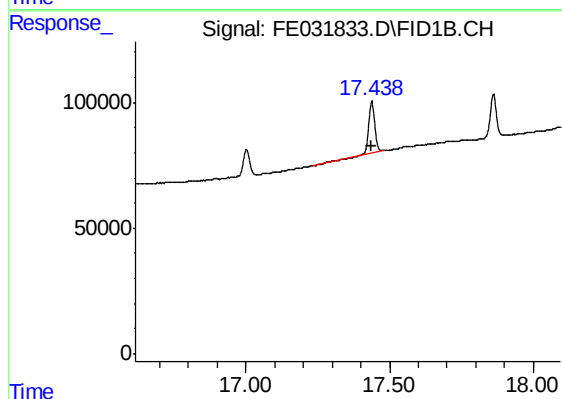

#13 N-TRIACONTANE


R.T.: 17.438 min
Delta R.T.: 0.000 min
Response: 299220
Conc: 0.73 ug/ml

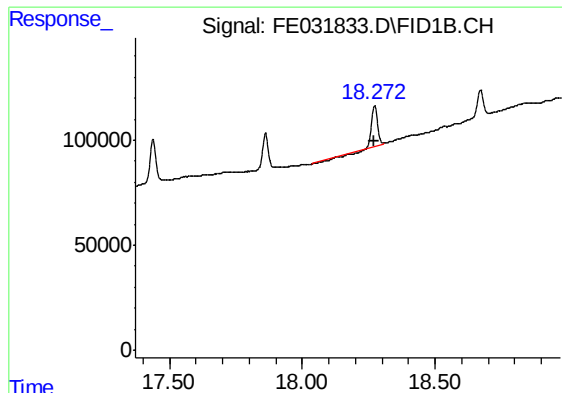

#14 N-DOTRIACONTANE


R.T.: 18.272 min
Delta R.T.: 0.002 min
Response: 274784
Conc: 0.70 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

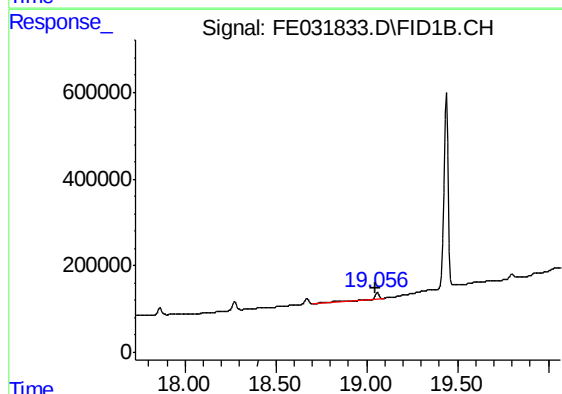


#15 N-TETRATRIACONTANE

R.T.: 19.057 min
Delta R.T.: 0.005 min
Response: 249791
Conc: 0.67 ug/ml

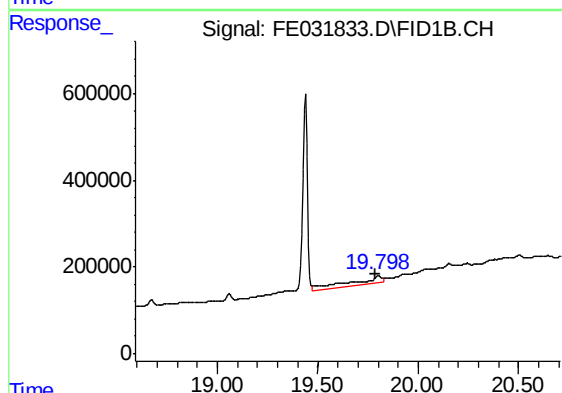


#16 N-HEXATRIACONTANE

R.T.: 19.799 min
Delta R.T.: 0.009 min
Response: 1716467
Conc: 4.98 ug/ml

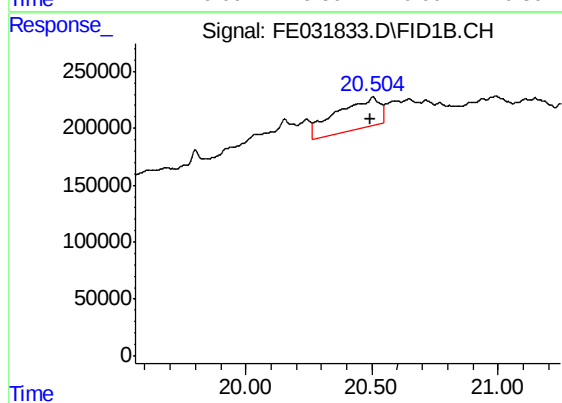

#17 N-OCTATRIACONTANE

R.T.: 20.502 min
Delta R.T.: 0.011 min
Response: 3229977
Conc: 10.44 ug/ml

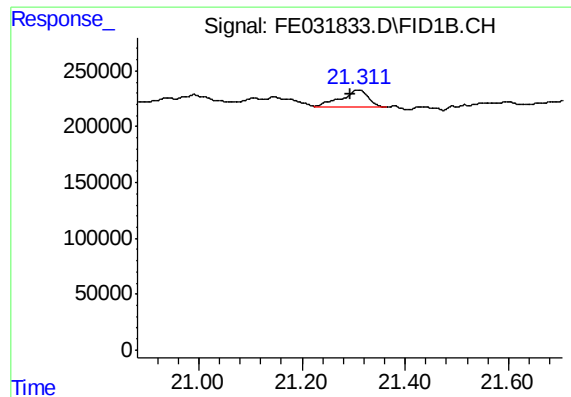

#18 N-TETRACONTANE

R.T.: 21.310 min
Delta R.T.: 0.015 min
Response: 533096
Conc: 1.69 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER