

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042520\
 Data File : FE031835.D
 Signal(s) : FID1B.CH
 Acq On : 25 Apr 2020 13:02
 Operator : DD\AJ
 Sample : L2331-07 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 TP-19B

Integration File: autoint1.e
 Quant Time: Apr 27 03:45:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
 Quant Title :
 QLast Update : Tue Apr 07 15:06:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.378	2609097	7.164 ug/ml
Target Compounds			
4) N-TETRADECANE	8.005f	1019827	2.573 ug/ml
7) N-EICOSANE	12.272	1151330	2.735 ug/ml
8) N-DOCOSANE	13.479	471892	1.113 ug/ml
10) N-TETRACOSANE	14.579	4644675	11.096 ug/ml
11) N-HEXACOSANE	15.606	307209	0.741 ug/ml
12) N-OCTACOSANE	16.553	969017	2.355 ug/ml
13) N-TRIACONTANE	17.444	1040902	2.531 ug/ml
14) N-DOTRIACONTANE	18.273	1319329	3.355 ug/ml
15) N-TETRATRIACONTANE	19.059	496208	1.340 ug/ml
16) N-HEXATRIACONTANE	19.798	648466	1.881 ug/ml
17) N-OCTATRIACONTANE	20.501	396582	1.282 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042520\
Data File : FE031835.D
Signal(s) : FID1B.CH
Acq On : 25 Apr 2020 13:02
Operator : DD\AJ
Sample : L2331-07 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TP-19B

Integration File: autoint1.e
Quant Time: Apr 27 03:45:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
Quant Title :
QLast Update : Tue Apr 07 15:06:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

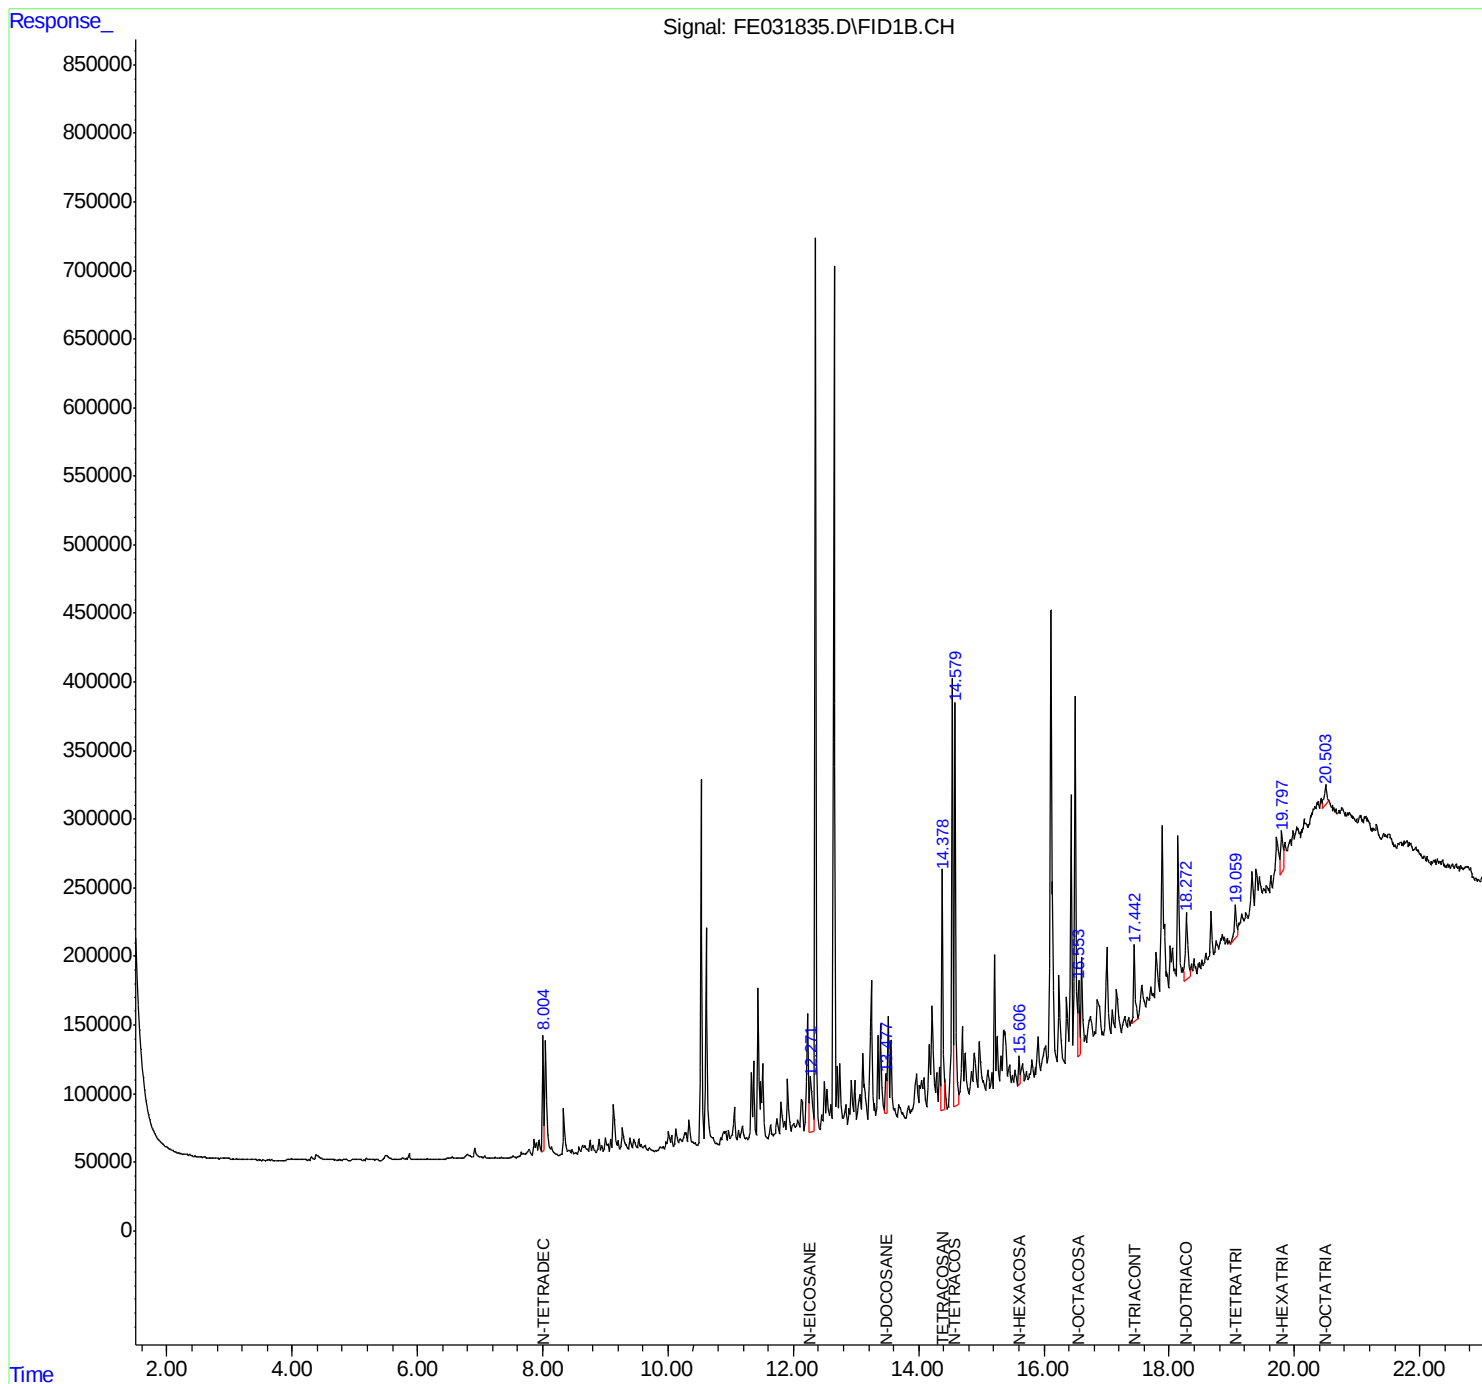


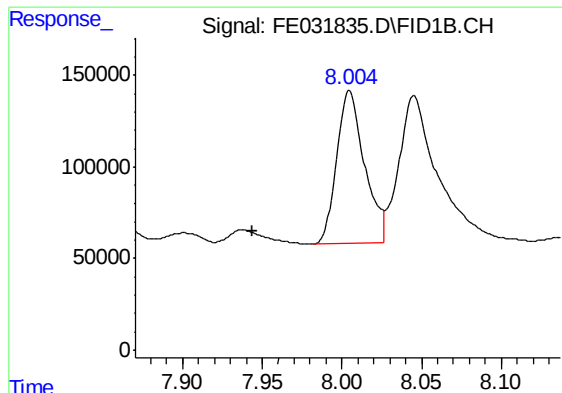

#4 N-TETRADECANE


R.T.: 8.005 min
Delta R.T.: 0.061 min
Response: 1019827
Conc: 2.57 ug/ml

Instrument :
FID_E
ClientSampleId :
TP-19B

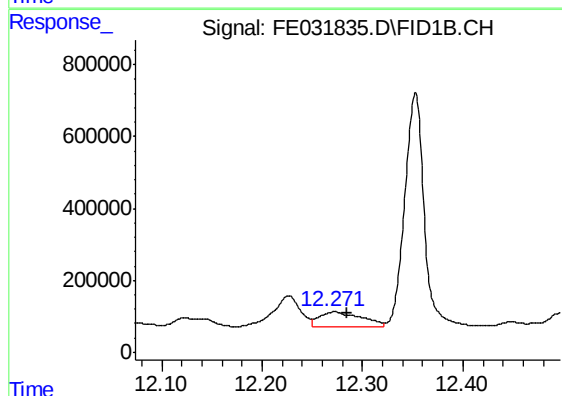


#7 N-EICOSANE

R.T.: 12.272 min
Delta R.T.: -0.013 min
Response: 1151330
Conc: 2.74 ug/ml

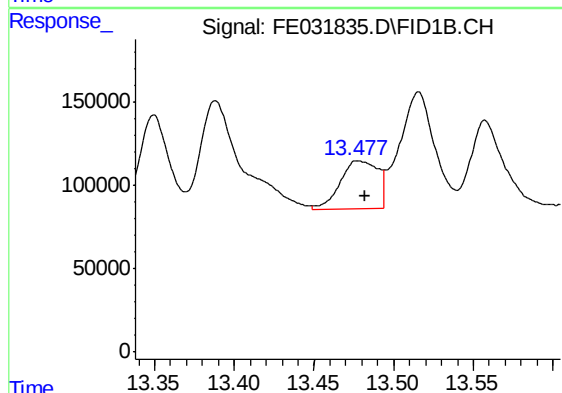


#8 N-DOCOSANE

R.T.: 13.479 min
Delta R.T.: -0.003 min
Response: 471892
Conc: 1.11 ug/ml

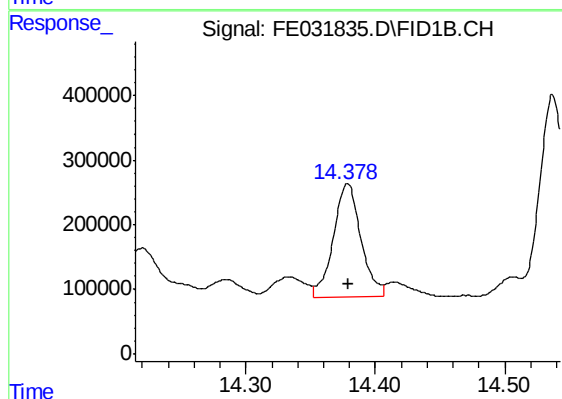

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.378 min
Delta R.T.: -0.001 min
Response: 2609097
Conc: 7.16 ug/ml

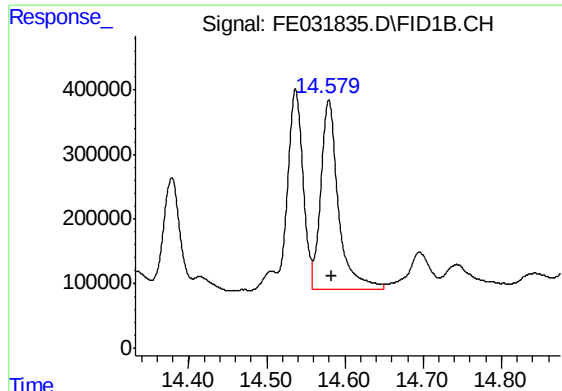

#10 N-TETRACOSANE


R.T.: 14.579 min
Delta R.T.: -0.005 min
Response: 4644675
Conc: 11.10 ug/ml

Instrument :
FID_E
ClientSampleId :
TP-19B

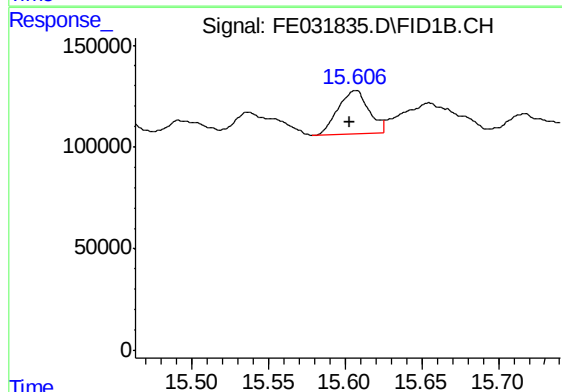


#11 N-HEXACOSANE

R.T.: 15.606 min
Delta R.T.: 0.003 min
Response: 307209
Conc: 0.74 ug/ml

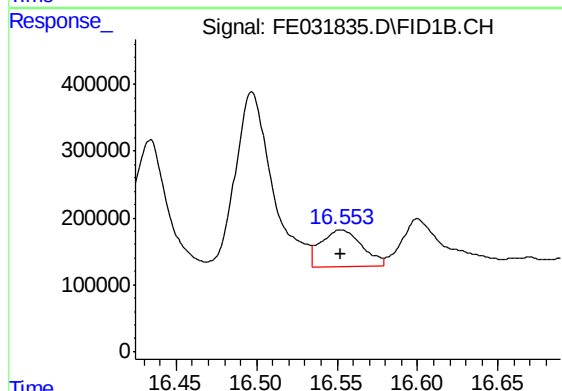


#12 N-OCTACOSANE

R.T.: 16.553 min
Delta R.T.: 0.000 min
Response: 969017
Conc: 2.36 ug/ml

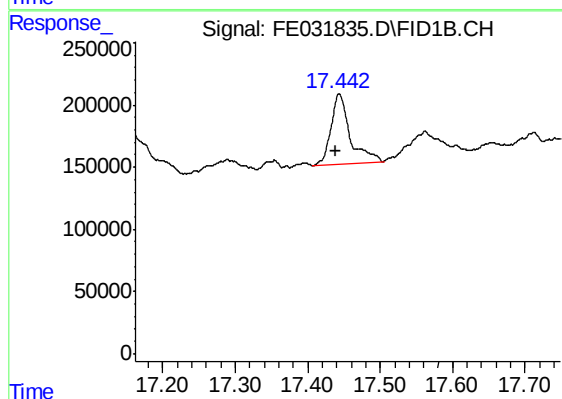

#13 N-TRIACONTANE


R.T.: 17.444 min
Delta R.T.: 0.005 min
Response: 1040902
Conc: 2.53 ug/ml

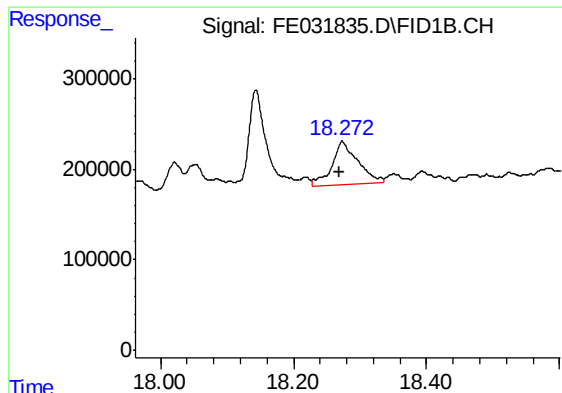

#14 N-DOTRIACONTANE


R.T.: 18.273 min
Delta R.T.: 0.003 min
Response: 1319329
Conc: 3.36 ug/ml

Instrument :
FID_E
ClientSampleId :
TP-19B

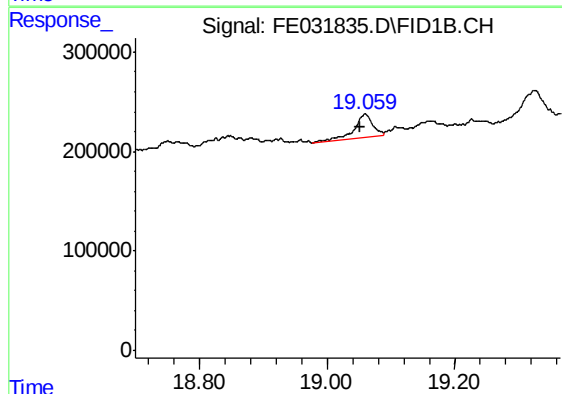


#15 N-TETRATRIACONTANE

R.T.: 19.059 min
Delta R.T.: 0.008 min
Response: 496208
Conc: 1.34 ug/ml

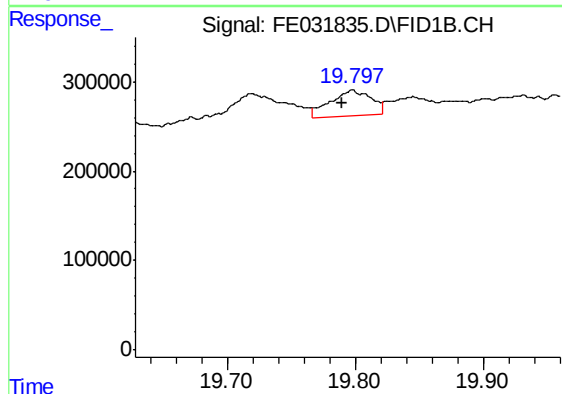

#16 N-HEXATRIACONTANE

R.T.: 19.798 min
Delta R.T.: 0.008 min
Response: 648466
Conc: 1.88 ug/ml

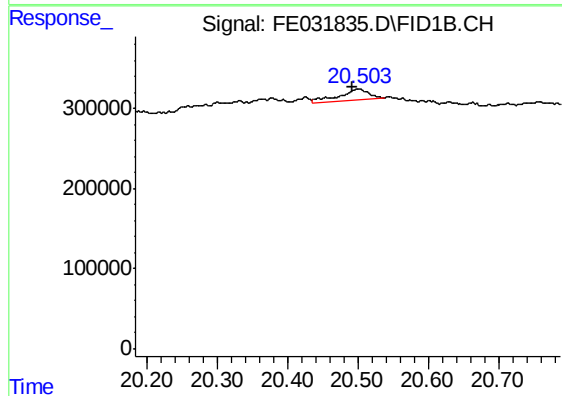

#17 N-OCTATRIACONTANE

R.T.: 20.501 min
Delta R.T.: 0.010 min
Response: 396582
Conc: 1.28 ug/ml