

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042721\
 Data File : FE033657.D
 Signal(s) : FID1B.CH
 Acq On : 27 Apr 2021 18:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Apr 28 06:05:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE042221.M
 Quant Title :
 QLast Update : Fri Apr 23 11:28:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.743	7430429	18.524 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.638	92849	0.230 ug/ml
16) N-HEXATRIACONTANE	20.160	255961	0.731 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE042721\
Data File : FE033657.D
Signal(s) : FID1B.CH
Acq On : 27 Apr 2021 18:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Apr 28 06:05:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE042221.M
Quant Title :
QLast Update : Fri Apr 23 11:28:58 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

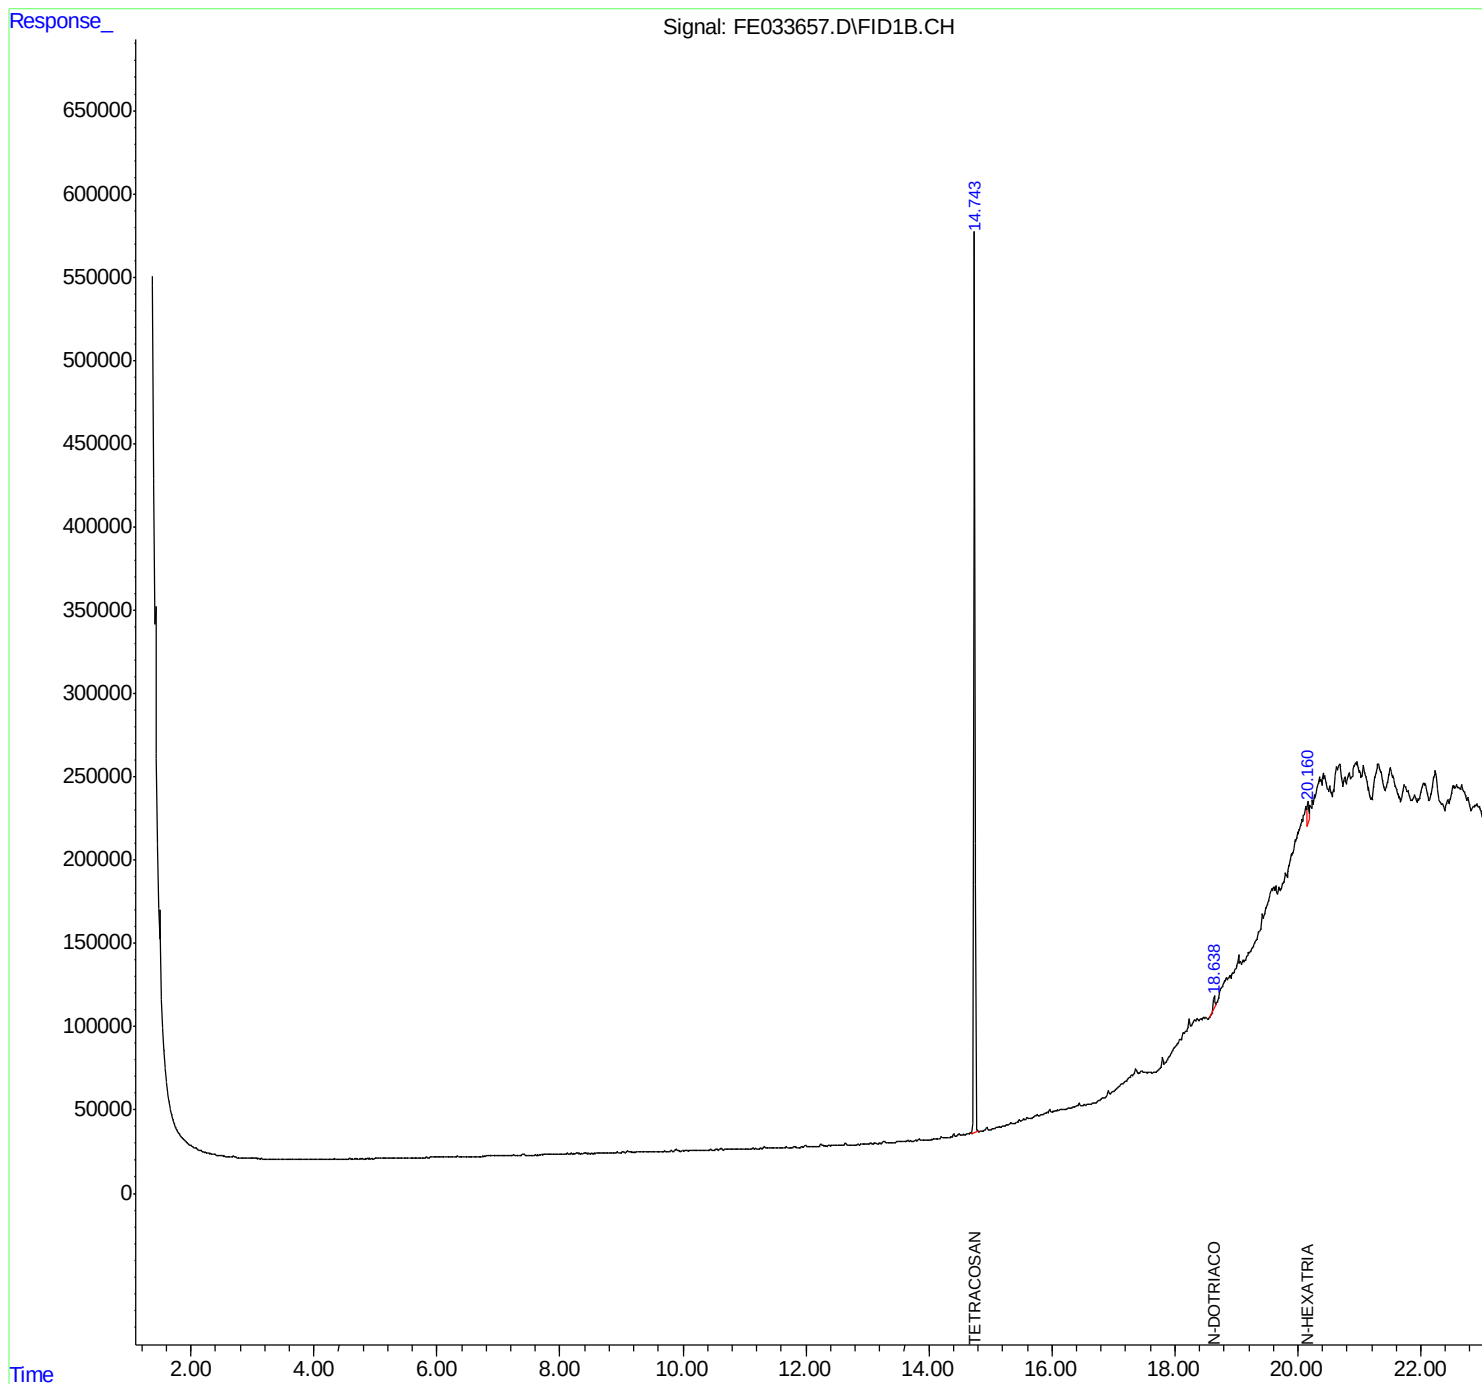


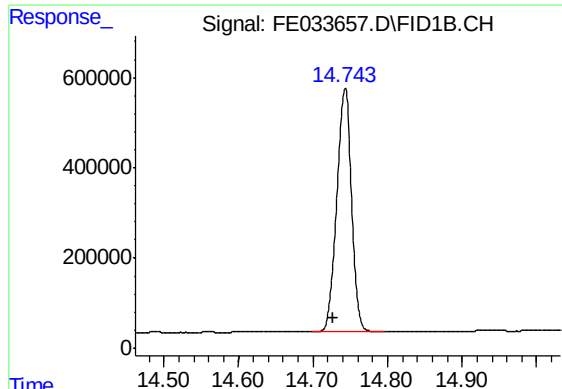

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.743 min
Delta R.T.: 0.016 min
Response: 7430429
Conc: 18.52 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK

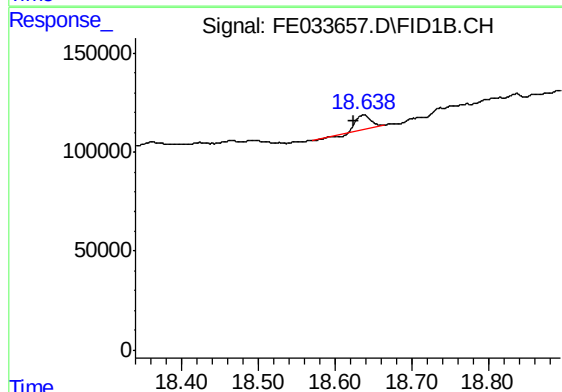

#14 N-DOTRIACONTANE

R.T.: 18.638 min
Delta R.T.: 0.015 min
Response: 92849
Conc: 0.23 ug/ml

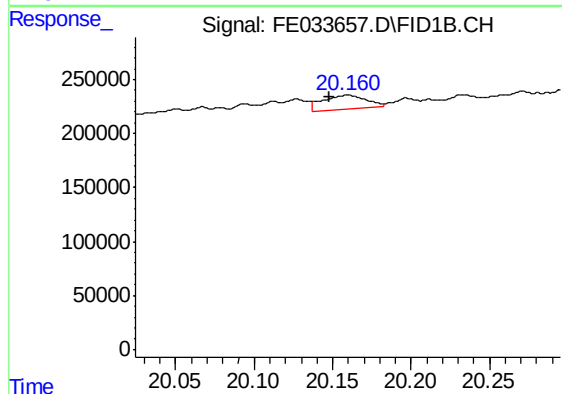

#16 N-HEXATRIACONTANE

R.T.: 20.160 min
Delta R.T.: 0.012 min
Response: 255961
Conc: 0.73 ug/ml