

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042924\
 Data File : PD082651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2024 12:44
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 14:06:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042924.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 29 14:02:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.775	111.2E6	330.6E6	72.626	72.356
28)	SA Decachlor...	9.120	7.906	136.0E6	274.5E6	72.148	72.368
Target Compounds							
23)	Chlordane-1	4.733	3.770	58814063	112.8E6	727.618	728.918
24)	Chlordane-2	5.264	4.345	59856540	126.0E6	732.363	726.185
25)	Chlordane-3	5.977	4.974	248.2E6	375.5E6	738.589	729.350
26)	Chlordane-4	6.058	5.038	291.8E6	355.4E6	737.887	732.778
27)	Chlordane-5	6.912	5.932	49730201	127.5E6	727.931	726.350


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042924\
Data File : PD082651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2024 12:44
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 14:06:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042924.M
Quant Title : GC Extractables
QLast Update : Mon Apr 29 14:02:15 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

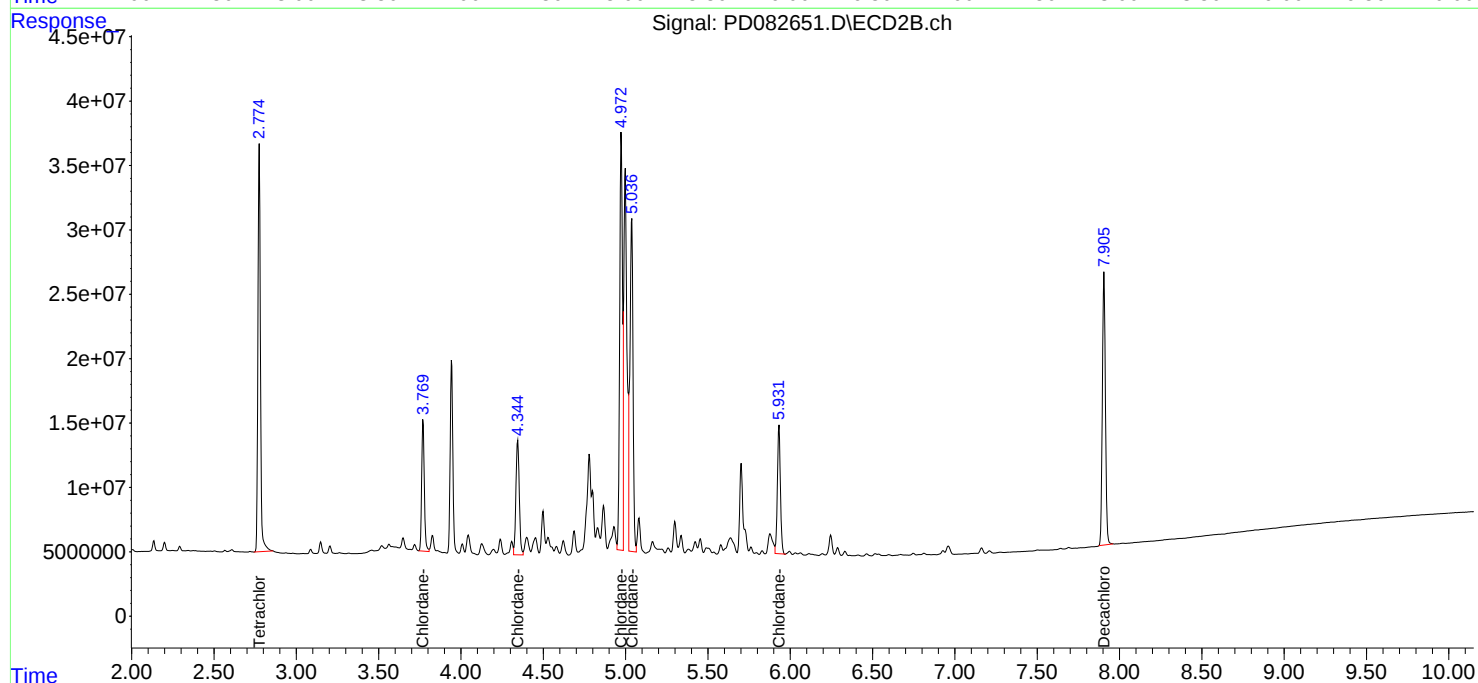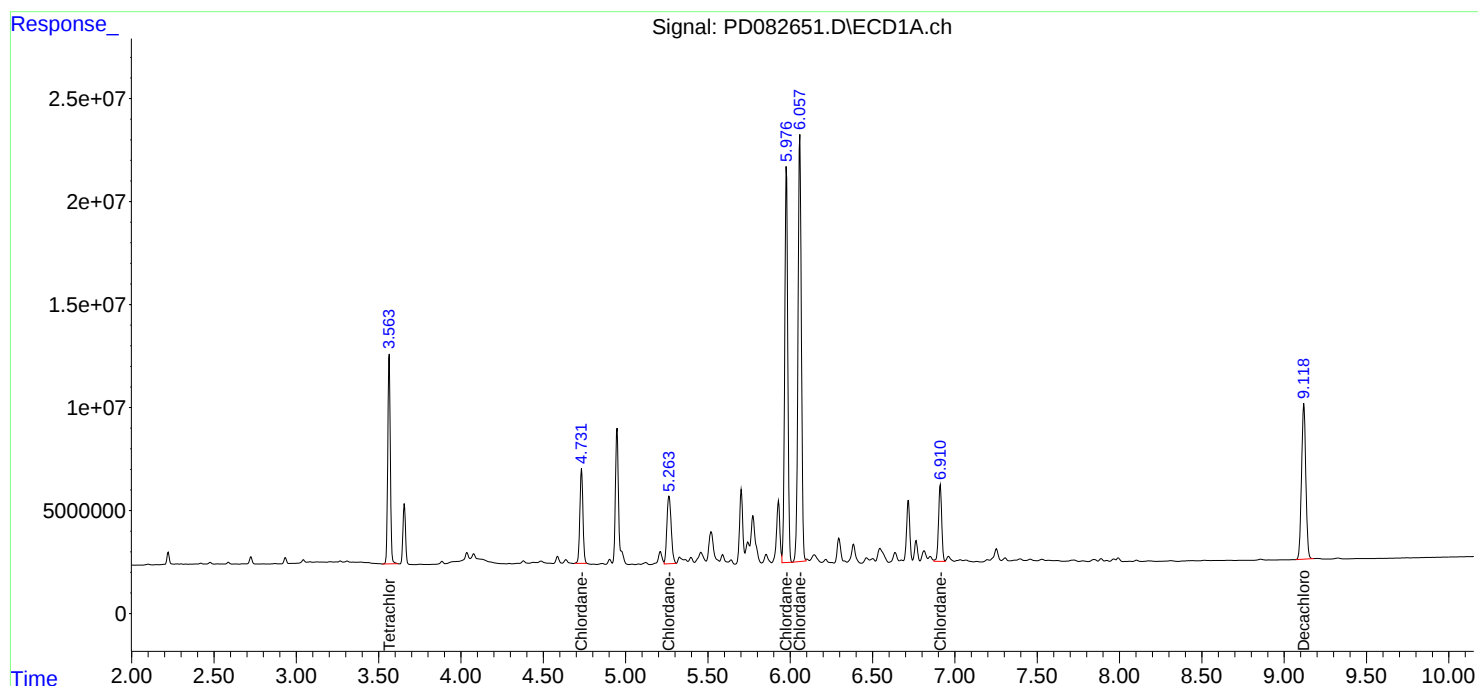

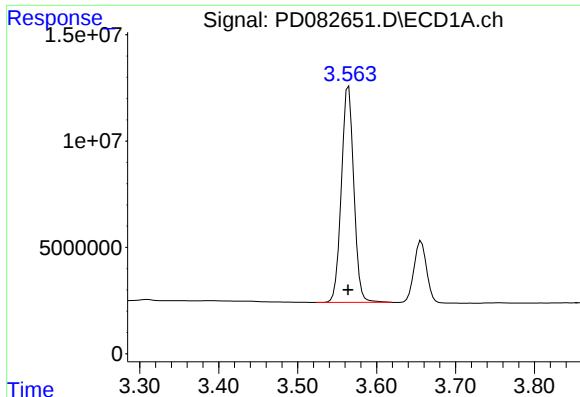


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 111237034
Conc: 72.63 ng/ml

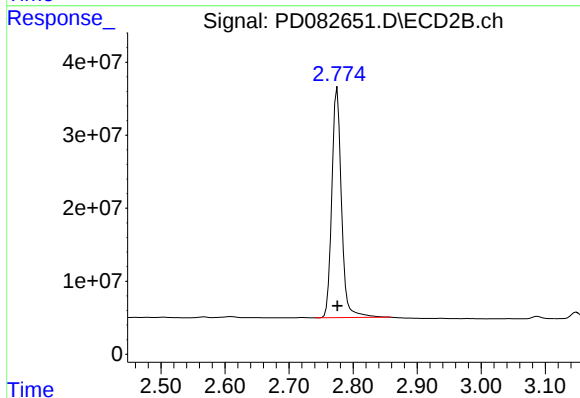


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 330567494
Conc: 72.36 ng/ml

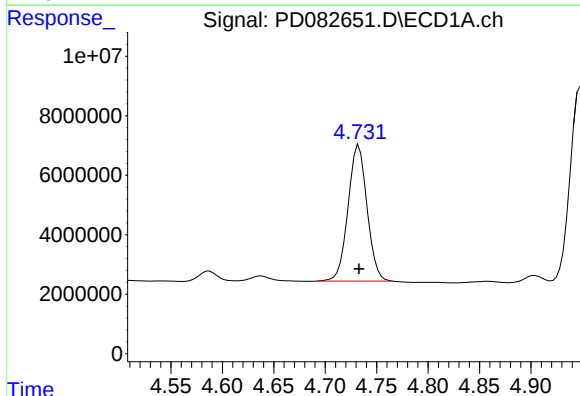


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 58814063
Conc: 727.62 ng/ml

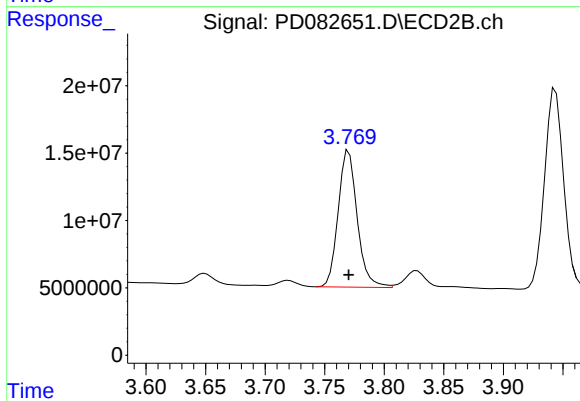


#23 Chlordane-1

R.T.: 3.770 min
Delta R.T.: 0.000 min
Response: 112830241
Conc: 728.92 ng/ml

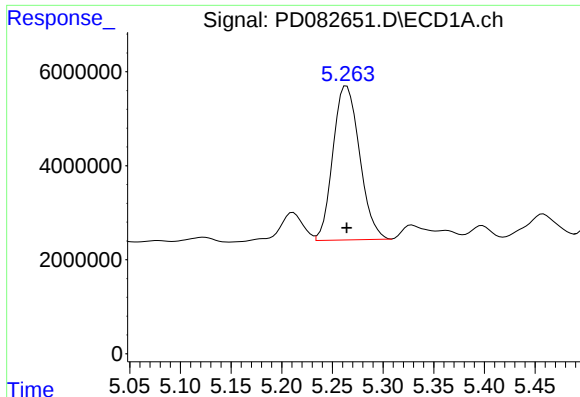


#24 Chlordane-2

R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 59856540
Conc: 732.36 ng/ml

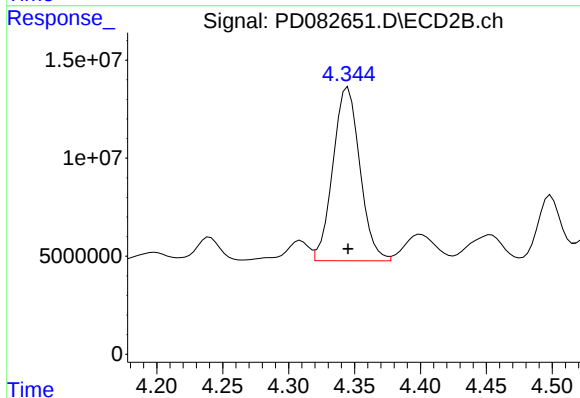


#24 Chlordane-2

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 126023379
Conc: 726.19 ng/ml

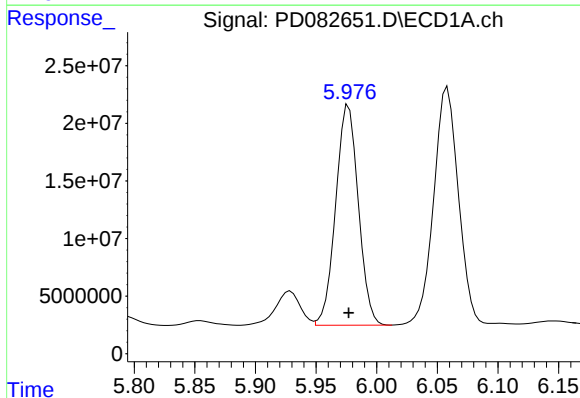


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 248192107
Conc: 738.59 ng/ml

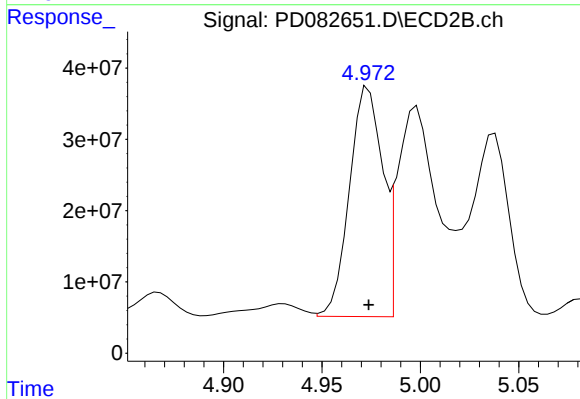


#25 Chlordane-3

R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 375481943
Conc: 729.35 ng/ml

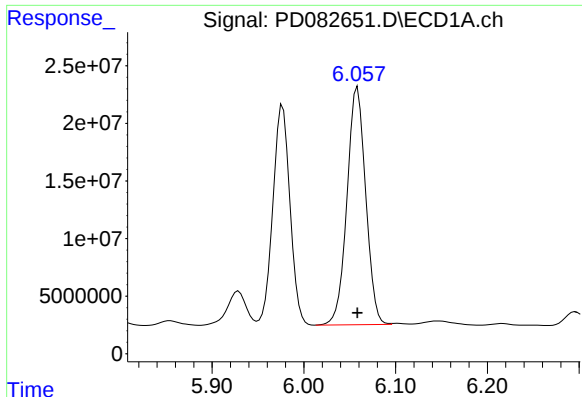


#26 Chlordane-4

R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 291825153
Conc: 737.89 ng/ml

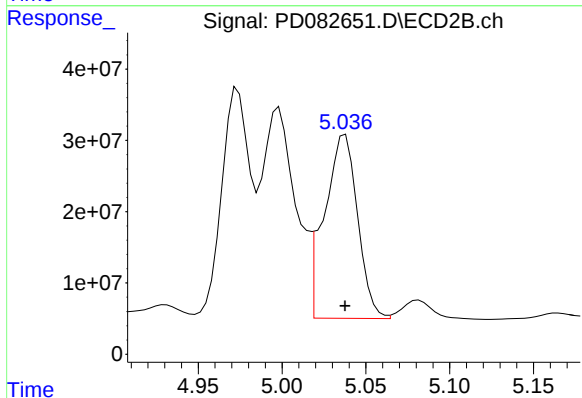


#26 Chlordane-4

R.T.: 5.038 min
Delta R.T.: 0.000 min
Response: 355363791
Conc: 732.78 ng/ml

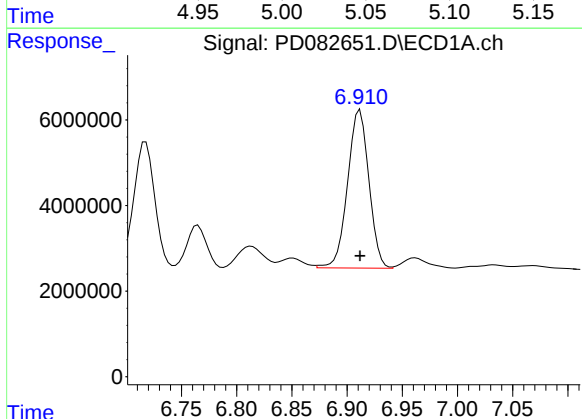


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 49730201
Conc: 727.93 ng/ml

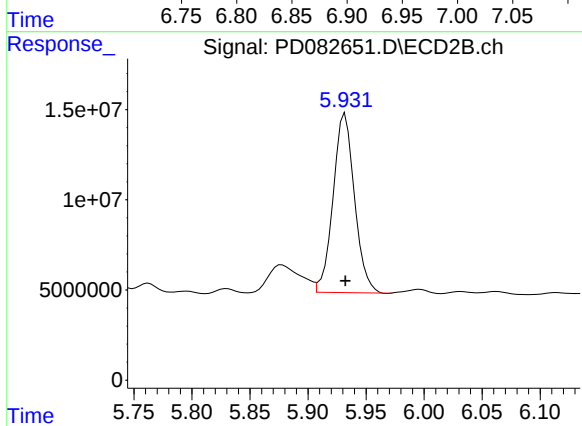


#27 Chlordane-5

R.T.: 5.932 min
Delta R.T.: 0.000 min
Response: 127501584
Conc: 726.35 ng/ml

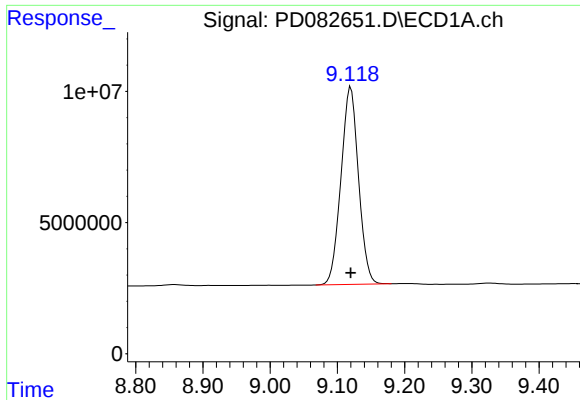

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 135995754
Conc: 72.15 ng/ml

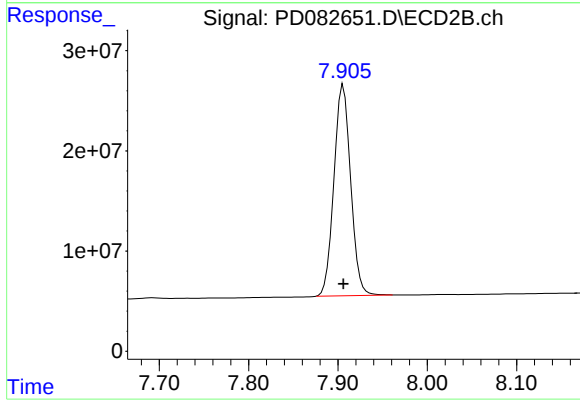

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: 0.000 min
Response: 274536325
Conc: 72.37 ng/ml