

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042924\
 Data File : PD082654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2024 13:24
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 14:10:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042924.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 29 14:02:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.775	8476222	24124683	5.395	5.203
28)	SA Decachlor...	9.119	7.906	11469187	21908821	5.758	5.542
Target Compounds							
23)	Chlordane-1	4.732	3.770	4363941	8363874	52.976	52.774
24)	Chlordane-2	5.264	4.345	4757229	10450752	55.580	57.178
25)	Chlordane-3	5.977	4.973	17443971	26835579	51.490	51.776
26)	Chlordane-4	6.059	5.037	21486017	26225441	53.130	53.196
27)	Chlordane-5	6.912	5.931	3622291	8624532	52.545	49.283


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042924\
Data File : PD082654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2024 13:24
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 14:10:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042924.M
Quant Title : GC Extractables
QLast Update : Mon Apr 29 14:02:15 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

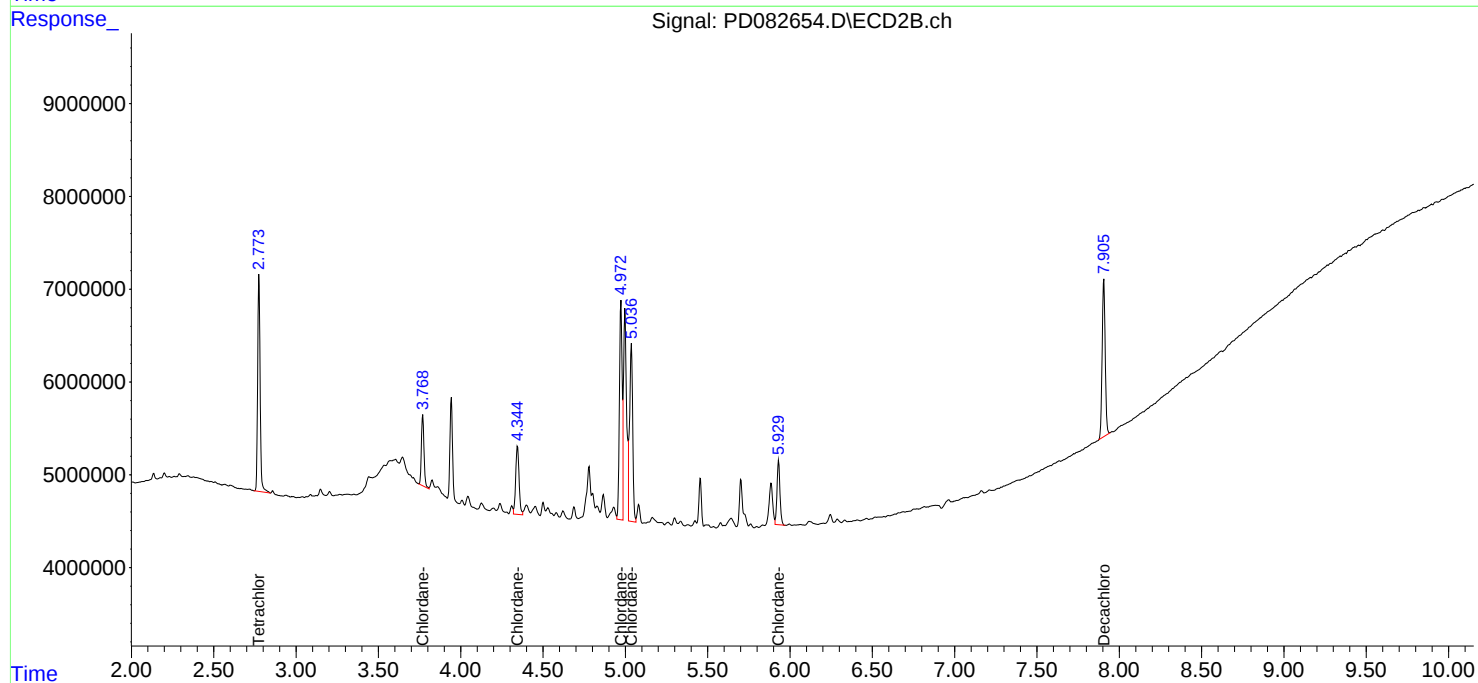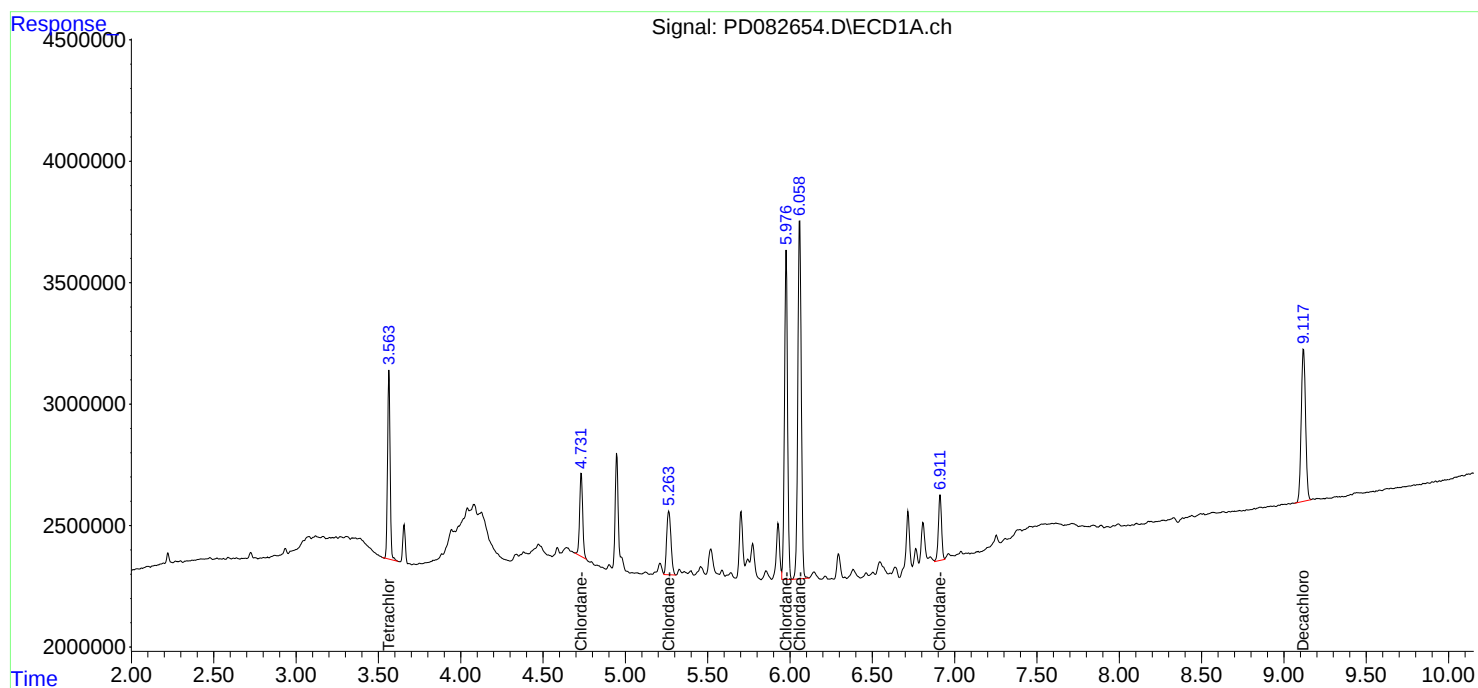

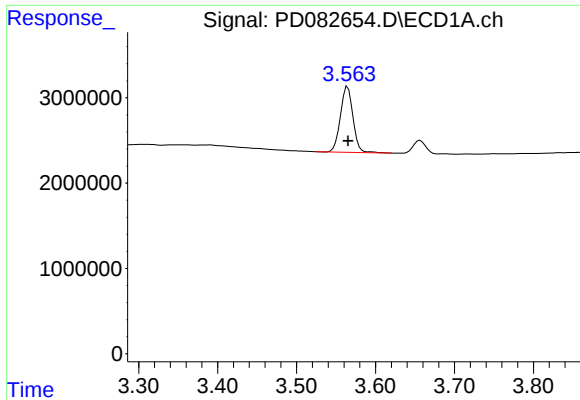


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 8476222
Conc: 5.39 ng/ml

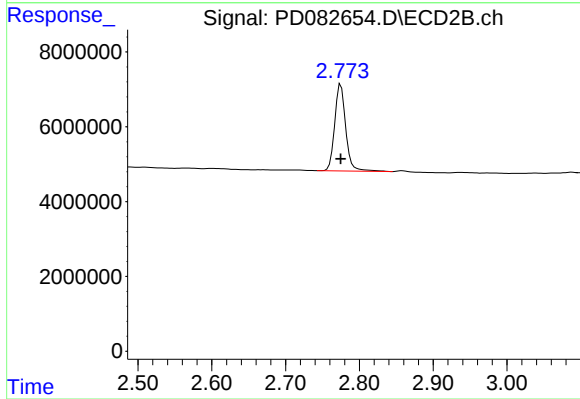


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 24124683
Conc: 5.20 ng/ml

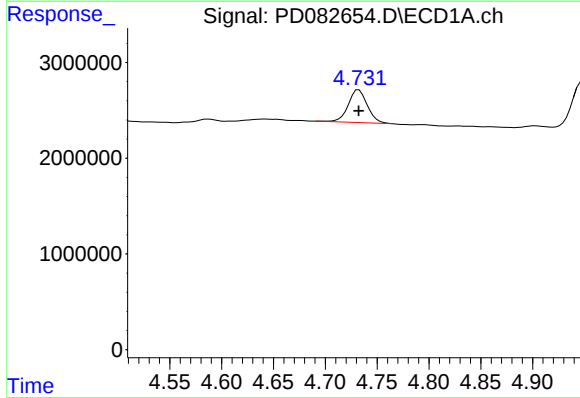


#23 Chlordane-1

R.T.: 4.732 min
Delta R.T.: 0.000 min
Response: 4363941
Conc: 52.98 ng/ml

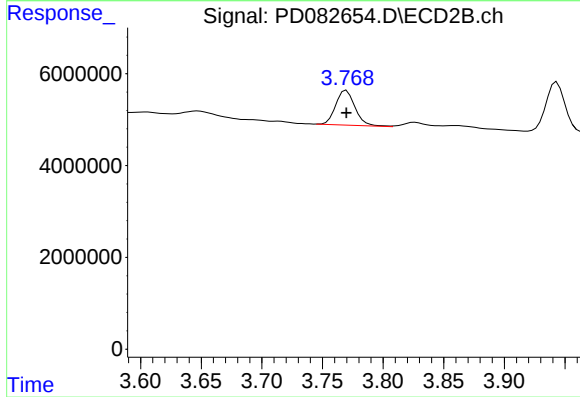


#23 Chlordane-1

R.T.: 3.770 min
Delta R.T.: 0.000 min
Response: 8363874
Conc: 52.77 ng/ml

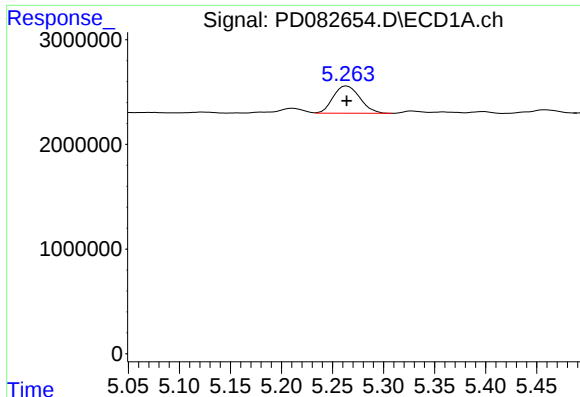


#24 Chlordane-2

R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 4757229
Conc: 55.58 ng/ml

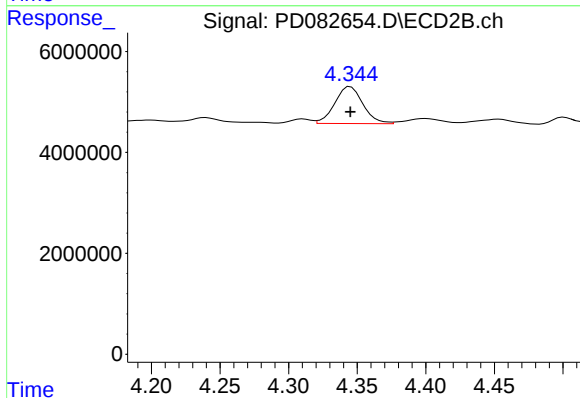


#24 Chlordane-2

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 10450752
Conc: 57.18 ng/ml

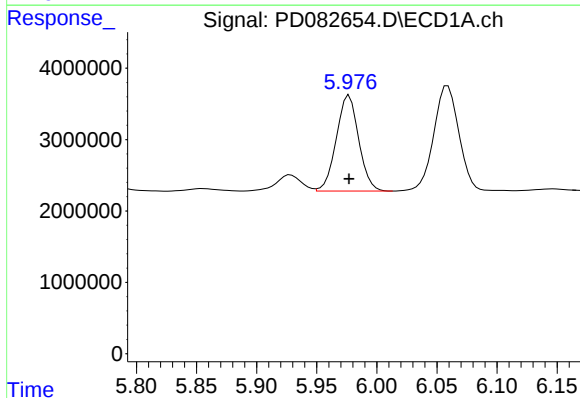


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 17443971
Conc: 51.49 ng/ml

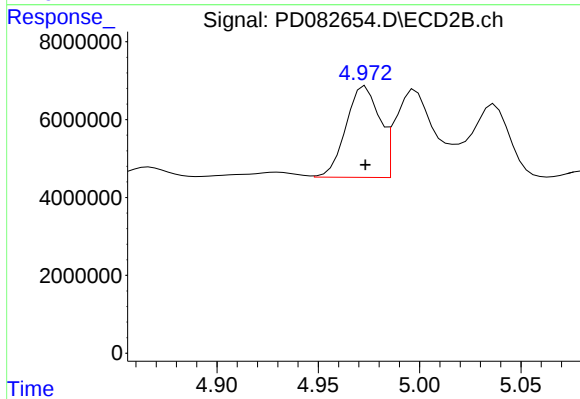


#25 Chlordane-3

R.T.: 4.973 min
Delta R.T.: 0.000 min
Response: 26835579
Conc: 51.78 ng/ml

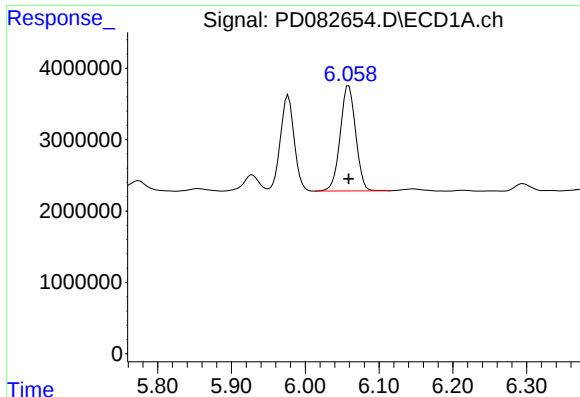


#26 Chlordane-4

R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 21486017
Conc: 53.13 ng/ml

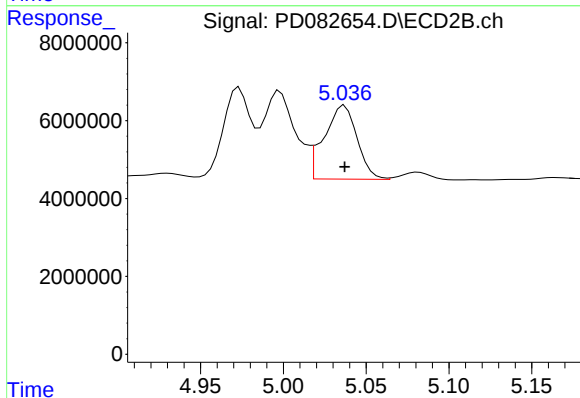


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 26225441
Conc: 53.20 ng/ml

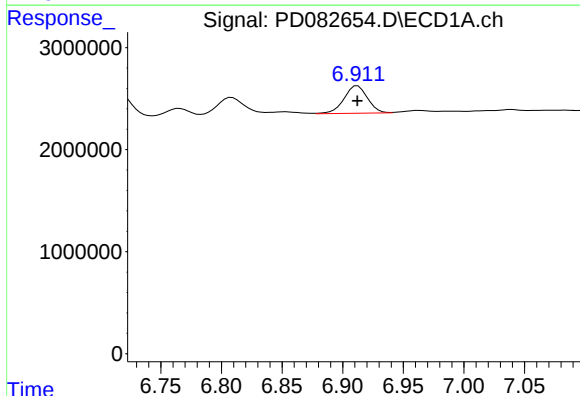


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 3622291
Conc: 52.55 ng/ml

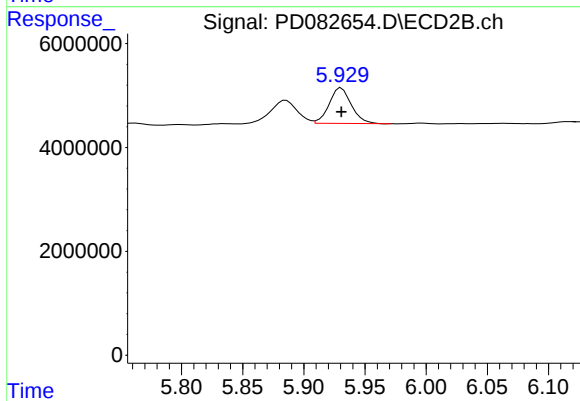


#27 Chlordane-5

R.T.: 5.931 min
Delta R.T.: 0.000 min
Response: 8624532
Conc: 49.28 ng/ml

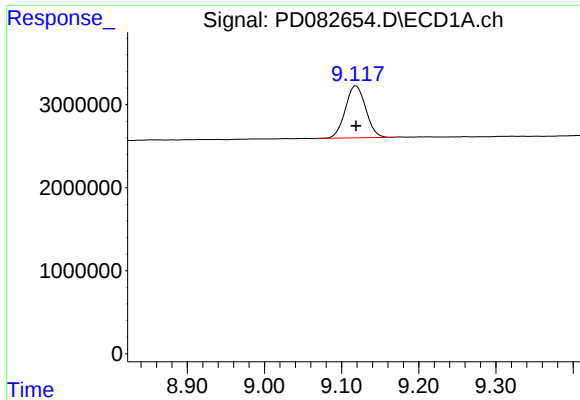

#28 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 11469187
Conc: 5.76 ng/ml

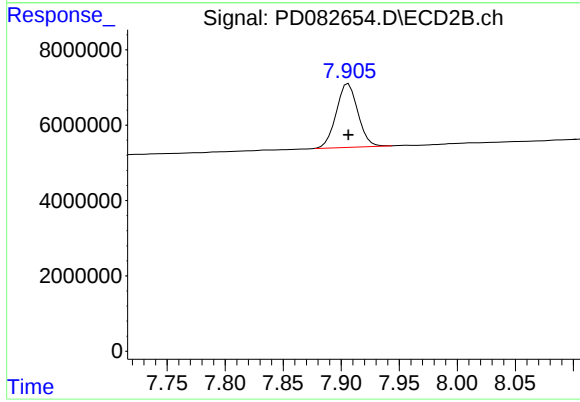

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: 0.000 min
Response: 21908821
Conc: 5.54 ng/ml