

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050120\
 Data File : FE031864.D
 Signal(s) : FID1B.CH
 Acq On : 01 May 2020 19:34
 Operator : DD\AJ
 Sample : PB128599BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 PB128599BL

Integration File: autoint1.e
 Quant Time: May 02 00:54:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
 Quant Title :
 QLast Update : Tue Apr 07 15:06:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.376	6628634	18.201 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.433	185087	0.450 ug/ml
14) N-DOTRIACONTANE	18.265	261442	0.665 ug/ml
15) N-TETRATRIACONTANE	19.051	195268	0.527 ug/ml
16) N-HEXATRIACONTANE	19.790	775718	2.250 ug/ml
17) N-OCTATRIACONTANE	20.495	2762060	8.931 ug/ml
18) N-TETRACONTANE	21.301	298420	0.944 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050120\
Data File : FE031864.D
Signal(s) : FID1B.CH
Acq On : 01 May 2020 19:34
Operator : DD\AJ
Sample : PB128599BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB128599BL

Integration File: autoint1.e
Quant Time: May 02 00:54:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
Quant Title :
QLast Update : Tue Apr 07 15:06:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

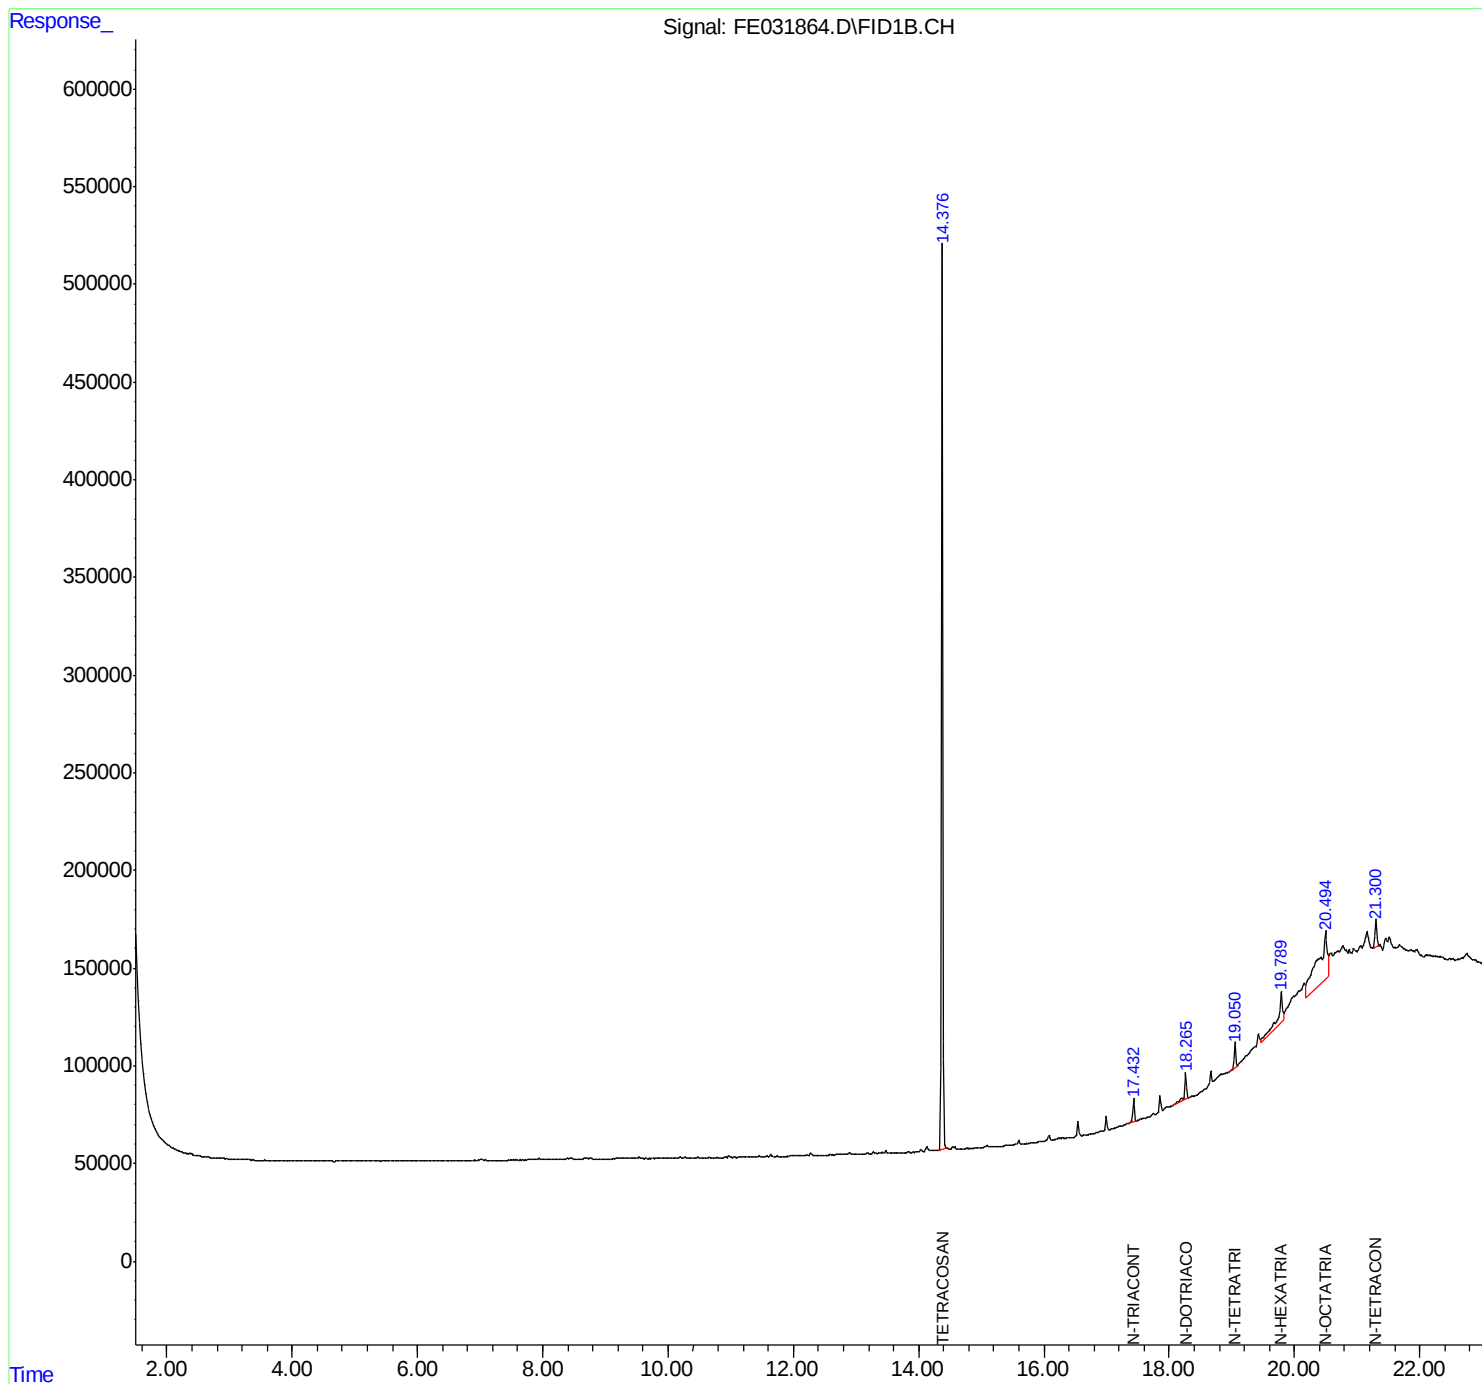


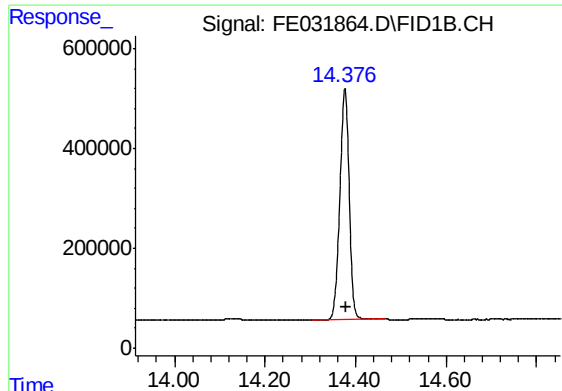

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.376 min
Delta R.T.: -0.003 min
Response: 6628634
Conc: 18.20 ug/ml

Instrument :
FID_E
ClientSampleId :
PB128599BL

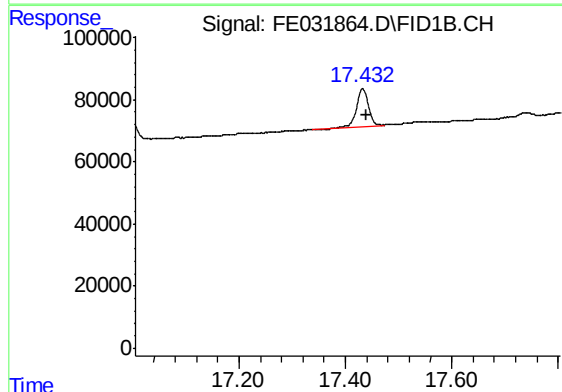


#13 N-TRIACONTANE

R.T.: 17.433 min
Delta R.T.: -0.006 min
Response: 185087
Conc: 0.45 ug/ml

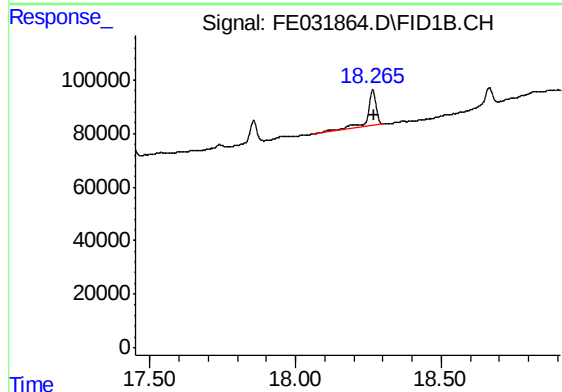


#14 N-DOTRIACONTANE

R.T.: 18.265 min
Delta R.T.: -0.005 min
Response: 261442
Conc: 0.66 ug/ml

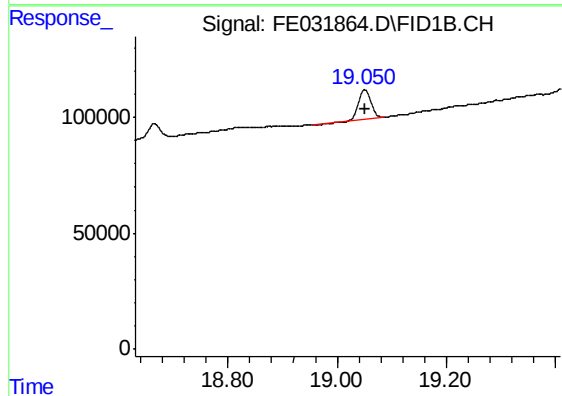

#15 N-TETRATRIACONTANE


R.T.: 19.051 min
Delta R.T.: 0.000 min
Response: 195268
Conc: 0.53 ug/ml

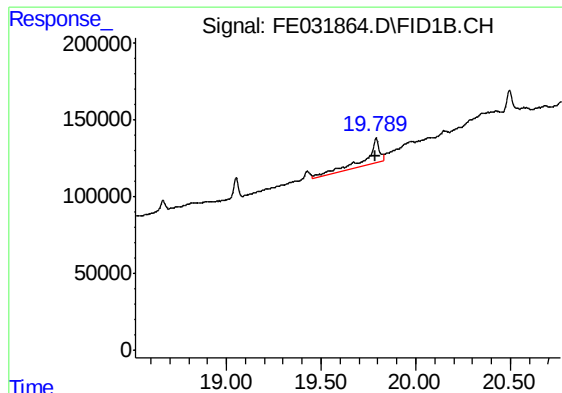

#16 N-HEXATRIACONTANE


R.T.: 19.790 min
Delta R.T.: 0.000 min
Response: 775718
Conc: 2.25 ug/ml

Instrument :
FID_E
ClientSampleId :
PB128599BL

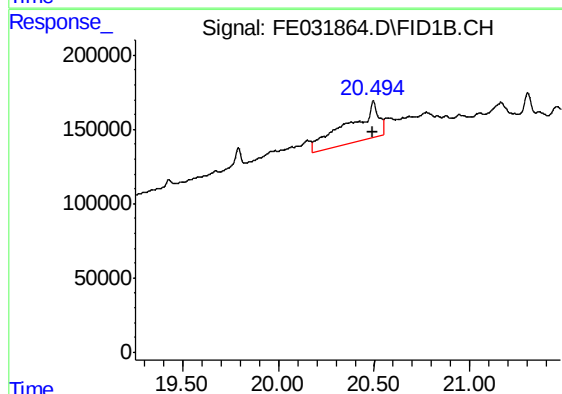

#17 N-OCTATRIACONTANE

R.T.: 20.495 min
Delta R.T.: 0.004 min
Response: 2762060
Conc: 8.93 ug/ml

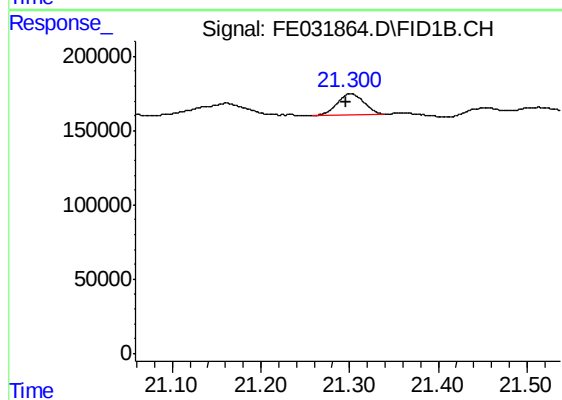

#18 N-TETRACONTANE

R.T.: 21.301 min
Delta R.T.: 0.006 min
Response: 298420
Conc: 0.94 ug/ml