

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050123AL\
 Data File : FE041622.D
 Signal(s) : FID1B.ch
 Acq On : 01 May 2023 08:14
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 01 12:08:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 07:33:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	18.144	35579	0.234 ug/ml
18) T	n-Dotriacontane (C32)	18.938	8042	0.054 ug/ml
19) T	n-Tetratriacontane (C34)	19.743	168231	1.194 ug/ml
20) T	n-Hexatriacontane (C36)	20.518	70839	0.530 ug/ml
21) T	n-Octatriacontane (C38)	21.196	132312	1.001 ug/ml
22) T	n-Tetracontane (C40)	22.155	46034	0.364 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050123AL\
Data File : FE041622.D
Signal(s) : FID1B.ch
Acq On : 01 May 2023 08:14
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 01 12:08:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

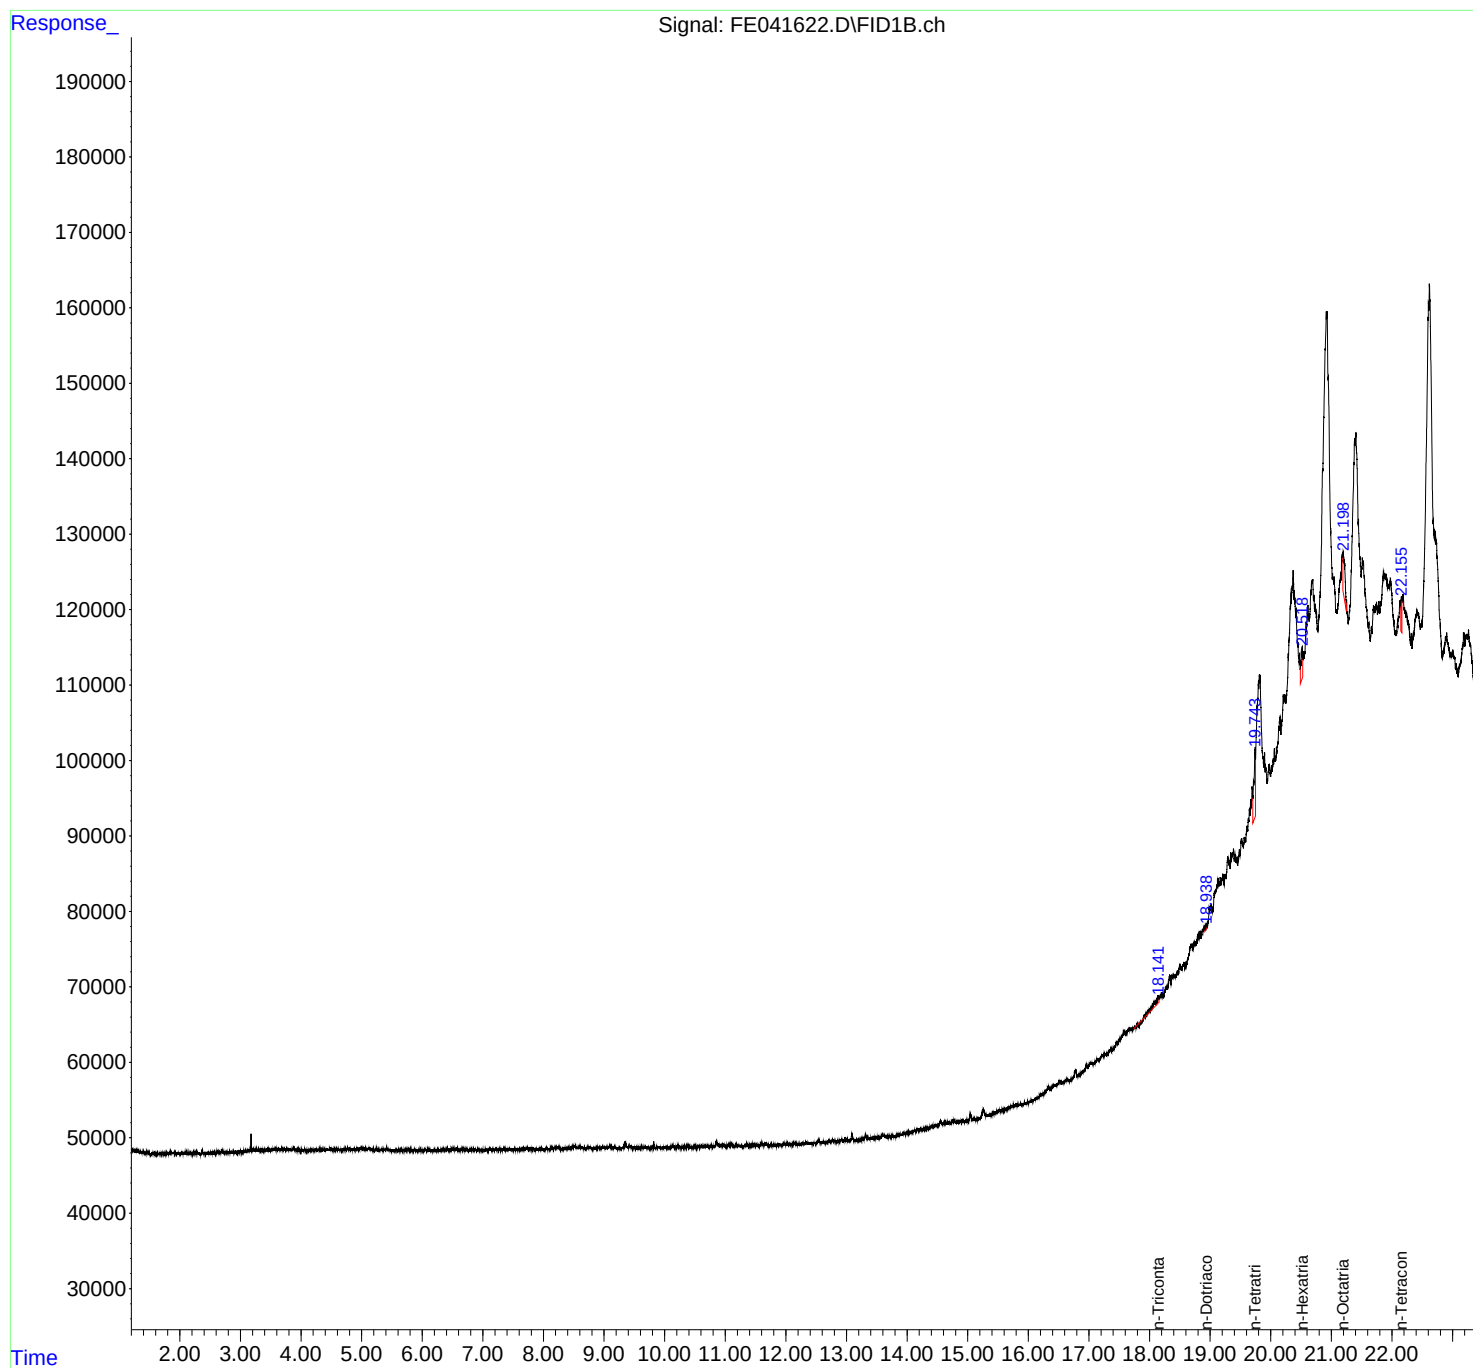


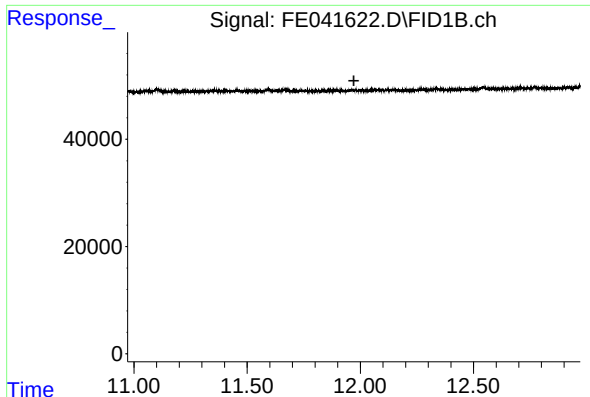

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.972 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

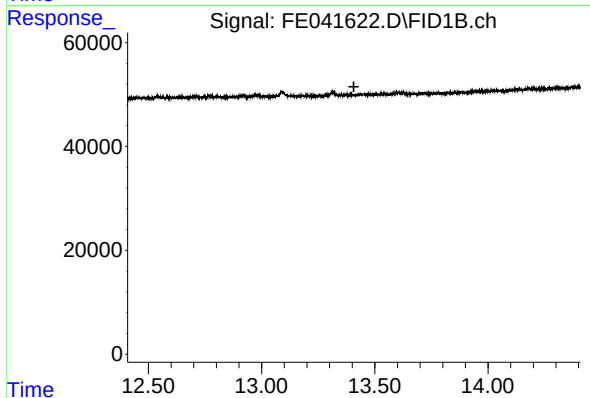


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.408 min
Response: 0
Conc: N.D.

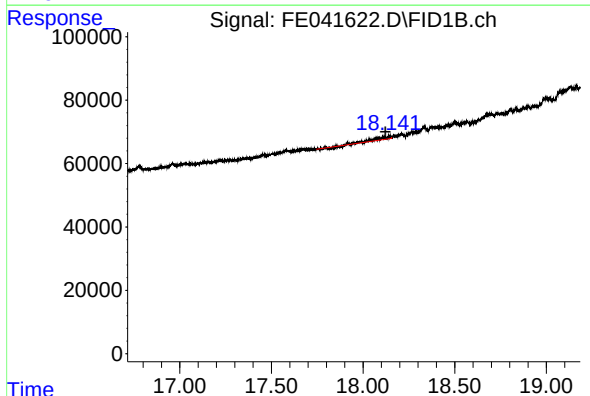


#17 n-Tricontane (C30)

R.T.: 18.144 min
Delta R.T.: 0.023 min
Response: 35579
Conc: 0.23 ug/ml

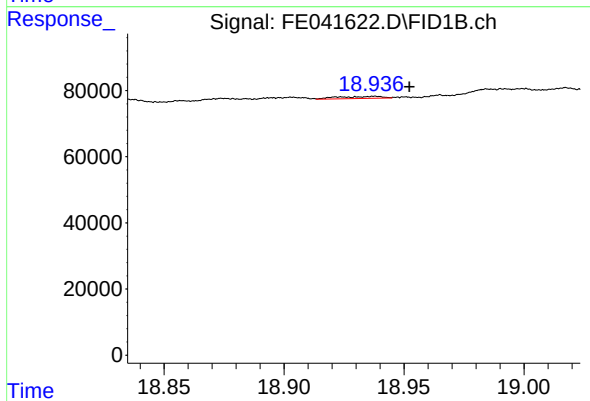

#18 n-Dotriacontane (C32)


R.T.: 18.938 min
Delta R.T.: -0.014 min
Response: 8042
Conc: 0.05 ug/ml

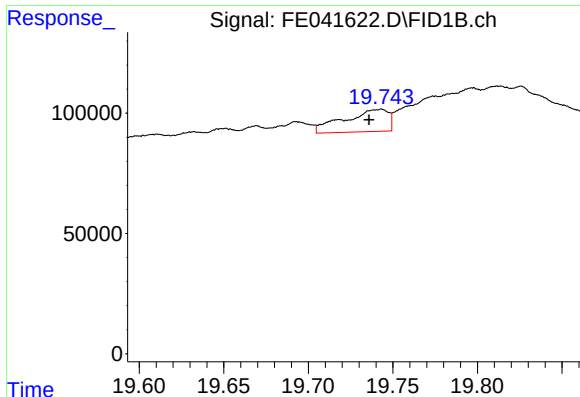

#19 n-Tetratriacontane (C34)


R.T.: 19.743 min
Delta R.T.: 0.007 min
Response: 168231
Conc: 1.19 ug/ml

Instrument :
FID_E
ClientSampleId :

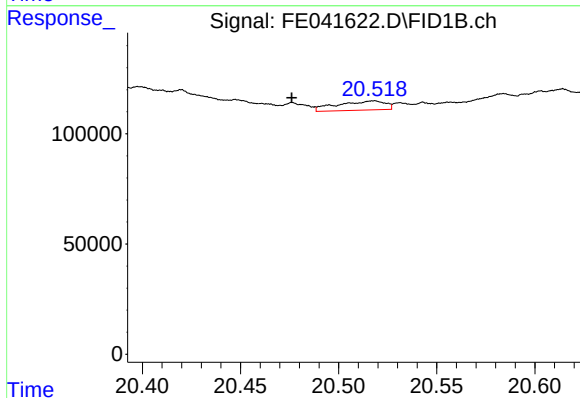


#20 n-Hexatriacontane (C36)

R.T.: 20.518 min
Delta R.T.: 0.042 min
Response: 70839
Conc: 0.53 ug/ml

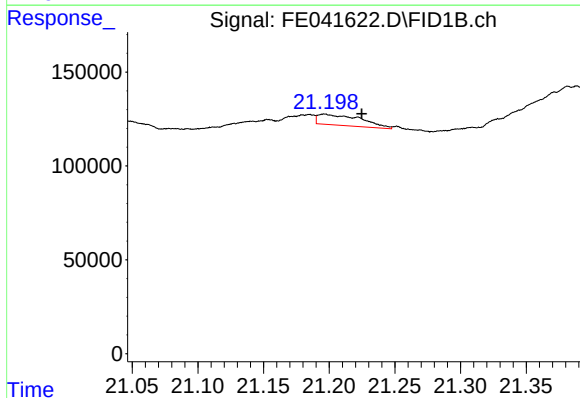

#21 n-Octatriacontane (C38)

R.T.: 21.196 min
Delta R.T.: -0.028 min
Response: 132312
Conc: 1.00 ug/ml

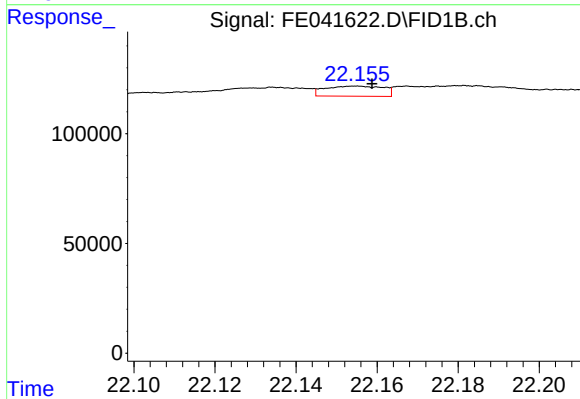

#22 n-Tetracontane (C40)

R.T.: 22.155 min
Delta R.T.: -0.004 min
Response: 46034
Conc: 0.36 ug/ml