

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050123AL\
 Data File : FE041659.D
 Signal(s) : FID1B.ch
 Acq On : 02 May 2023 06:54
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 02 07:51:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 07:33:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) T n-Octacosane (C28)	17.252	21920	0.142 ug/ml
17) T n-Tricontane (C30)	18.142	19438	0.128 ug/ml
18) T n-Dotriacontane (C32)	18.976	51365	0.345 ug/ml
19) T n-Tetratriacontane (C34)	19.753	33405	0.237 ug/ml
20) T n-Hexatriacontane (C36)	20.497	46291	0.346 ug/ml
21) T n-Octatriacontane (C38)	21.209	95830	0.725 ug/ml
22) T n-Tetracontane (C40)	22.194	23199	0.183 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050123AL\
Data File : FE041659.D
Signal(s) : FID1B.ch
Acq On : 02 May 2023 06:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 02 07:51:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

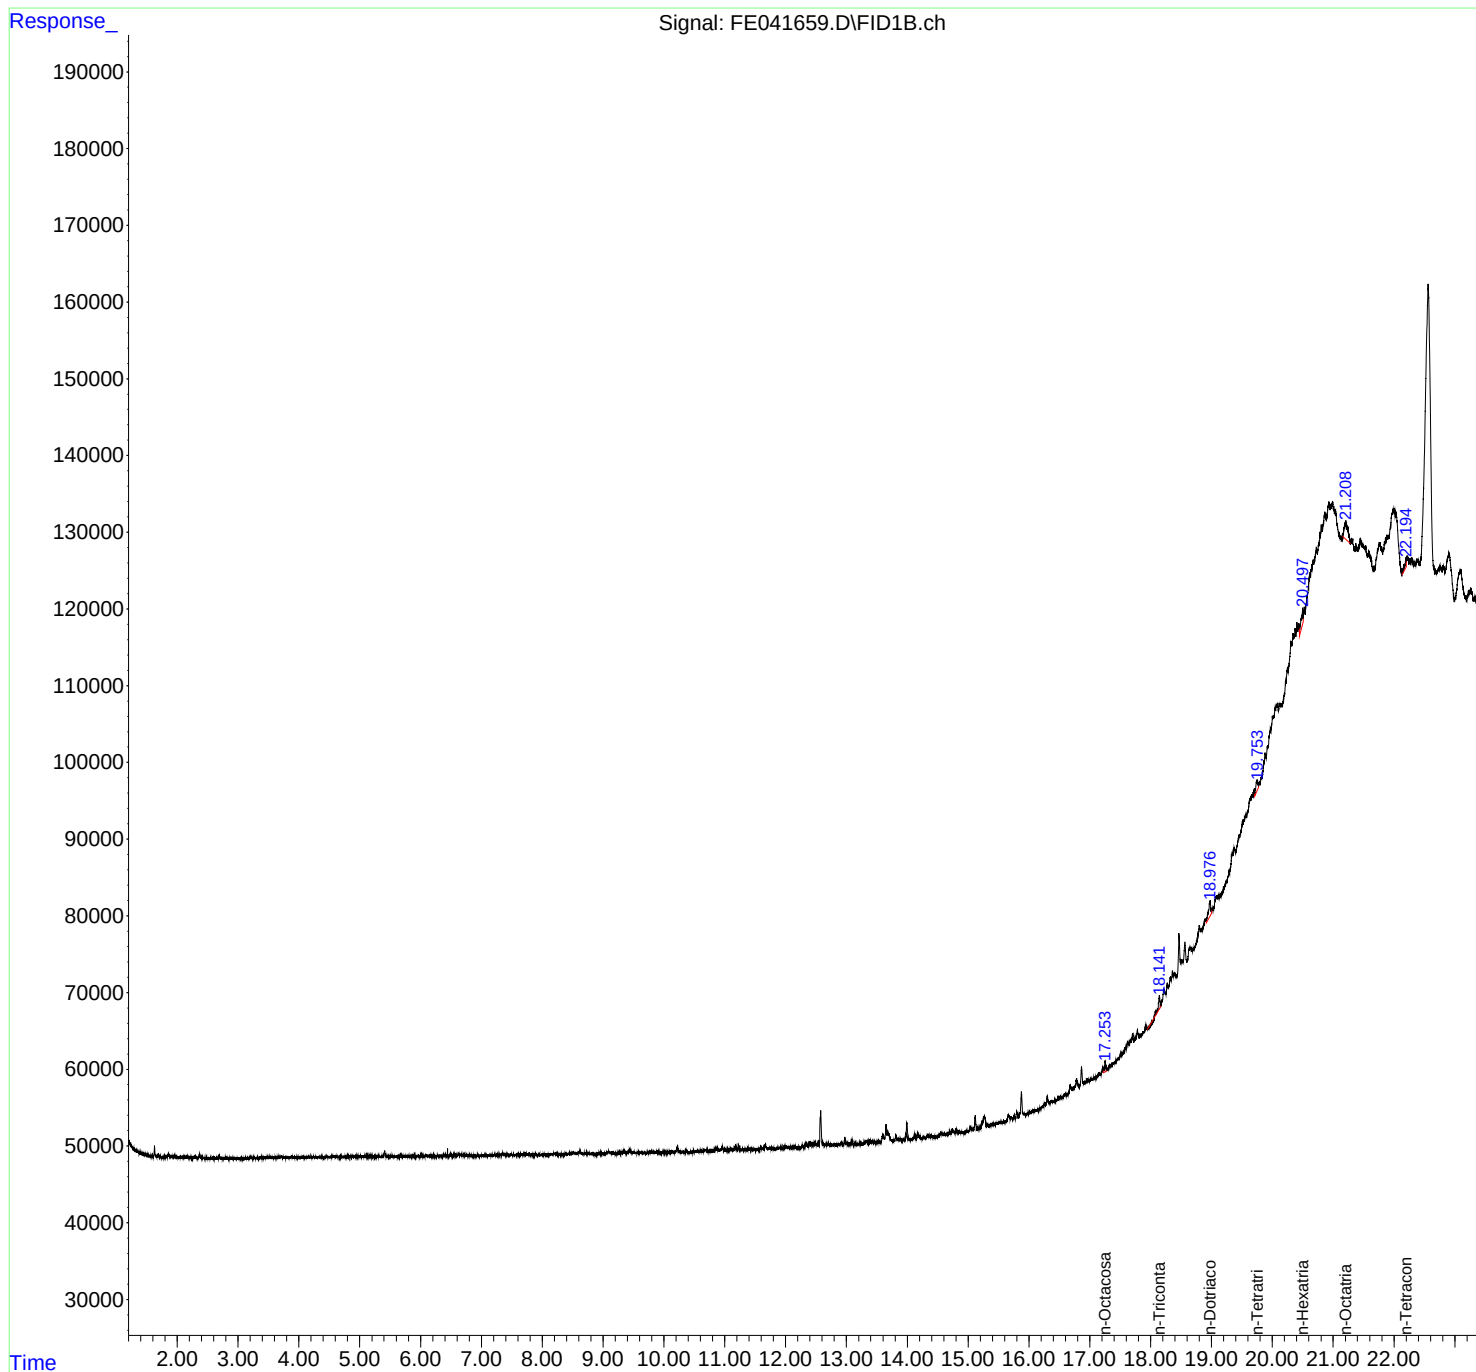


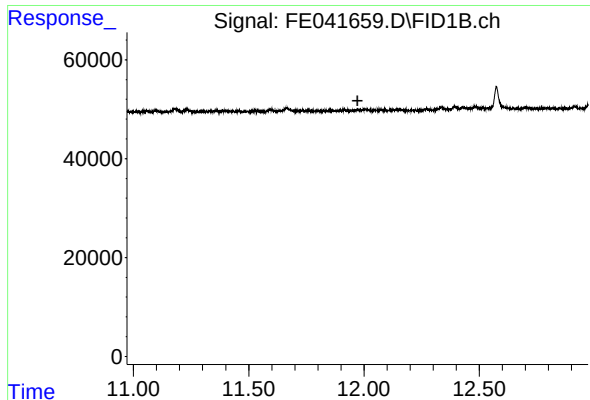

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.972 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

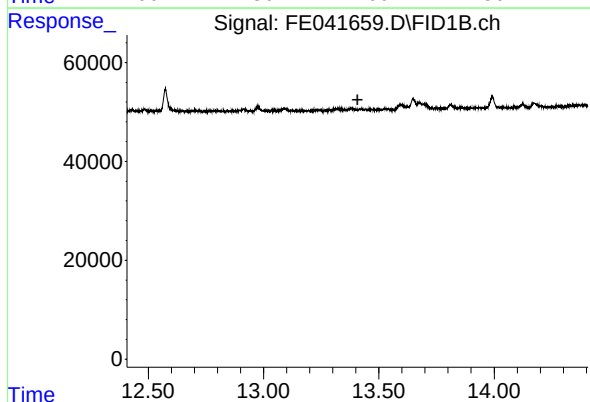


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.408 min
Response: 0
Conc: N.D.

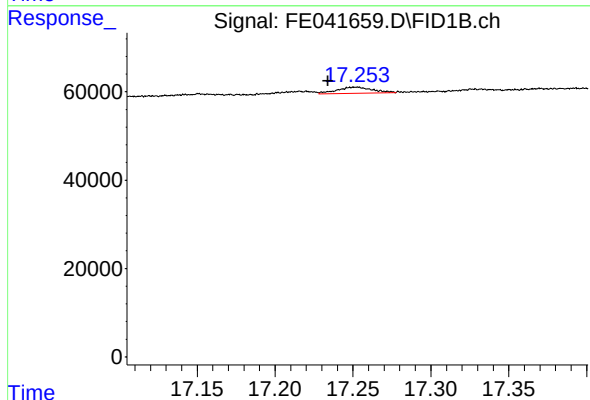


#16 n-Octacosane (C28)

R.T.: 17.252 min
Delta R.T.: 0.018 min
Response: 21920
Conc: 0.14 ug/ml

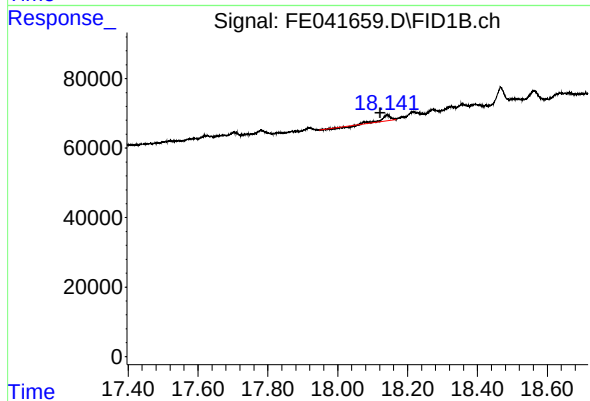

#17 n-Tricontane (C30)


R.T.: 18.142 min
Delta R.T.: 0.021 min
Response: 19438
Conc: 0.13 ug/ml

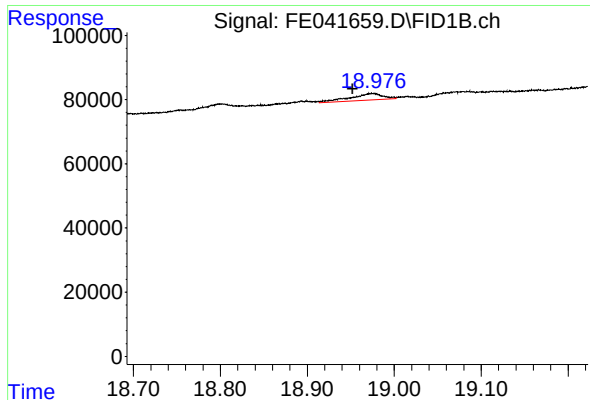

#18 n-Dotriacontane (C32)


R.T.: 18.976 min
Delta R.T.: 0.024 min
Response: 51365
Conc: 0.34 ug/ml

Instrument :
FID_E
ClientSampleId :

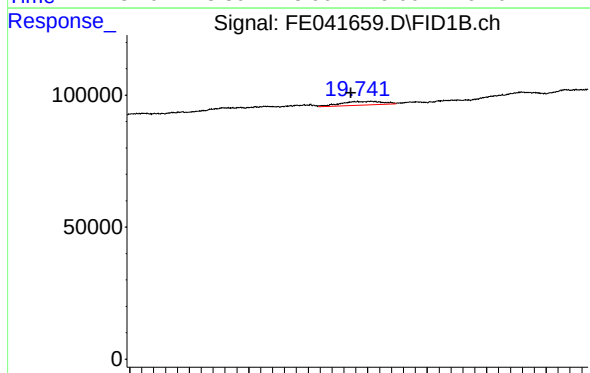


#19 n-Tetratriacontane (C34)

R.T.: 19.753 min
Delta R.T.: 0.017 min
Response: 33405
Conc: 0.24 ug/ml

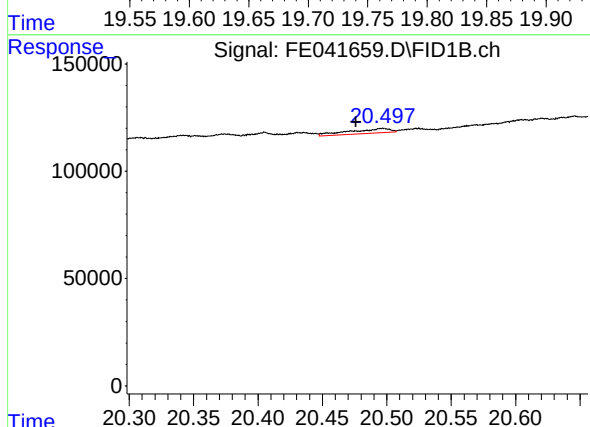


#20 n-Hexatriacontane (C36)

R.T.: 20.497 min
Delta R.T.: 0.021 min
Response: 46291
Conc: 0.35 ug/ml

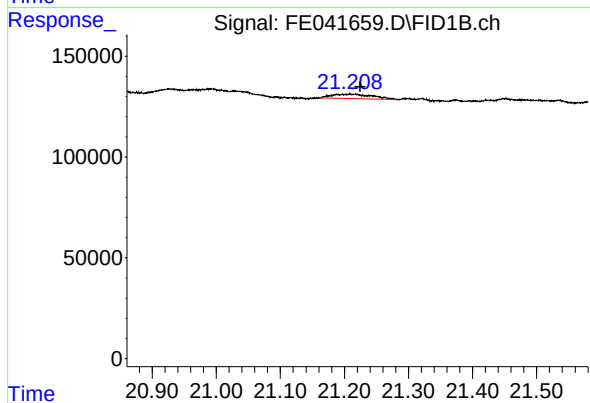

#21 n-Octatriacontane (C38)

R.T.: 21.209 min
Delta R.T.: -0.016 min
Response: 95830
Conc: 0.73 ug/ml

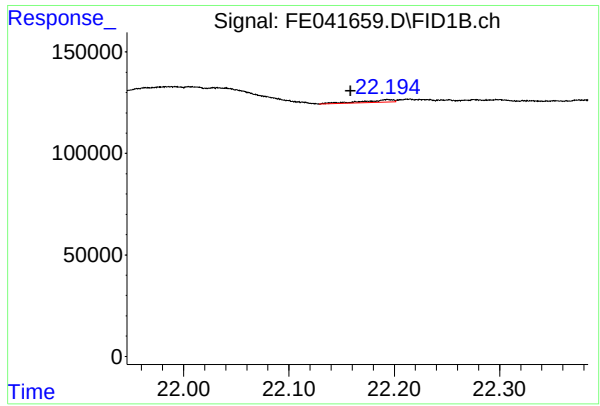

#22 n-Tetracontane (C40)

R.T.: 22.194 min
Delta R.T.: 0.035 min
Response: 23199
Conc: 0.18 ug/ml

Instrument :

FID_E

ClientSampleId :