

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050223AL\
 Data File : FE041691.D
 Signal(s) : FID1B.ch
 Acq On : 03 May 2023 01:08
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 03 02:59:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 07:33:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	18.137	26197	0.172 ug/ml
18) T n-Dotriacontane (C32)	18.965	32892	0.221 ug/ml
19) T n-Tetratriacontane (C34)	19.752	7399	0.053 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050223AL\
Data File : FE041691.D
Signal(s) : FID1B.ch
Acq On : 03 May 2023 01:08
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 03 02:59:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

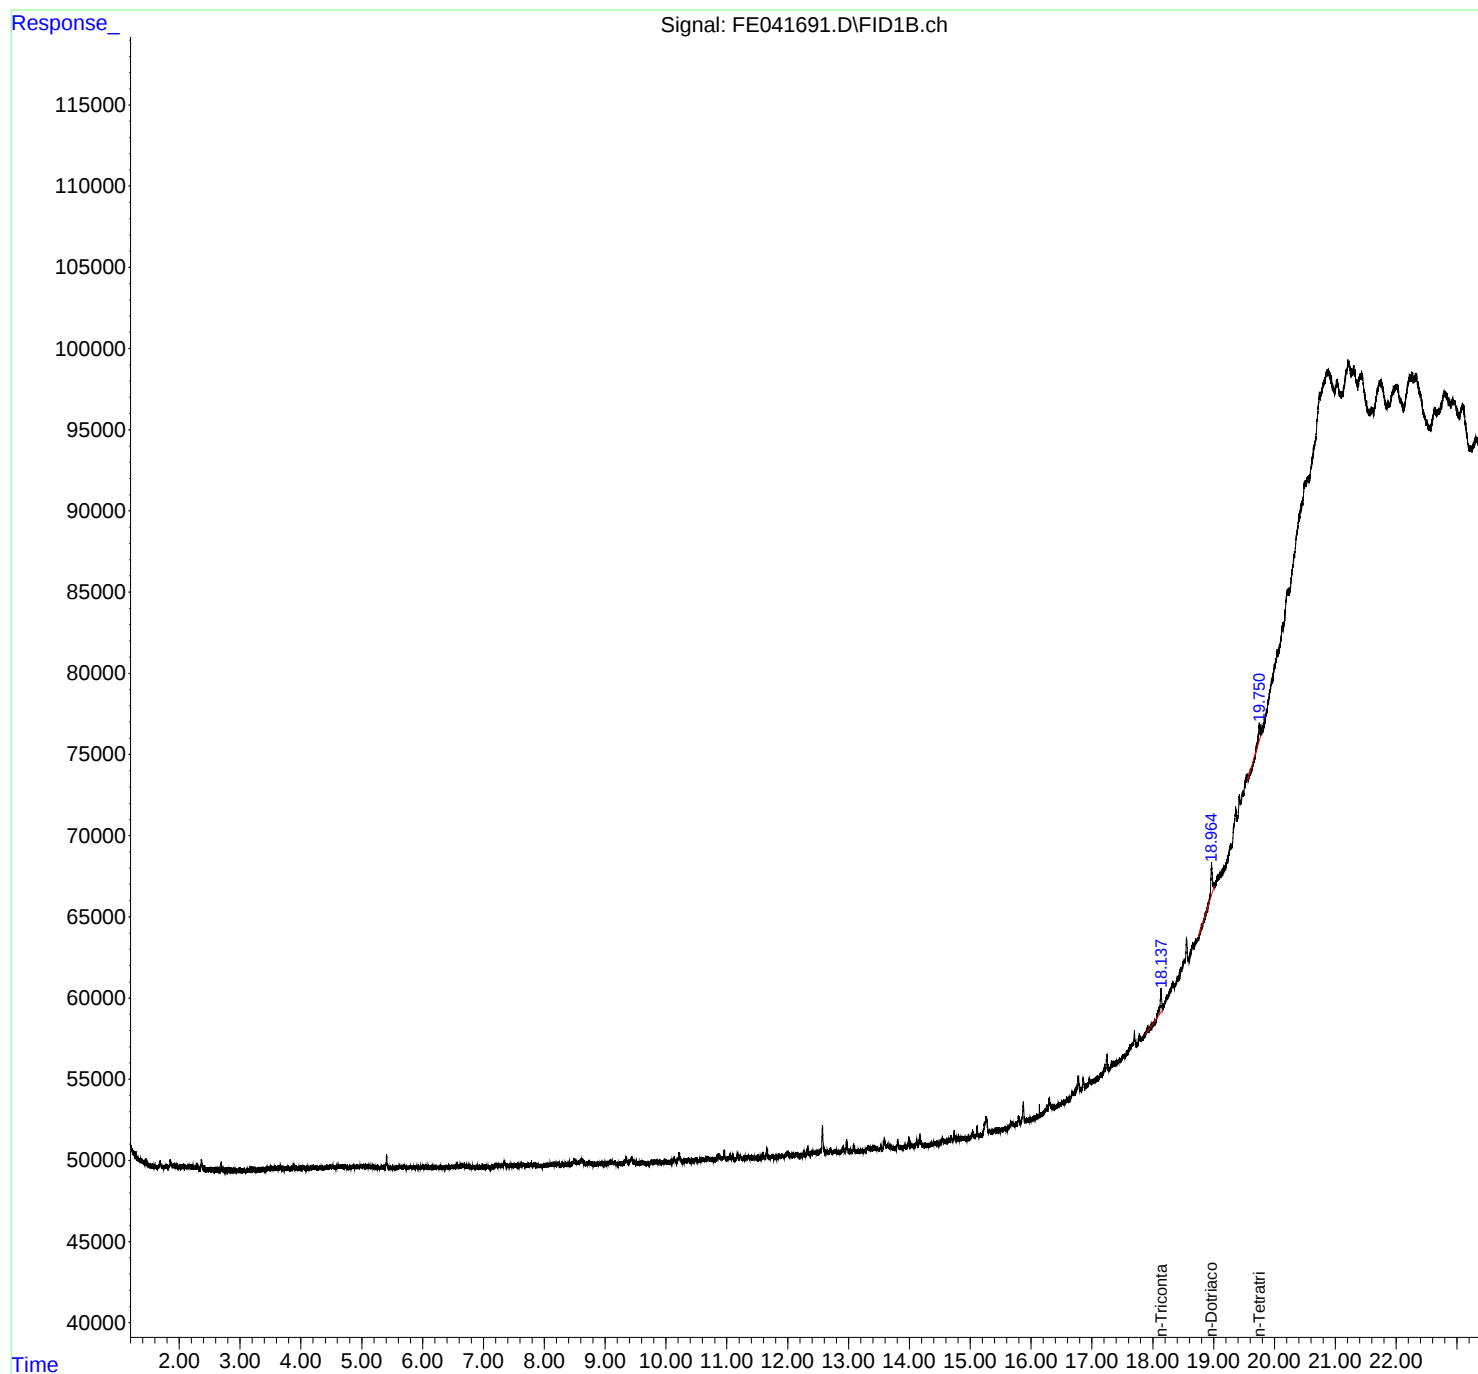


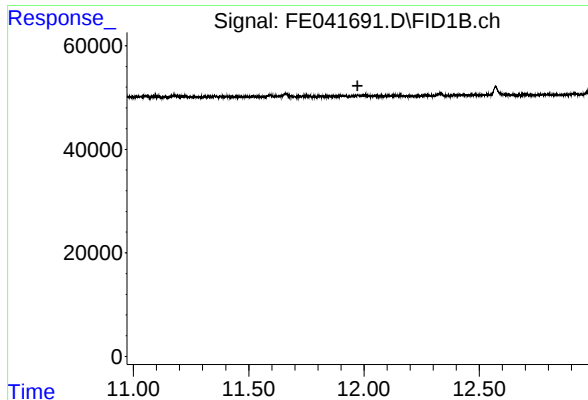

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.972 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

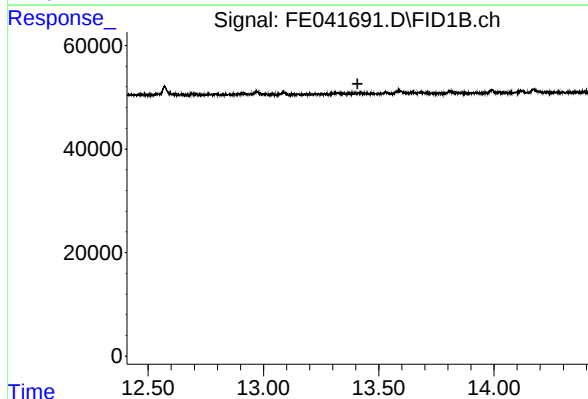


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.408 min
Response: 0
Conc: N.D.

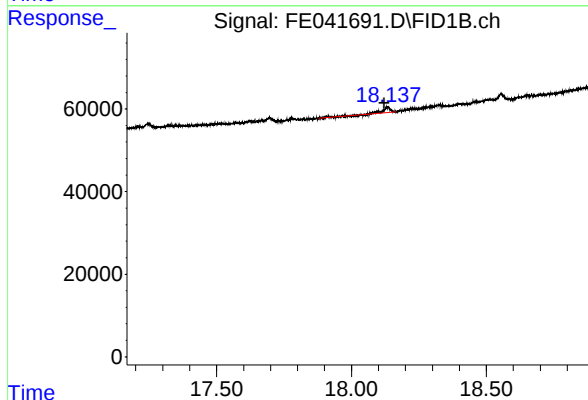


#17 n-Tricontane (C30)

R.T.: 18.137 min
Delta R.T.: 0.015 min
Response: 26197
Conc: 0.17 ug/ml

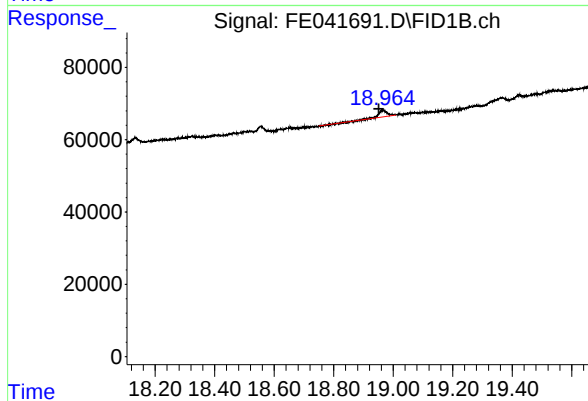

#18 n-Dotriacontane (C32)

R.T.: 18.965 min
Delta R.T.: 0.012 min
Response: 32892
Conc: 0.22 ug/ml

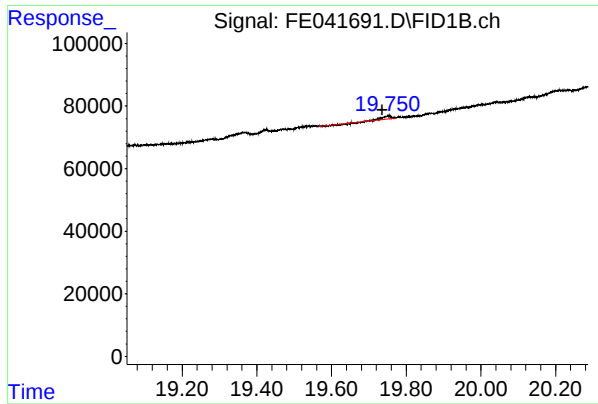

#19 n-Tetratriacontane (C34)

R.T.: 19.752 min
Delta R.T.: 0.016 min
Response: 7399
Conc: 0.05 ug/ml

Instrument :
FID_E
ClientSampleId :