

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE050324AL\  
 Data File : FE047966.D  
 Signal(s) : FID1B.ch  
 Acq On : 03 May 2024 14:48  
 Operator : YP\AJ  
 Sample : P2332-01  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 PAT-DIS-02-05012024

Integration File: autoint1.e  
 Quant Time: May 03 23:46:27 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 042724.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Apr 29 03:29:12 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.967 | 3593700    | 24.910 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 49.82%       |
| 12) S 1-chlorooctadecane (S... | 13.402 | 2975387    | 26.628 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 53.26%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE050324AL\  
Data File : FE047966.D  
Signal(s) : FID1B.ch  
Acq On : 03 May 2024 14:48  
Operator : YP\AJ  
Sample : P2332-01  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
PAT-DIS-02-05012024

Integration File: autoint1.e  
Quant Time: May 03 23:46:27 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 042724.M  
Quant Title : GC Extractables  
QLast Update : Mon Apr 29 03:29:12 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

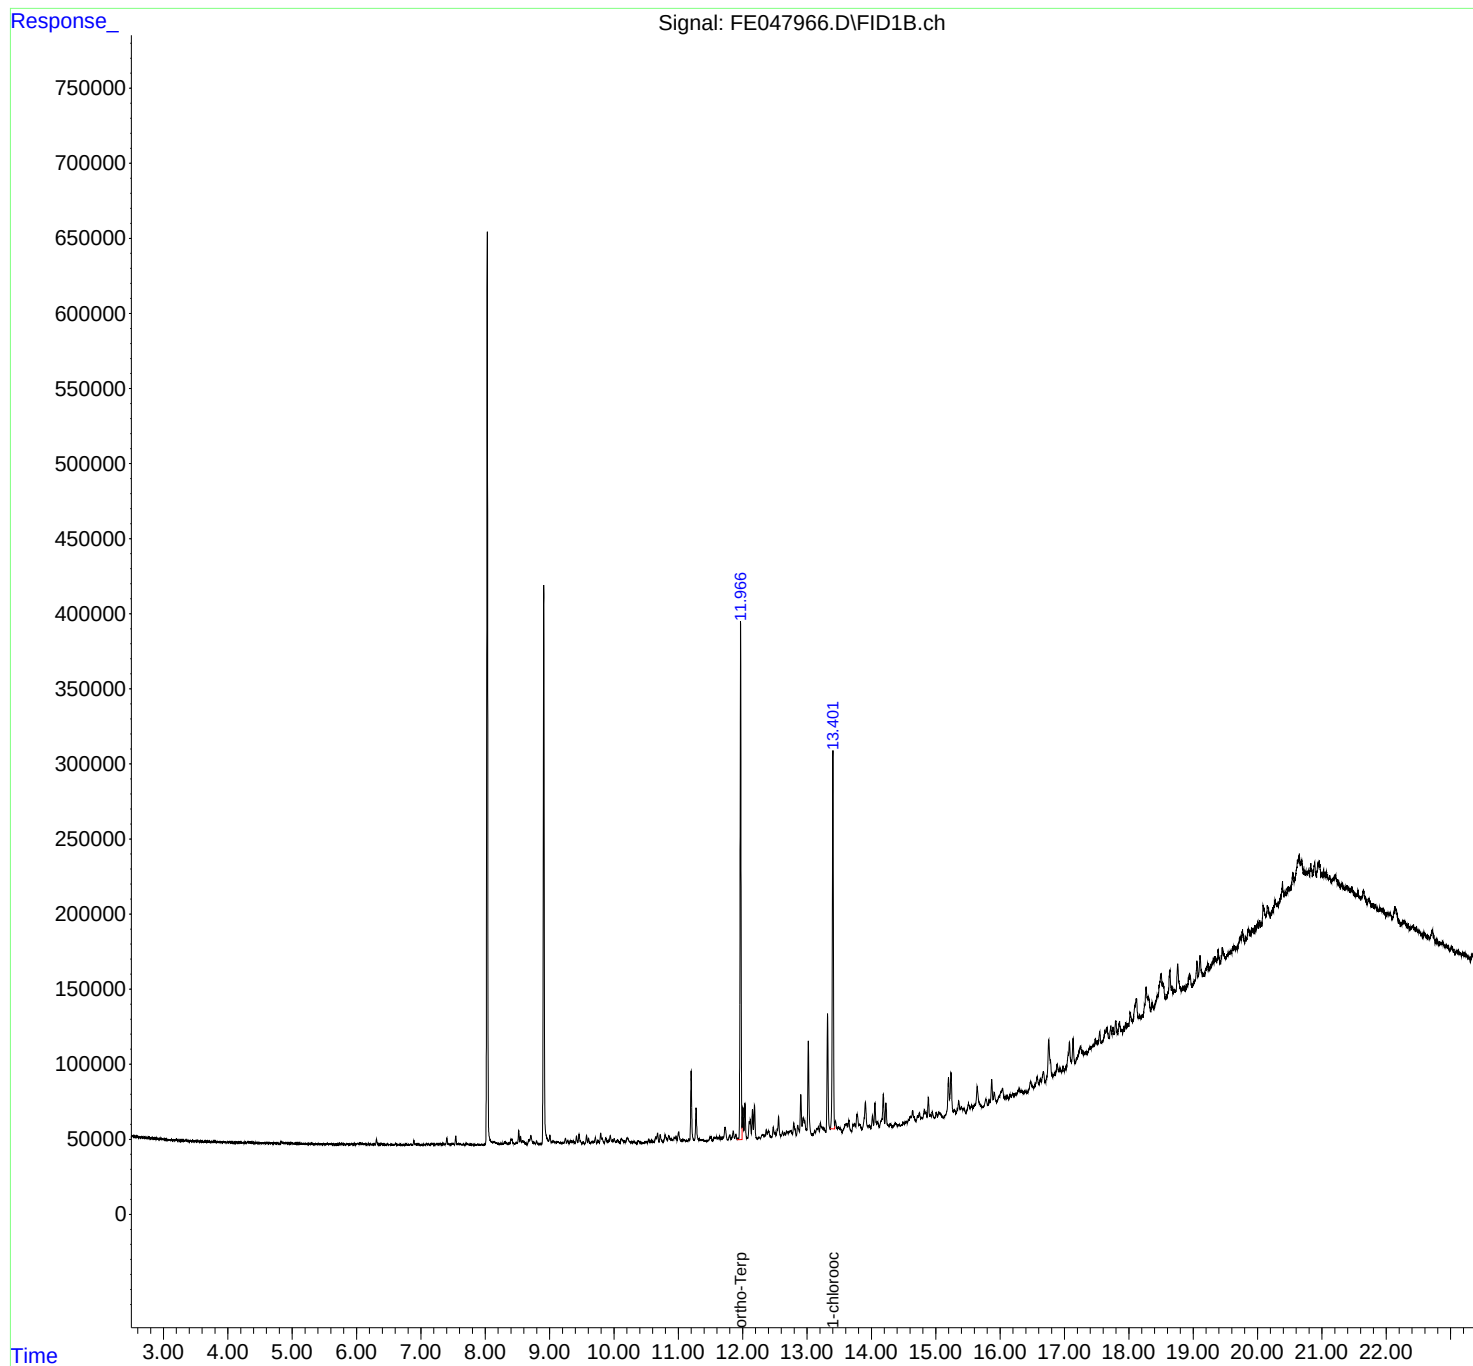


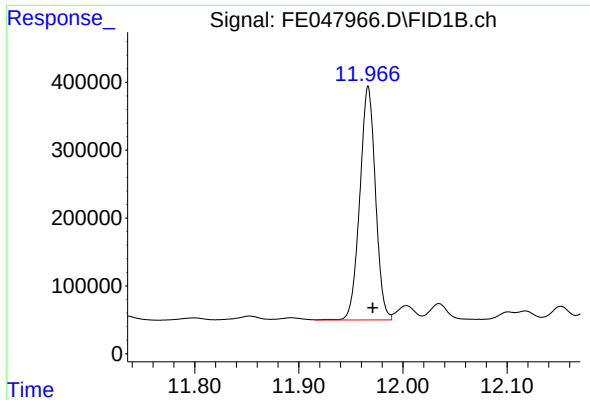

#9 ortho-Terphenyl (SURR)

R.T.: 11.967 min  
Delta R.T.: -0.004 min  
Response: 3593700  
Conc: 24.91 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
PAT-DIS-02-05012024

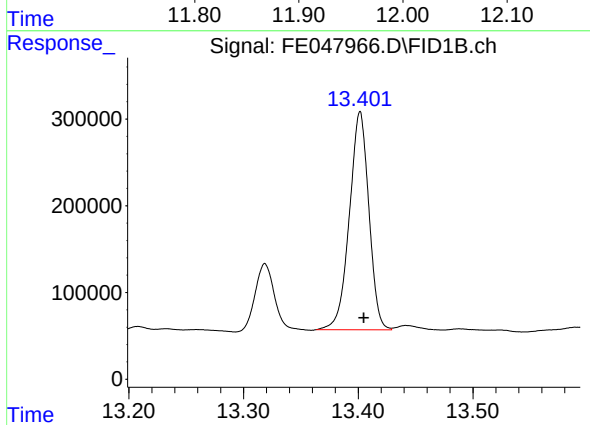

#12 1-chlorooctadecane (SURR)

R.T.: 13.402 min  
Delta R.T.: -0.003 min  
Response: 2975387  
Conc: 26.63 ug/ml