

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE050324AL\  
 Data File : FE047968.D  
 Signal(s) : FID1B.ch  
 Acq On : 03 May 2024 15:49  
 Operator : YP\AJ  
 Sample : P2332-04  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 PAT-DIS-02-05012024-E3

Integration File: autoint1.e  
 Quant Time: May 03 23:46:55 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 042724.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Apr 29 03:29:12 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.969 | 4365430    | 30.260 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 60.52%       |
| 12) S 1-chlorooctadecane (S... | 13.403 | 3502316    | 31.343 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 62.69%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE050324AL\  
Data File : FE047968.D  
Signal(s) : FID1B.ch  
Acq On : 03 May 2024 15:49  
Operator : YP\AJ  
Sample : P2332-04  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
PAT-DIS-02-05012024-E3

Integration File: autoint1.e  
Quant Time: May 03 23:46:55 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 042724.M  
Quant Title : GC Extractables  
QLast Update : Mon Apr 29 03:29:12 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

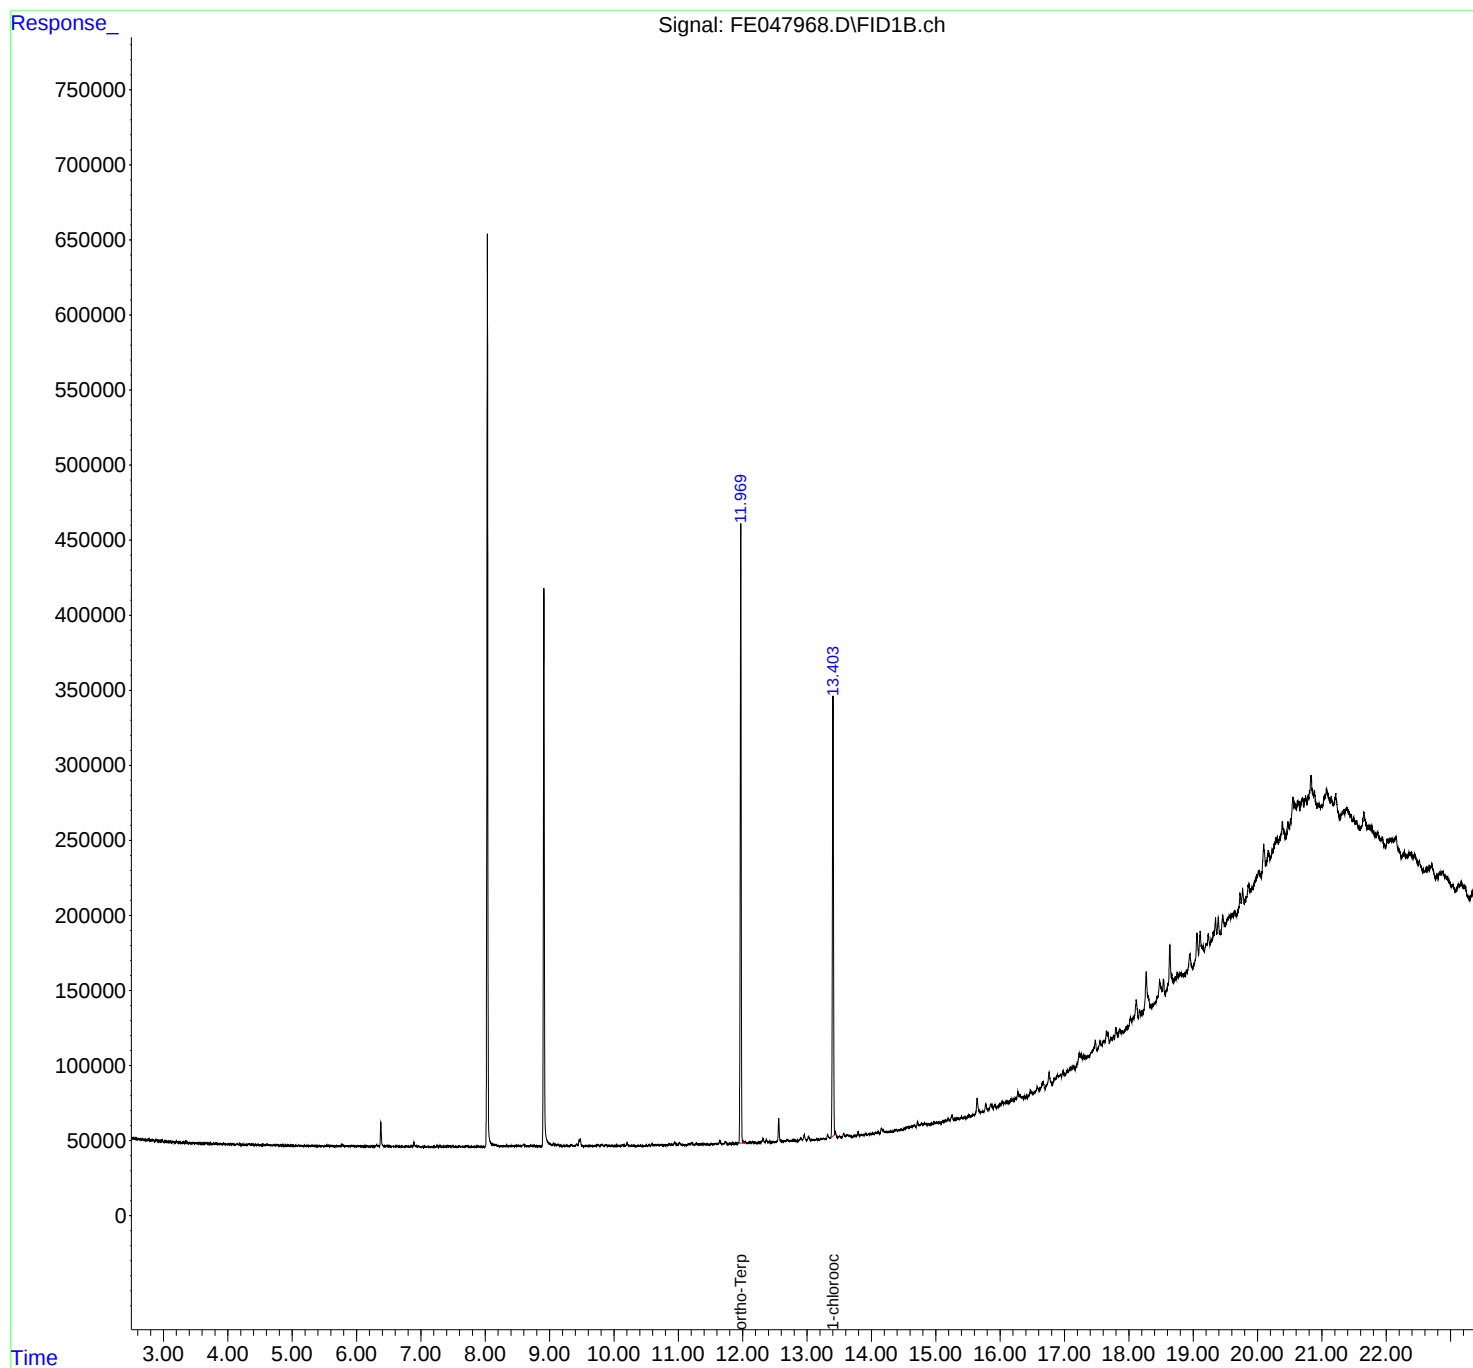


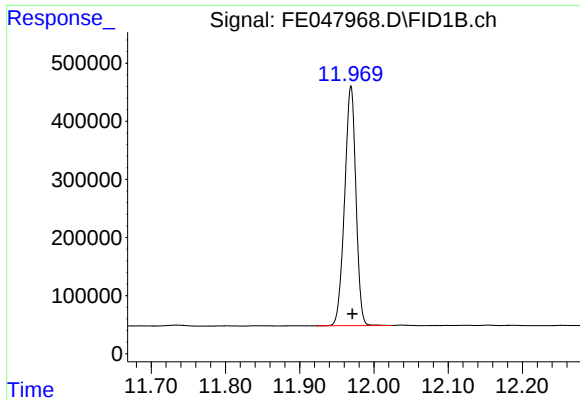

#9 ortho-Terphenyl (SURR)

R.T.: 11.969 min  
Delta R.T.: -0.002 min  
Response: 4365430  
Conc: 30.26 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
PAT-DIS-02-05012024-E3

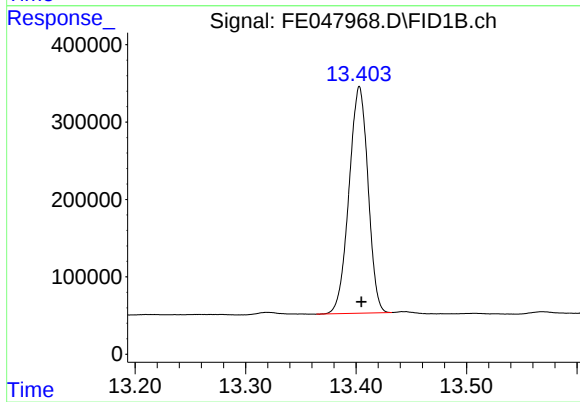

#12 1-chlorooctadecane (SURR)

R.T.: 13.403 min  
Delta R.T.: -0.002 min  
Response: 3502316  
Conc: 31.34 ug/ml