

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050420\
 Data File : FE031890.D
 Signal(s) : FID1B.CH
 Acq On : 04 May 2020 15:02
 Operator : DD\AJ
 Sample : L2463-18 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 JHDS-SOUTH-D

Integration File: autoint1.e
 Quant Time: May 05 00:47:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
 Quant Title :
 QLast Update : Tue Apr 07 15:06:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.371	1202779	3.303 ug/ml
Target Compounds			
7) N-EICOSANE	12.355f	634389	1.507 ug/ml
10) N-TETRACOSANE	14.587	697372	1.666 ug/ml
11) N-HEXACOSANE	15.595	367089	0.886 ug/ml
12) N-OCTACOSANE	16.546	1349243	3.280 ug/ml
13) N-TRIACONTANE	17.433	1025365	2.493 ug/ml
14) N-DOTRIACONTANE	18.267	527209	1.341 ug/ml
15) N-TETRATRIACONTANE	19.051	177620	0.480 ug/ml
16) N-HEXATRIACONTANE	19.797	234734	0.681 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050420\
Data File : FE031890.D
Signal(s) : FID1B.CH
Acq On : 04 May 2020 15:02
Operator : DD\AJ
Sample : L2463-18 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JHDS-SOUTH-D

Integration File: autoint1.e
Quant Time: May 05 00:47:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
Quant Title :
QLast Update : Tue Apr 07 15:06:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

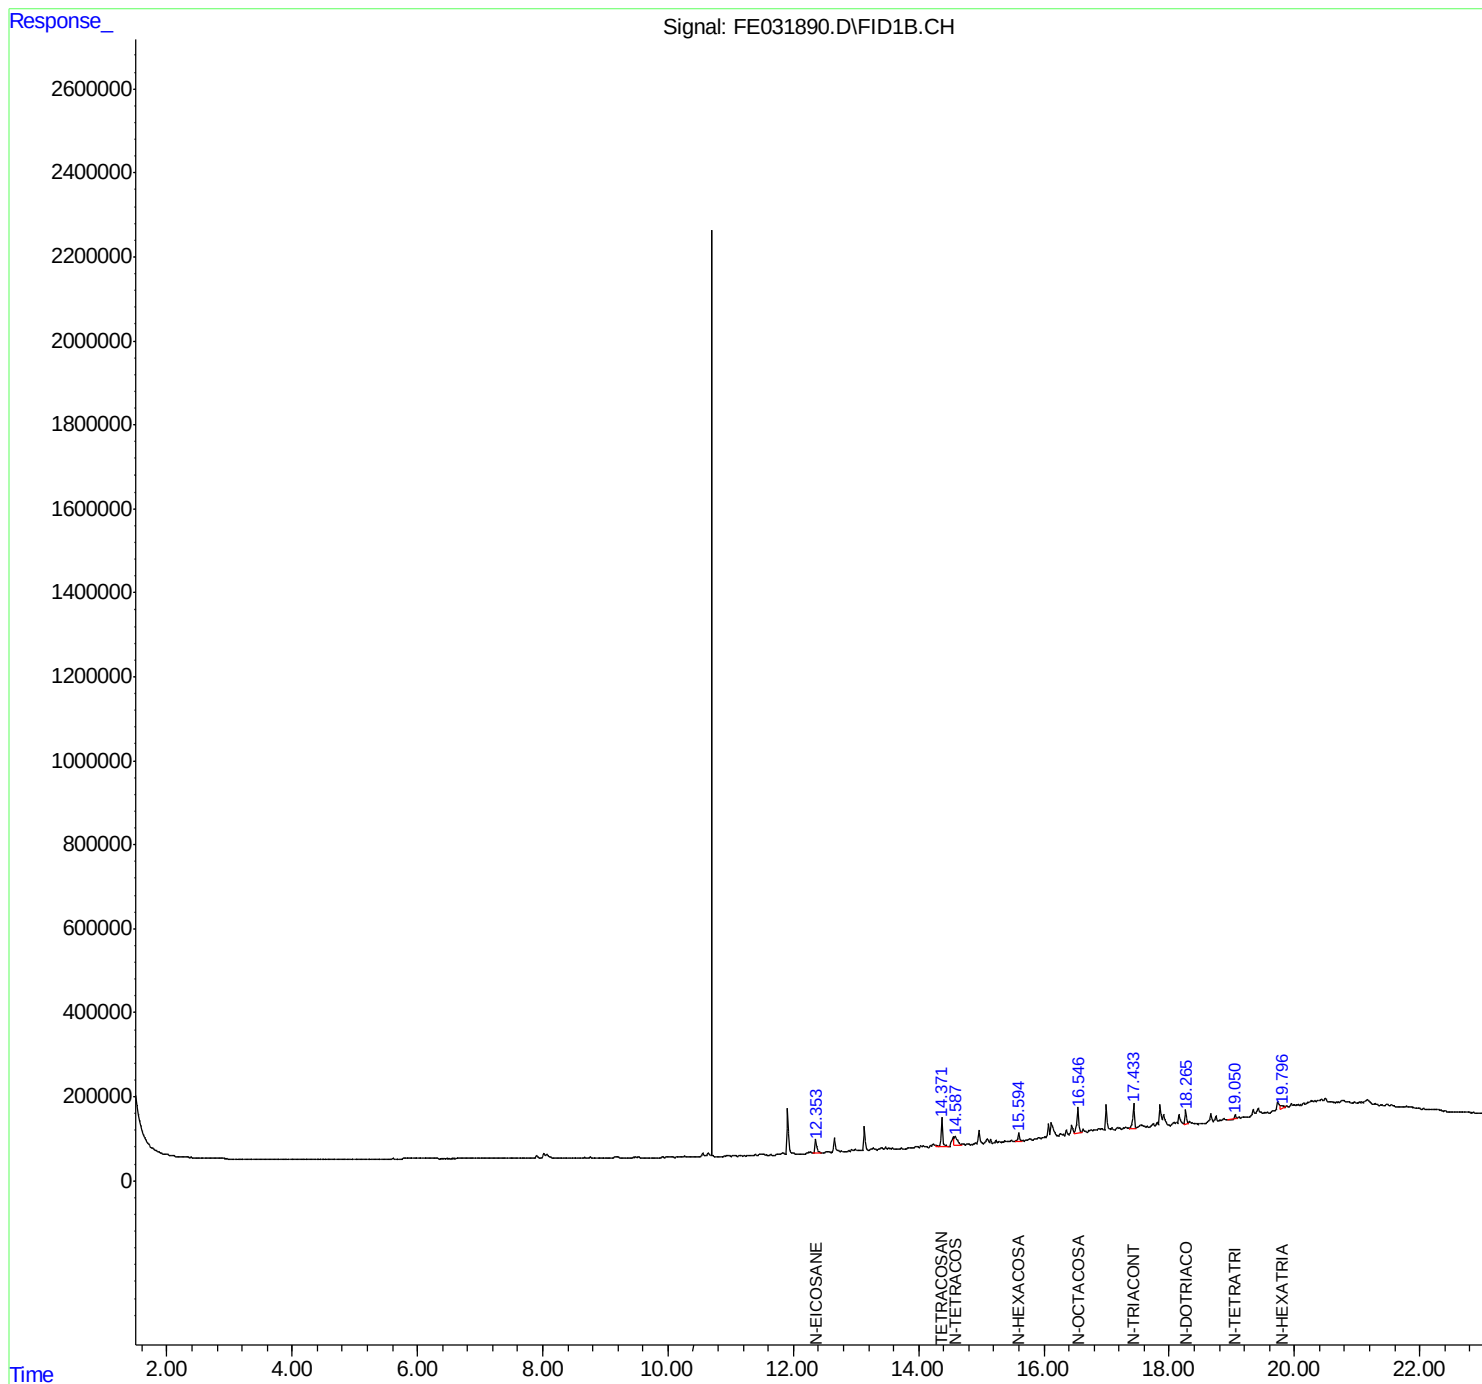


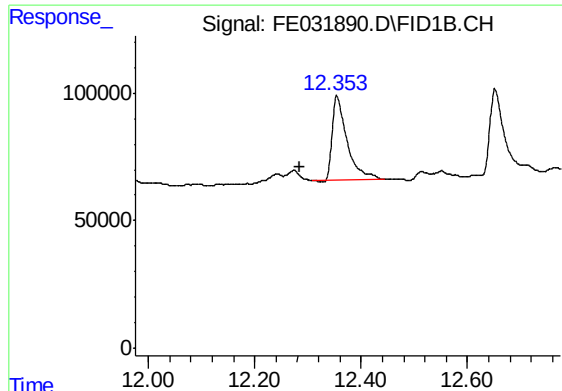

#7 N-EICOSANE


R.T.: 12.355 min
Delta R.T.: 0.070 min
Response: 634389
Conc: 1.51 ug/ml

Instrument :
FID_E
ClientSampleId :
JHDS-SOUTH-D

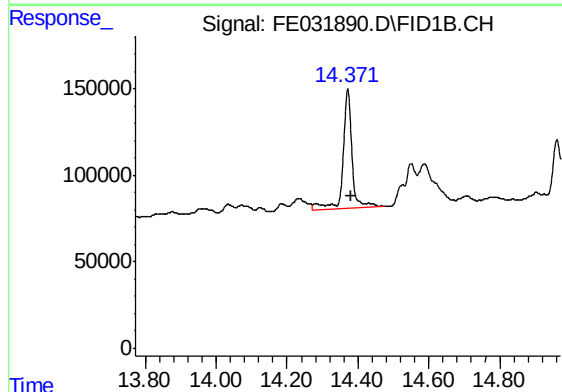


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.371 min
Delta R.T.: -0.008 min
Response: 1202779
Conc: 3.30 ug/ml

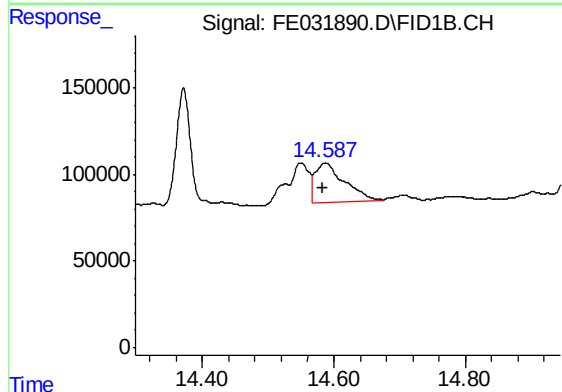


#10 N-TETRACOSANE

R.T.: 14.587 min
Delta R.T.: 0.003 min
Response: 697372
Conc: 1.67 ug/ml

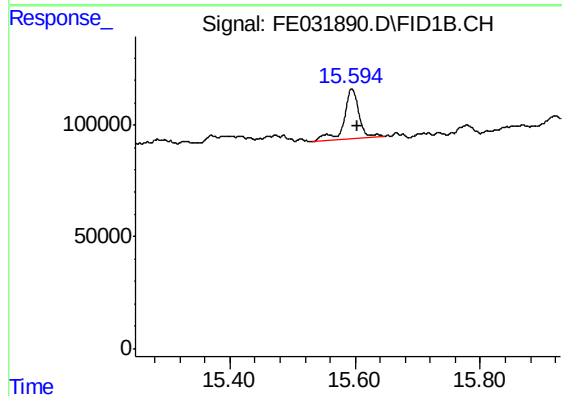

#11 N-HEXACOSANE


R.T.: 15.595 min
Delta R.T.: -0.008 min
Response: 367089
Conc: 0.89 ug/ml

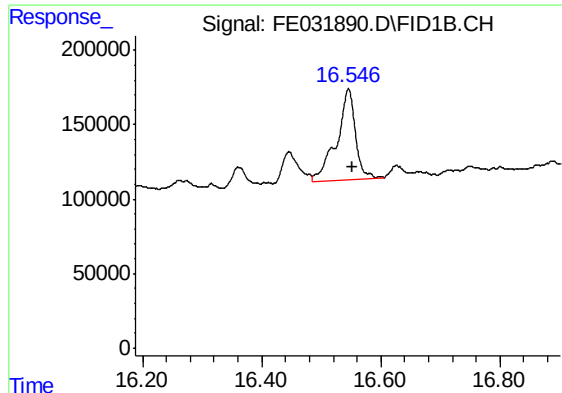

#12 N-OCTACOSANE


R.T.: 16.546 min
Delta R.T.: -0.007 min
Response: 1349243
Conc: 3.28 ug/ml

Instrument :
FID_E
ClientSampleId :
JHDS-SOUTH-D

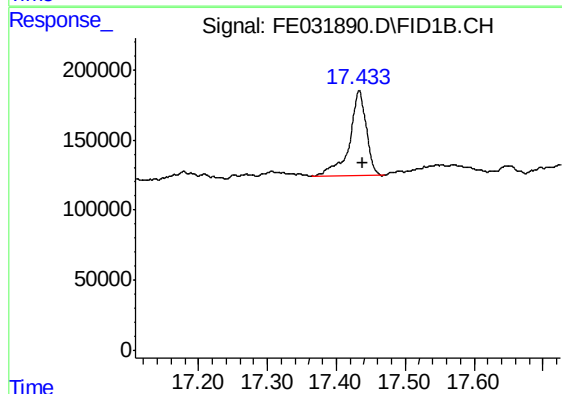


#13 N-TRIACONTANE

R.T.: 17.433 min
Delta R.T.: -0.005 min
Response: 1025365
Conc: 2.49 ug/ml

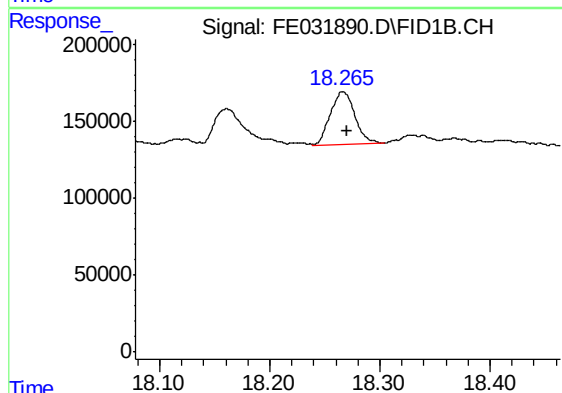


#14 N-DOTRIACONTANE

R.T.: 18.267 min
Delta R.T.: -0.003 min
Response: 527209
Conc: 1.34 ug/ml

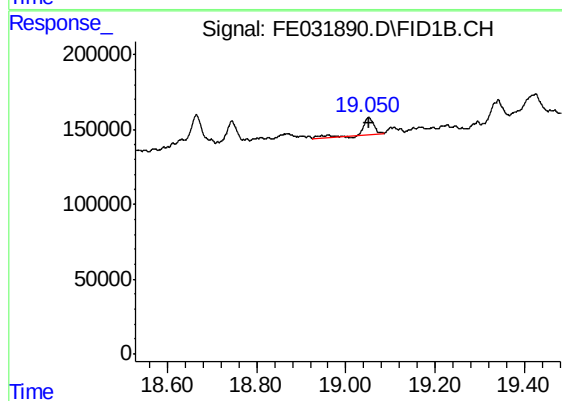

#15 N-TETRATRIACONTANE

R.T.: 19.051 min
Delta R.T.: 0.000 min
Response: 177620
Conc: 0.48 ug/ml

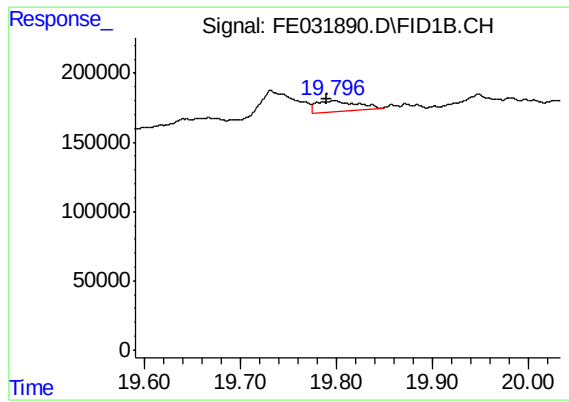

#16 N-HEXATRIACONTANE

R.T.: 19.797 min
Delta R.T.: 0.007 min
Response: 234734
Conc: 0.68 ug/ml

Instrument :
FID_E
ClientSampleId :
JHDS-SOUTH-D