

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050423AL\
Data File : FE041745.D
Signal(s) : FID1B.ch
Acq On : 04 May 2023 23:03
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 05 01:19:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.124	25201	0.165 ug/ml
18) T	n-Dotriacontane (C32)	18.953	32693	0.219 ug/ml
19) T	n-Tetratriacontane (C34)	19.741	24309	0.173 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050423AL\
Data File : FE041745.D
Signal(s) : FID1B.ch
Acq On : 04 May 2023 23:03
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 05 01:19:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

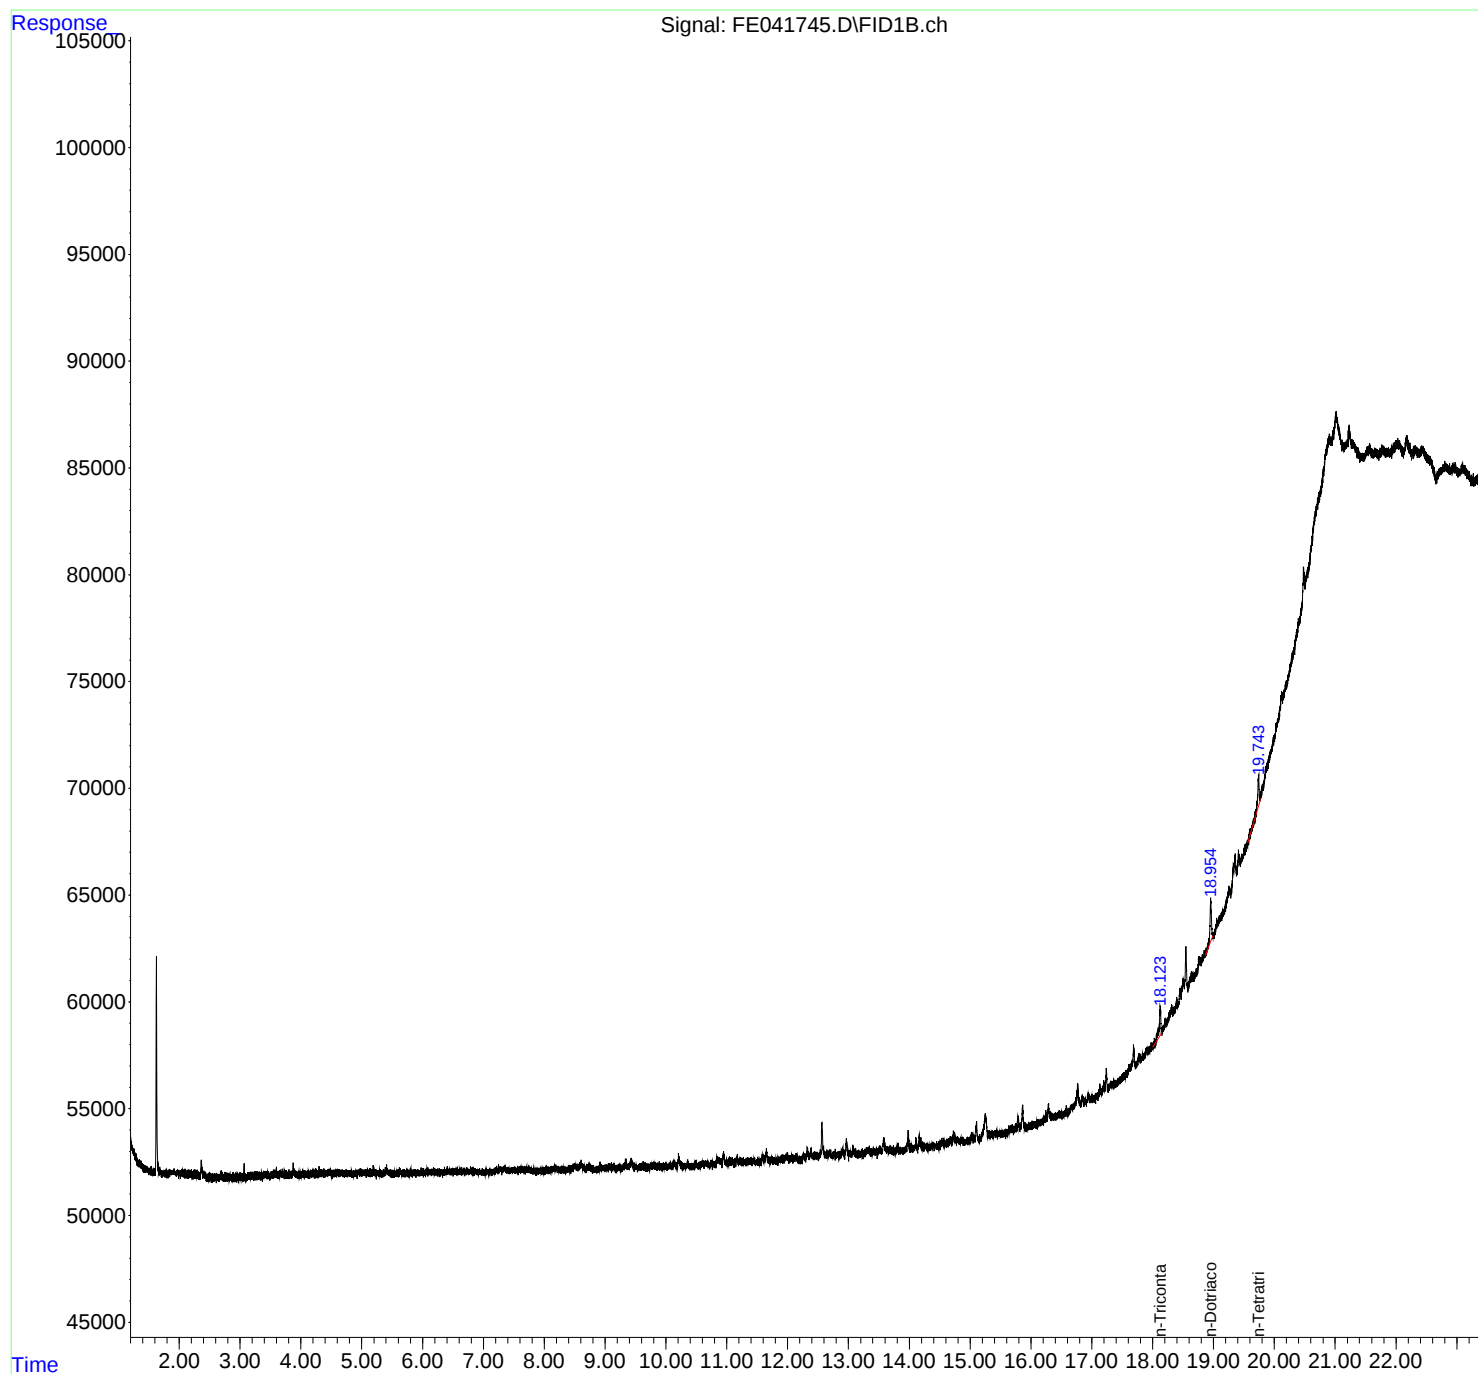


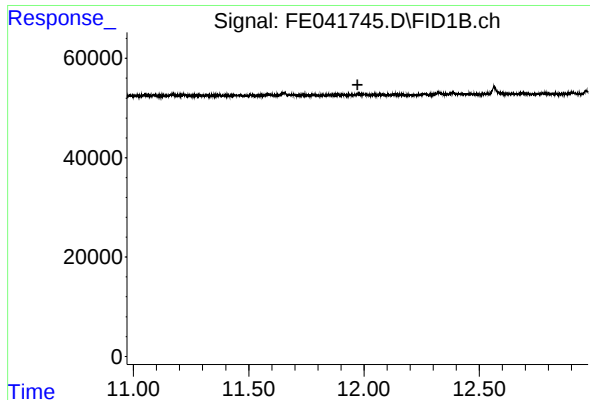

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.972 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

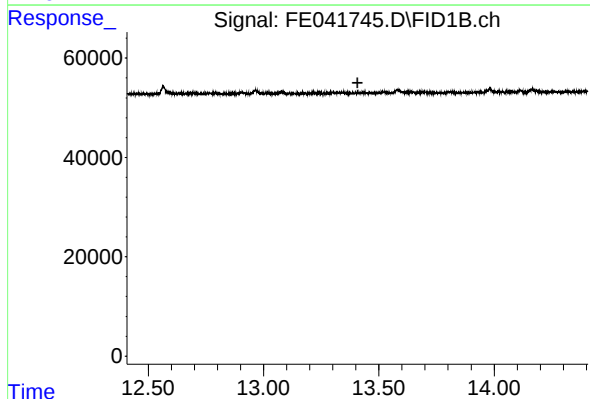


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.408 min
Response: 0
Conc: N.D.

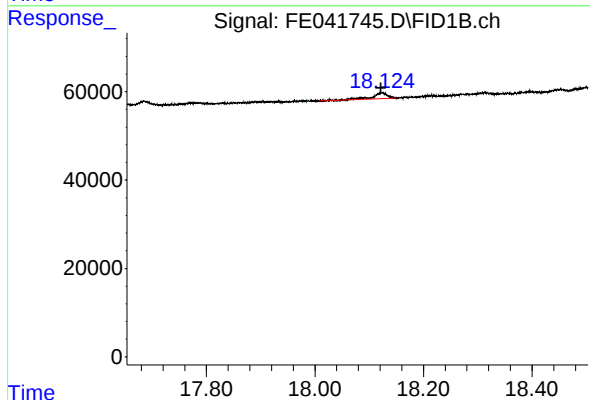


#17 n-Tricontane (C30)

R.T.: 18.124 min
Delta R.T.: 0.003 min
Response: 25201
Conc: 0.17 ug/ml

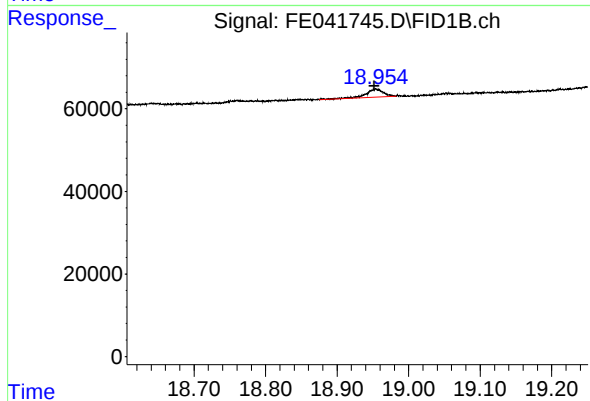

#18 n-Dotriacontane (C32)

R.T.: 18.953 min
Delta R.T.: 0.001 min
Response: 32693
Conc: 0.22 ug/ml

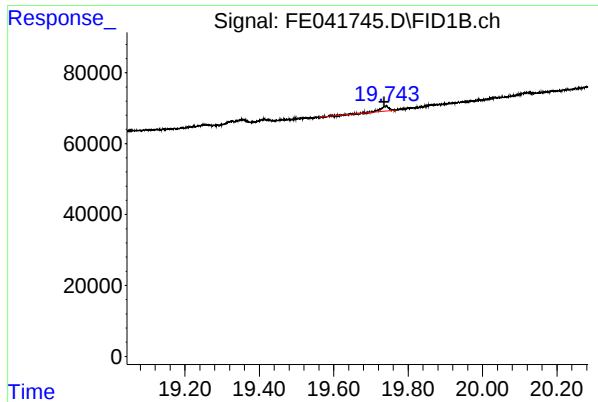

#19 n-Tetratriacontane (C34)

R.T.: 19.741 min
Delta R.T.: 0.005 min
Response: 24309
Conc: 0.17 ug/ml

Instrument :

FID_E

ClientSampleId :