

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050520\
 Data File : FE031897.D
 Signal(s) : FID1B.CH
 Acq On : 05 May 2020 8:49
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 05 14:01:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
 Quant Title :
 QLast Update : Tue Apr 07 15:06:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.142	10773009	28.758 ug/ml
12)	N-OCTACOSANE	16.551	12289501	29.872 ug/ml
13)	N-TRIACONTANE	17.428	754869	1.835 ug/ml
14)	N-DOTRIACONTANE	18.262	869318	2.211 ug/ml
15)	N-TETRATRIACONTANE	19.045	710493	1.919 ug/ml
16)	N-HEXATRIACONTANE	19.786	595799	1.728 ug/ml
17)	N-OCTATRIACONTANE	20.488	488550	1.580 ug/ml
18)	N-TETRACONTANE	21.292	784914	2.483 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050520\
Data File : FE031897.D
Signal(s) : FID1B.CH
Acq On : 05 May 2020 8:49
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 05 14:01:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
Quant Title :
QLast Update : Tue Apr 07 15:06:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

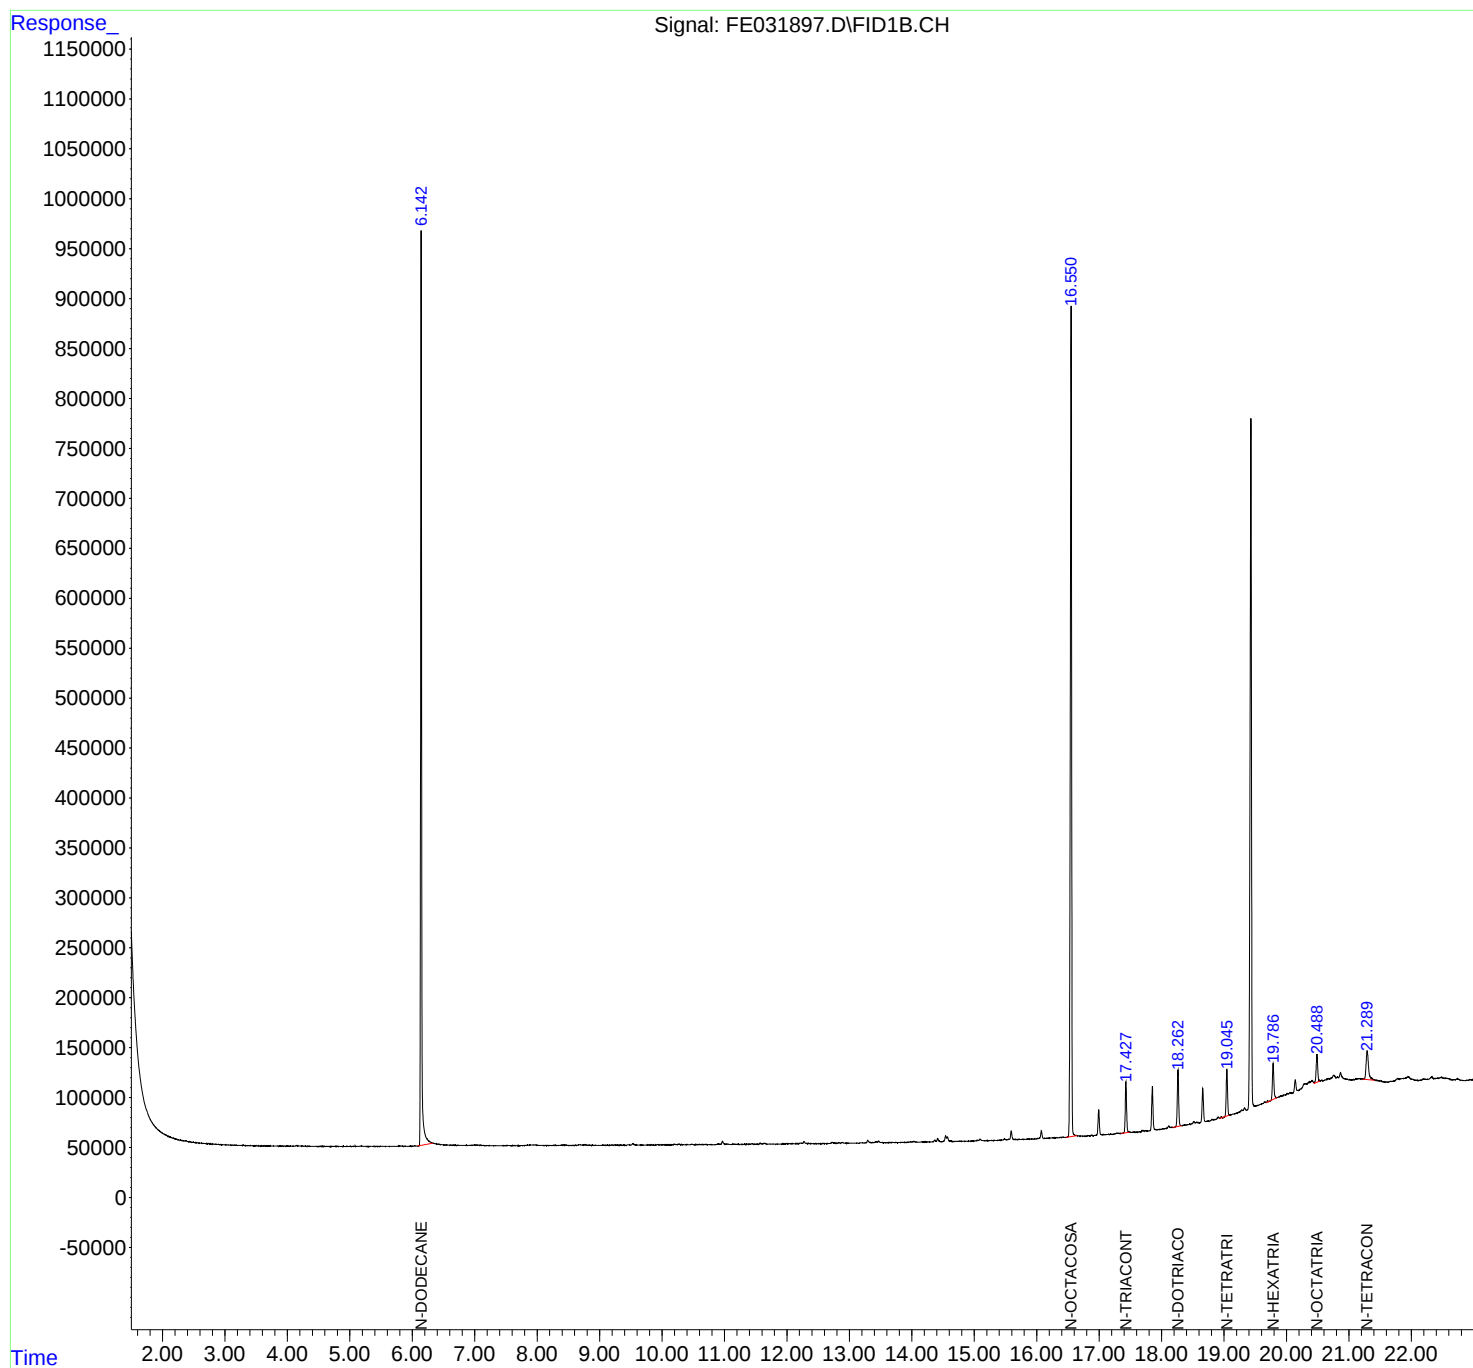


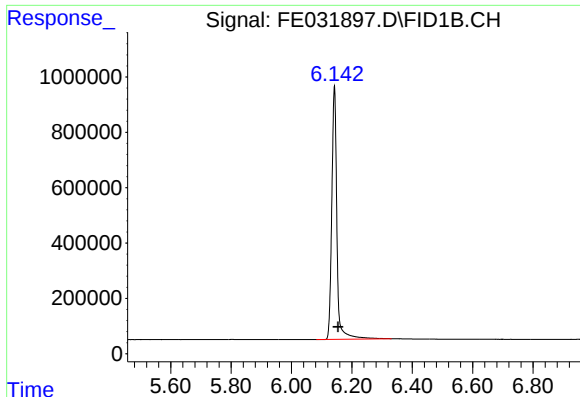

#3 N-DODECANE


R.T.: 6.142 min
Delta R.T.: -0.012 min
Response: 10773009
Conc: 28.76 ug/ml

Instrument :
FID_E
ClientSampleId :

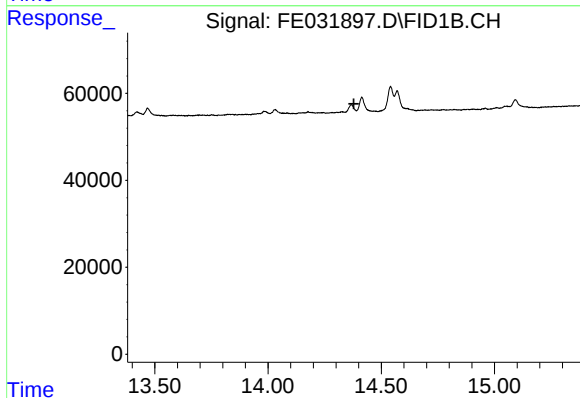


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.379 min
Response: 0
Conc: N.D.

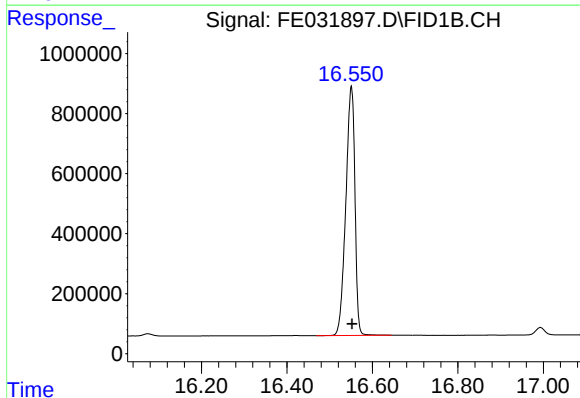


#12 N-OCTACOSANE

R.T.: 16.551 min
Delta R.T.: -0.002 min
Response: 12289501
Conc: 29.87 ug/ml

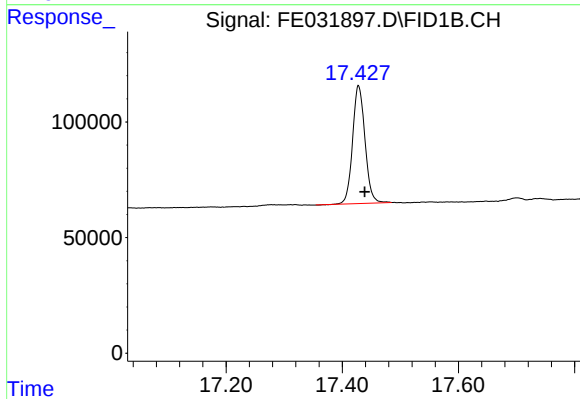

#13 N-TRIACONTANE


R.T.: 17.428 min
Delta R.T.: -0.010 min
Response: 754869
Conc: 1.84 ug/ml

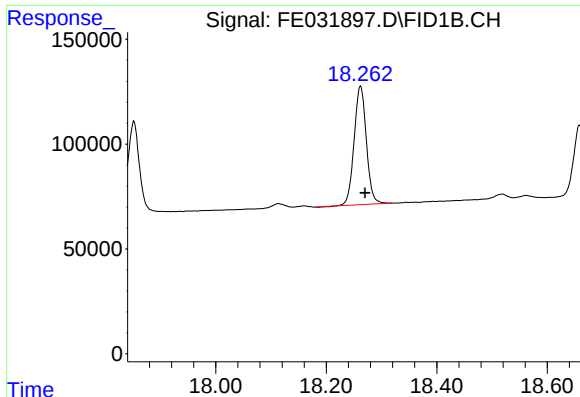

#14 N-DOTRIACONTANE


R.T.: 18.262 min
Delta R.T.: -0.008 min
Response: 869318
Conc: 2.21 ug/ml

Instrument :
FID_E
ClientSampleId :

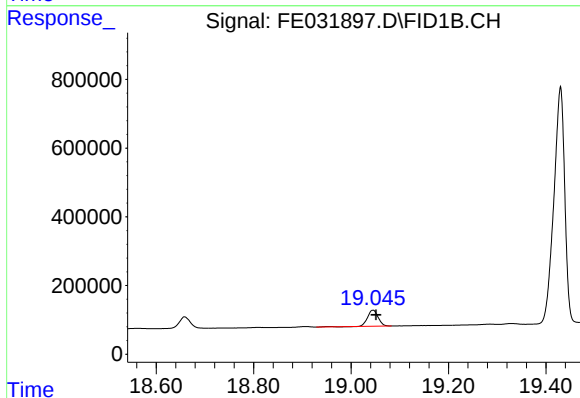


#15 N-TETRATRIACONTANE

R.T.: 19.045 min
Delta R.T.: -0.007 min
Response: 710493
Conc: 1.92 ug/ml

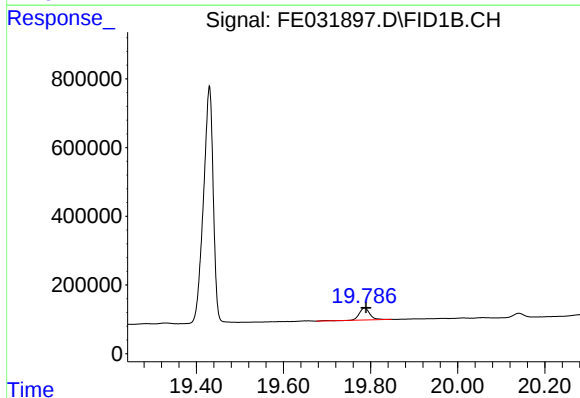


#16 N-HEXATRIACONTANE

R.T.: 19.786 min
Delta R.T.: -0.004 min
Response: 595799
Conc: 1.73 ug/ml

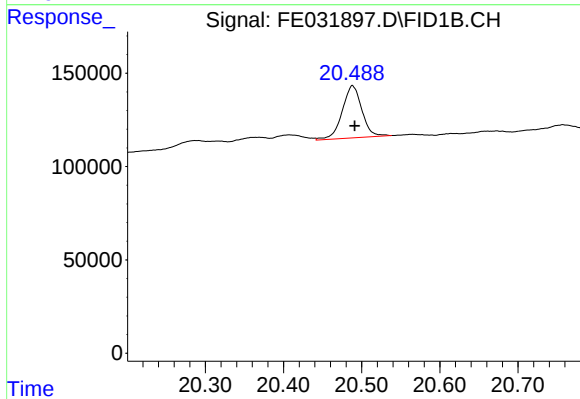

#17 N-OCTATRIACONTANE

R.T.: 20.488 min
Delta R.T.: -0.003 min
Response: 488550
Conc: 1.58 ug/ml

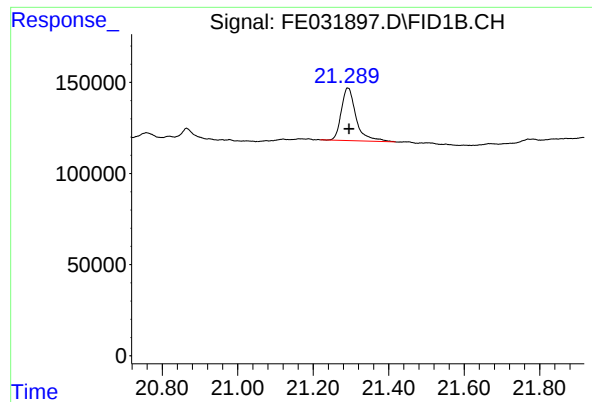

#18 N-TETRACONTANE

R.T.: 21.292 min
Delta R.T.: -0.004 min
Response: 784914
Conc: 2.48 ug/ml

Instrument :
FID_E
ClientSampleId :