

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050520\
 Data File : FE031908.D
 Signal(s) : FID1B.CH
 Acq On : 05 May 2020 15:29
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 05 16:11:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
 Quant Title :
 QLast Update : Tue Apr 07 15:06:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.144	11536955	30.797 ug/ml
12)	N-OCTACOSANE	16.555	12513894	30.417 ug/ml
13)	N-TRIACONTANE	17.433	802602	1.951 ug/ml
14)	N-DOTRIACONTANE	18.266	983205	2.500 ug/ml
15)	N-TETRATRIACONTANE	19.052	740685	2.000 ug/ml
16)	N-HEXATRIACONTANE	19.793	778873	2.259 ug/ml
17)	N-OCTATRIACONTANE	20.497	453857	1.468 ug/ml
18)	N-TETRACONTANE	21.305	941304	2.978 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050520\
Data File : FE031908.D
Signal(s) : FID1B.CH
Acq On : 05 May 2020 15:29
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: May 05 16:11:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE040720.M
Quant Title :
QLast Update : Tue Apr 07 15:06:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

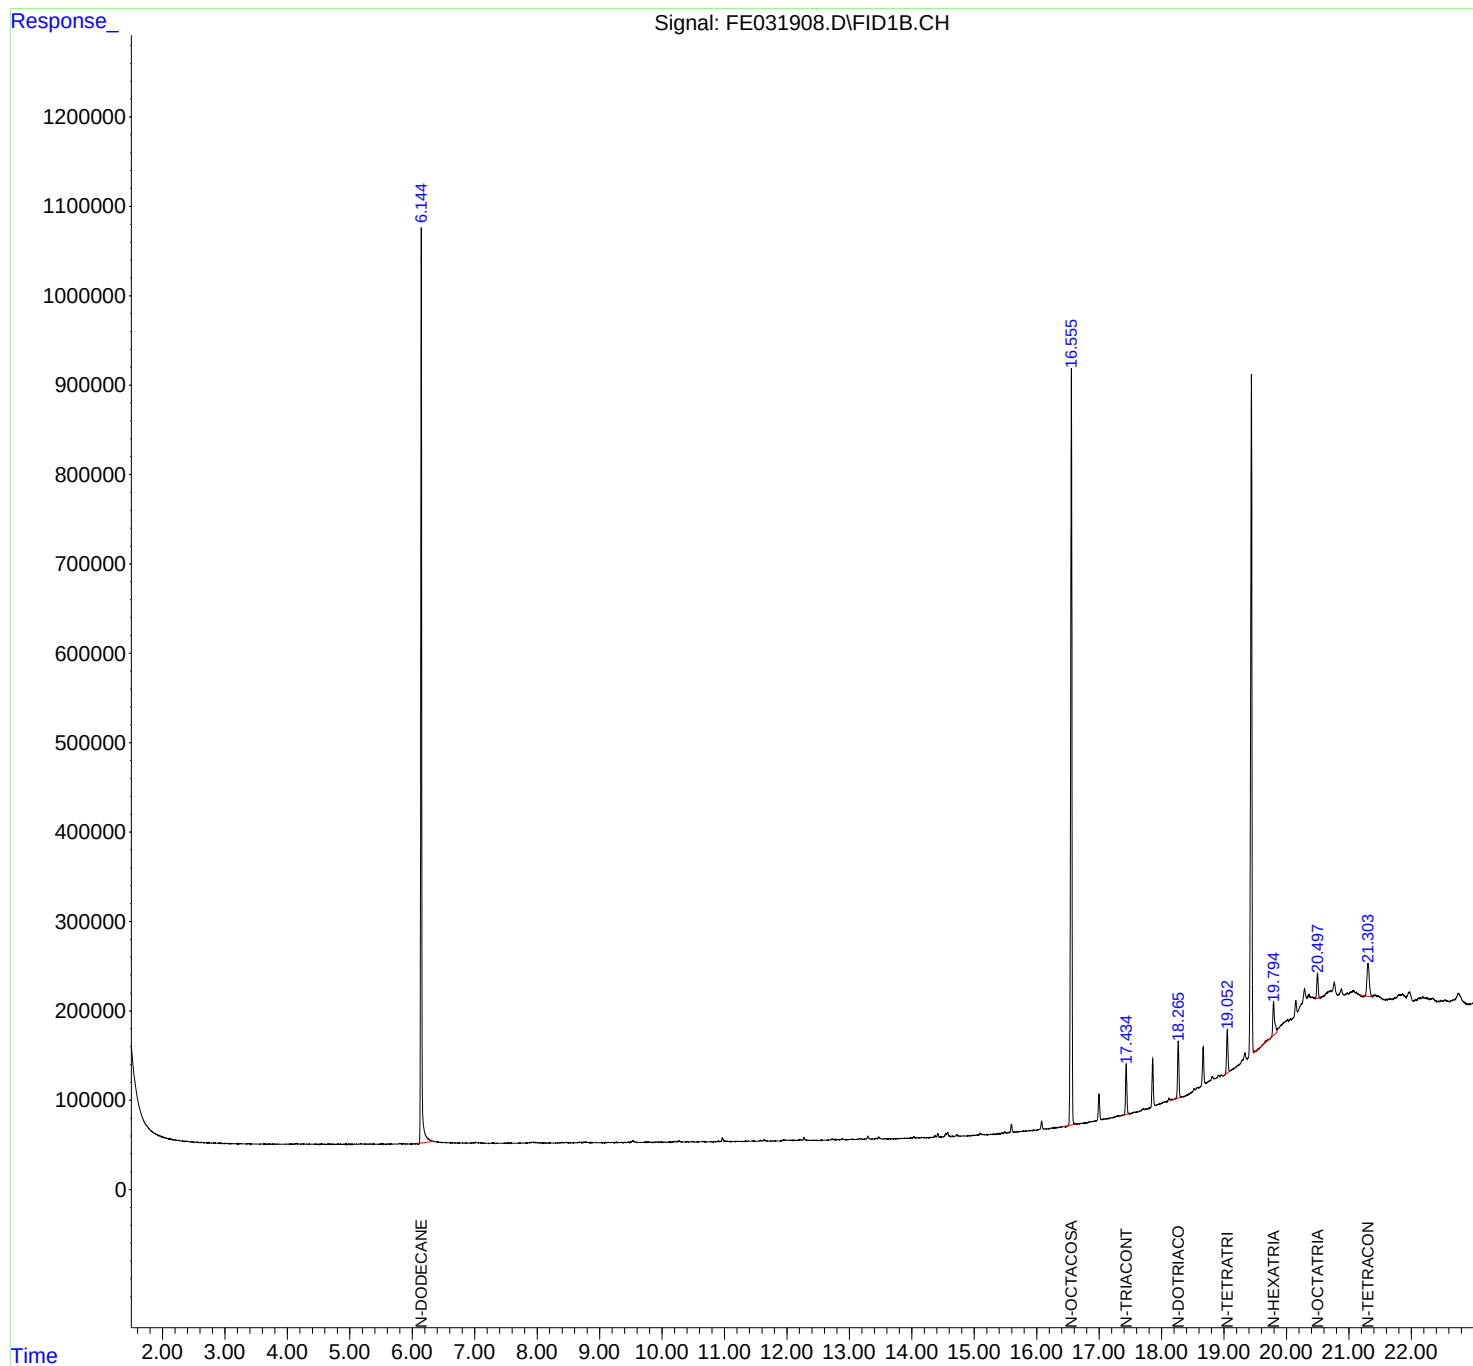


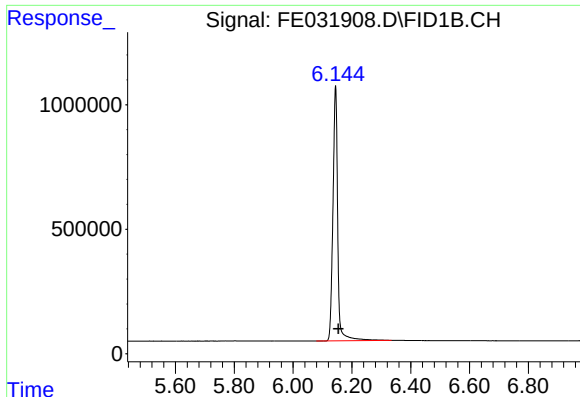

#3 N-DODECANE


R.T.: 6.144 min
Delta R.T.: -0.010 min
Response: 11536955
Conc: 30.80 ug/ml

Instrument :
FID_E
ClientSampleId :

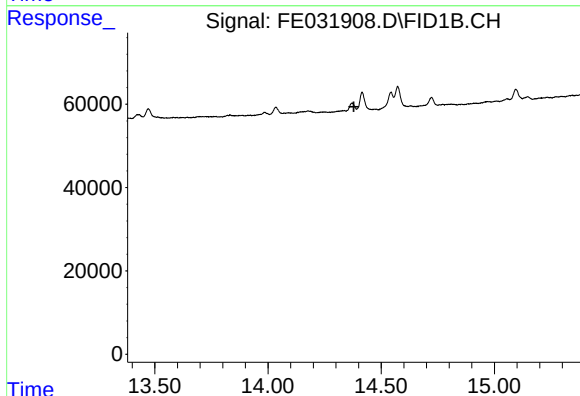


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.379 min
Response: 0
Conc: N.D.

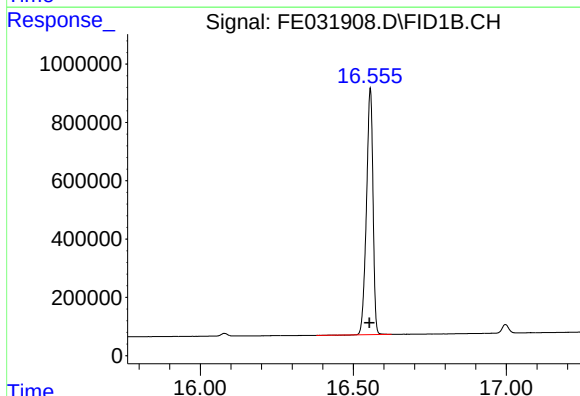


#12 N-OCTACOSANE

R.T.: 16.555 min
Delta R.T.: 0.003 min
Response: 12513894
Conc: 30.42 ug/ml

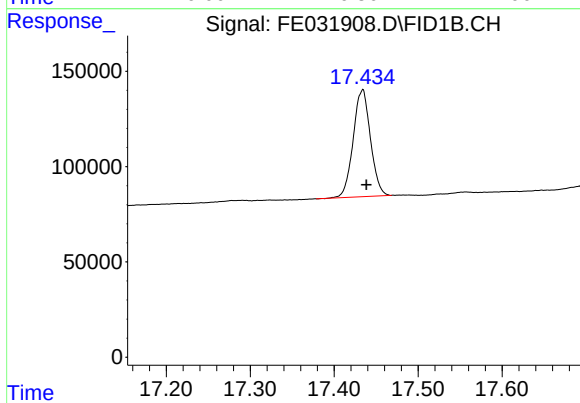

#13 N-TRIACONTANE


R.T.: 17.433 min
Delta R.T.: -0.005 min
Response: 802602
Conc: 1.95 ug/ml

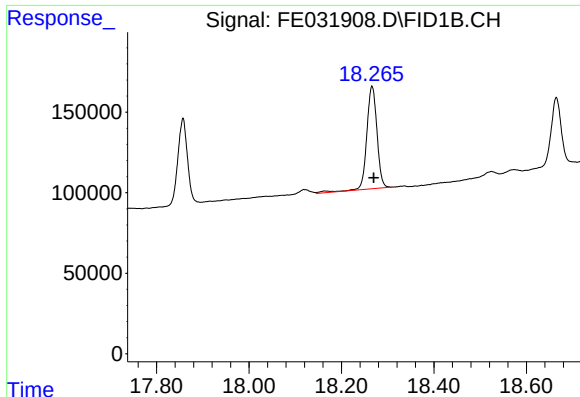

#14 N-DOTRIACONTANE


R.T.: 18.266 min
Delta R.T.: -0.004 min
Response: 983205
Conc: 2.50 ug/ml

Instrument :
FID_E
ClientSampleId :

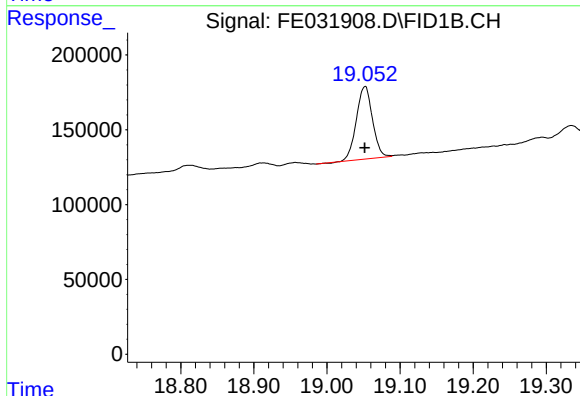


#15 N-TETRATRIACONTANE

R.T.: 19.052 min
Delta R.T.: 0.000 min
Response: 740685
Conc: 2.00 ug/ml

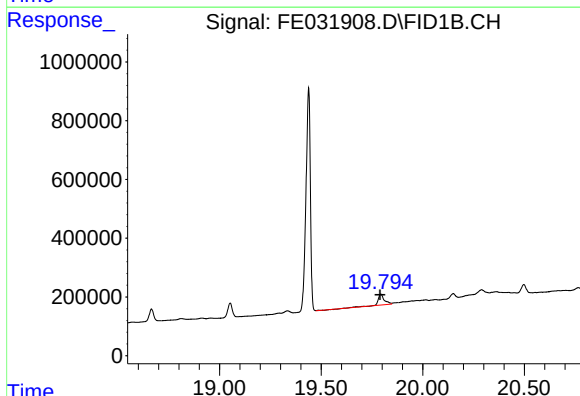


#16 N-HEXATRIACONTANE

R.T.: 19.793 min
Delta R.T.: 0.004 min
Response: 778873
Conc: 2.26 ug/ml

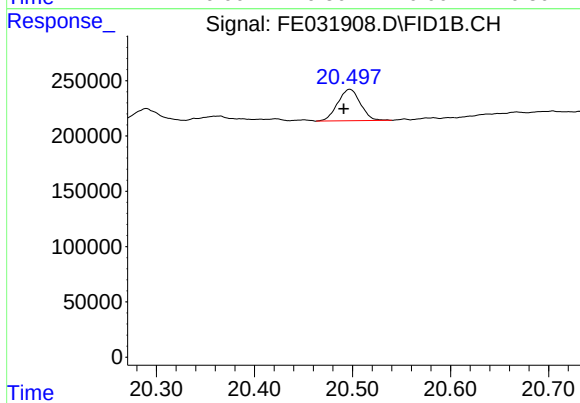

#17 N-OCTATRIACONTANE

R.T.: 20.497 min
Delta R.T.: 0.006 min
Response: 453857
Conc: 1.47 ug/ml

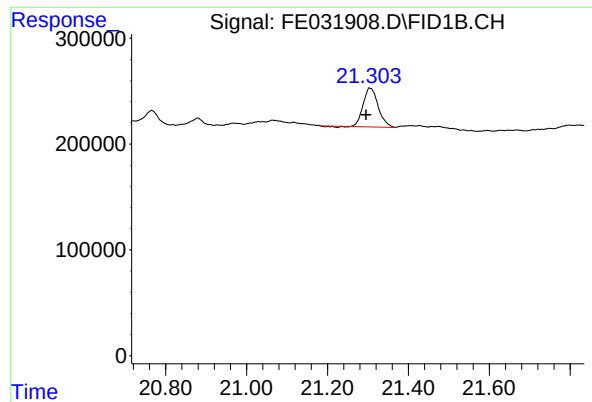

#18 N-TETRACONTANE

R.T.: 21.305 min
Delta R.T.: 0.010 min
Response: 941304
Conc: 2.98 ug/ml

Instrument :
FID_E
ClientSampleId :