

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050523AL\
 Data File : FE041747.D
 Signal(s) : FID1B.ch
 Acq On : 05 May 2023 08:25
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 06 01:25:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 07:33:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.949	127343	0.792 ug/ml
11) T n-Heneicosane (C21)	13.569	159054	0.998 ug/ml
13) T n-Docosane (C22)	14.158	124982	0.784 ug/ml
14) T n-Tetracosane (C24)	15.241	369285	2.291 ug/ml
15) T n-Hexacosane (C26)	16.286	122464	0.775 ug/ml
16) T n-Octacosane (C28)	17.234	82668	0.537 ug/ml
17) T n-Tricontane (C30)	18.123	66229	0.435 ug/ml
18) T n-Dotriacontane (C32)	18.957	106914	0.718 ug/ml
19) T n-Tetratriacontane (C34)	19.718	128902	0.915 ug/ml
20) T n-Hexatriacontane (C36)	20.480	48990	0.366 ug/ml
22) T n-Tetracontane (C40)	22.165	41842	0.330 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050523AL\
Data File : FE041747.D
Signal(s) : FID1B.ch
Acq On : 05 May 2023 08:25
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 06 01:25:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 042123.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 07:33:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

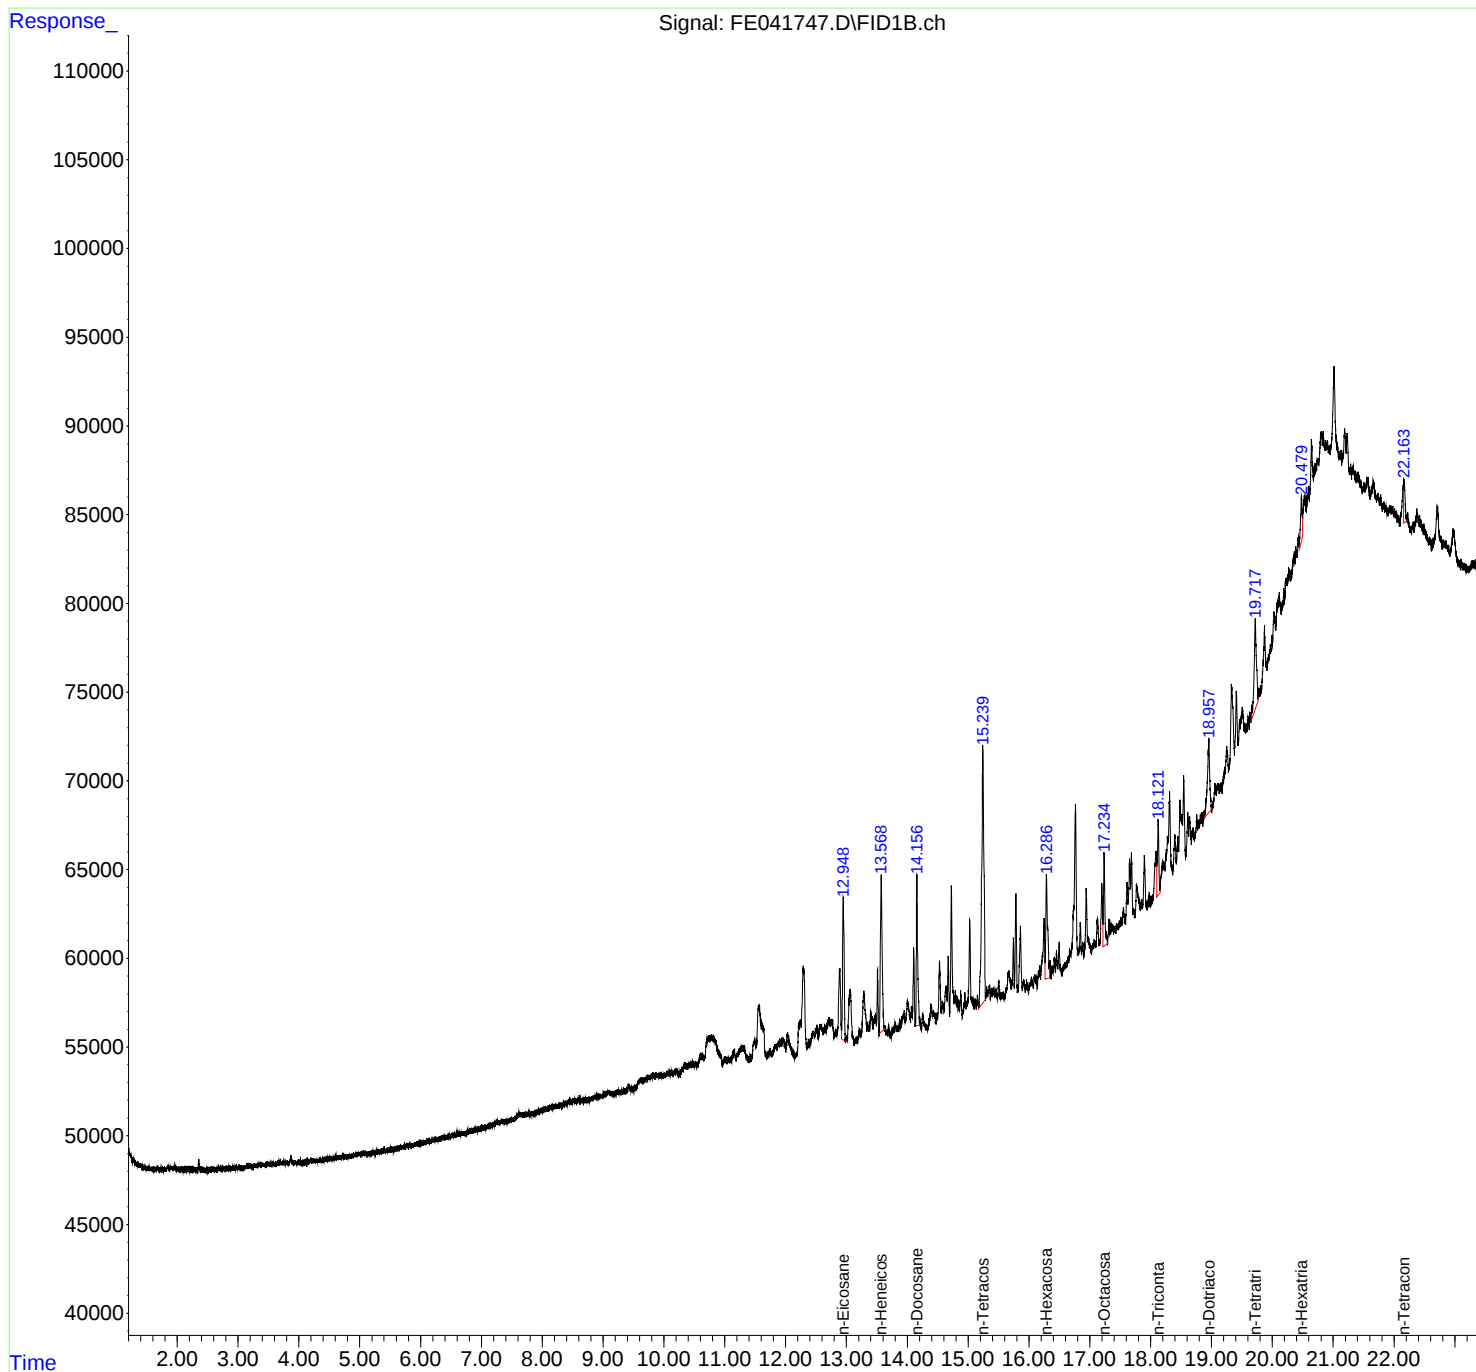


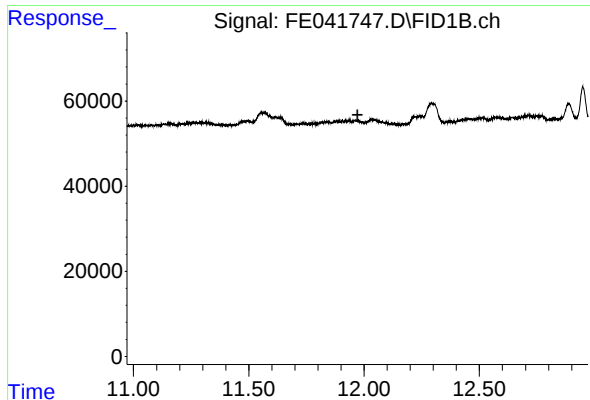

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.972 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

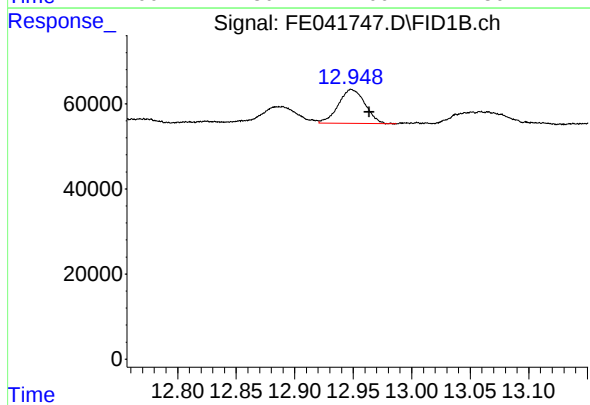


#10 n-Eicosane (C20)

R.T.: 12.949 min
Delta R.T.: -0.015 min
Response: 127343
Conc: 0.79 ug/ml

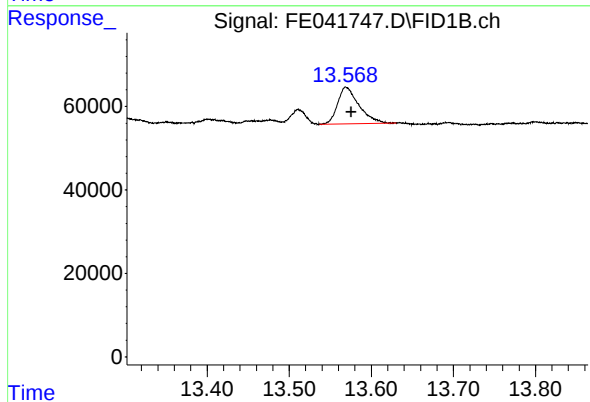


#11 n-Heneicosane (C21)

R.T.: 13.569 min
Delta R.T.: -0.007 min
Response: 159054
Conc: 1.00 ug/ml

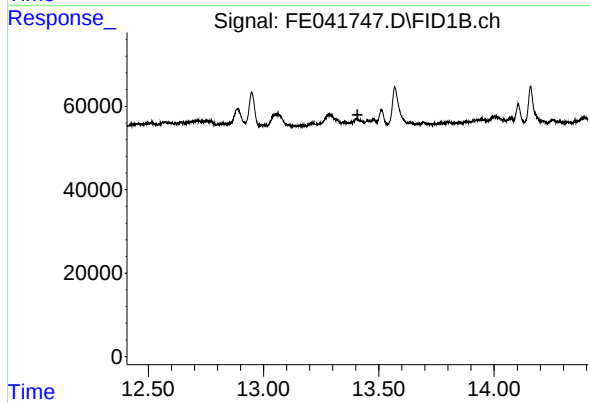

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.408 min
Response: 0
Conc: N.D.

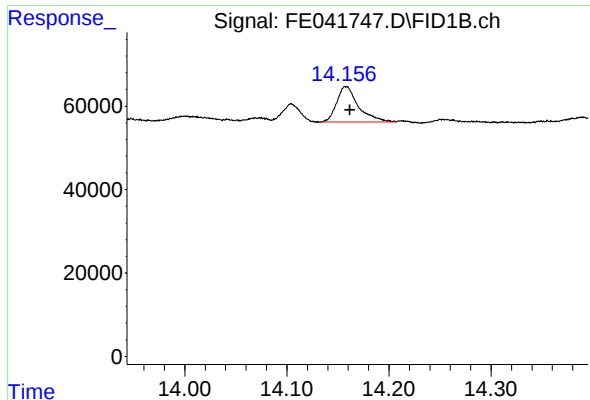

#13 n-Docosane (C22)


R.T.: 14.158 min
Delta R.T.: -0.004 min
Response: 124982
Conc: 0.78 ug/ml

Instrument :
FID_E
ClientSampleId :

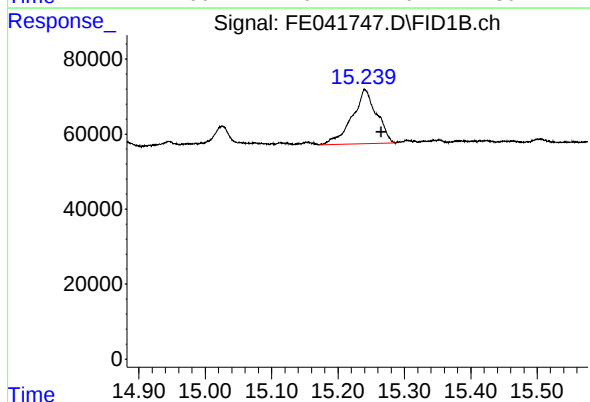


#14 n-Tetracosane (C24)

R.T.: 15.241 min
Delta R.T.: -0.024 min
Response: 369285
Conc: 2.29 ug/ml

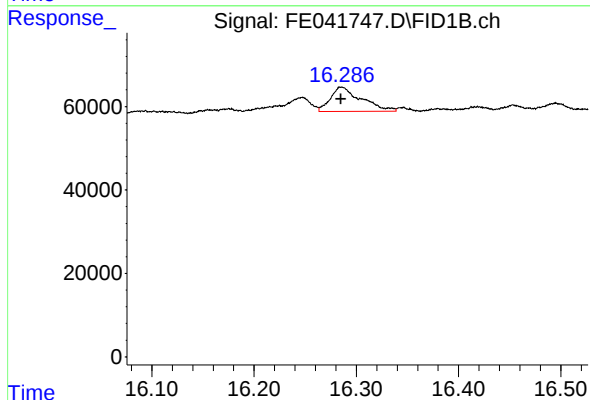


#15 n-Hexacosane (C26)

R.T.: 16.286 min
Delta R.T.: 0.000 min
Response: 122464
Conc: 0.77 ug/ml

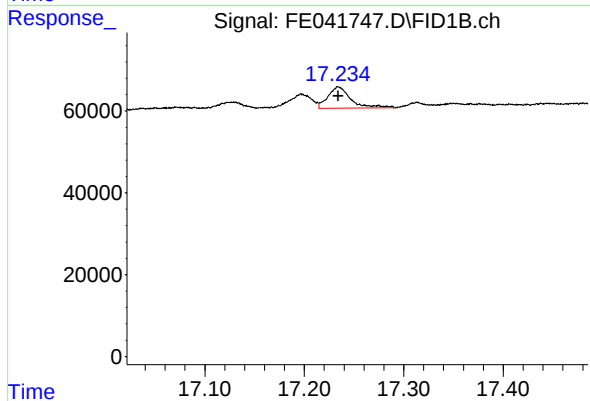

#16 n-Octacosane (C28)


R.T.: 17.234 min
Delta R.T.: 0.000 min
Response: 82668
Conc: 0.54 ug/ml

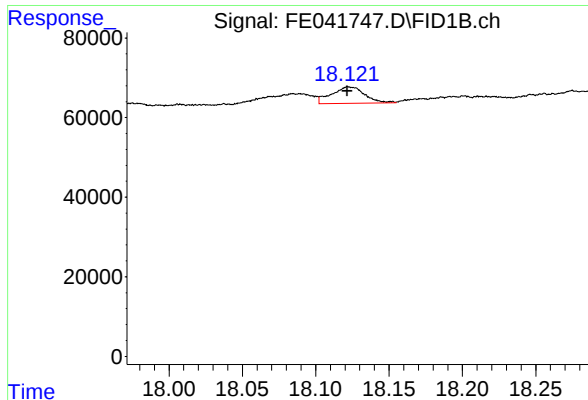

#17 n-Tricontane (C30)


R.T.: 18.123 min
Delta R.T.: 0.000 min
Response: 66229
Conc: 0.43 ug/ml

Instrument :
FID_E
ClientSampleId :

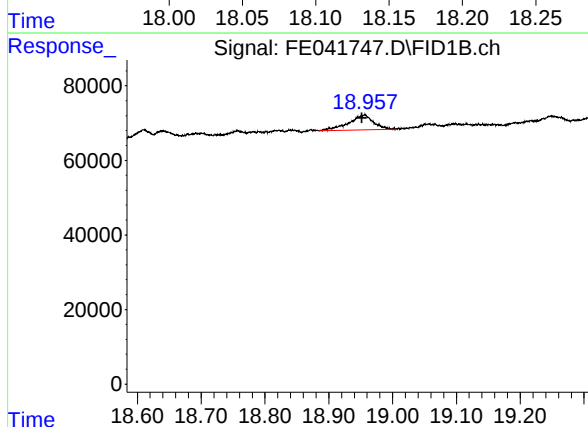


#18 n-Dotriacontane (C32)

R.T.: 18.957 min
Delta R.T.: 0.005 min
Response: 106914
Conc: 0.72 ug/ml

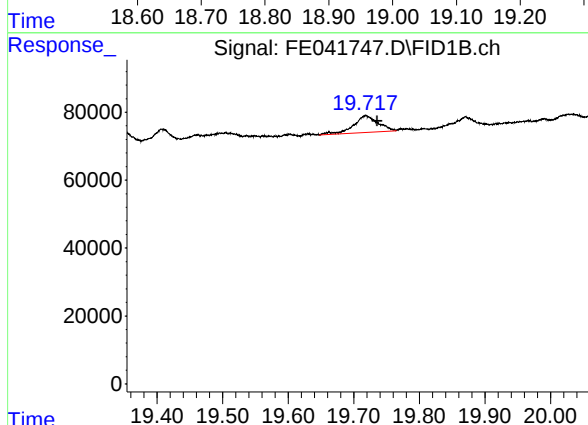


#19 n-Tetratriacontane (C34)

R.T.: 19.718 min
Delta R.T.: -0.018 min
Response: 128902
Conc: 0.91 ug/ml

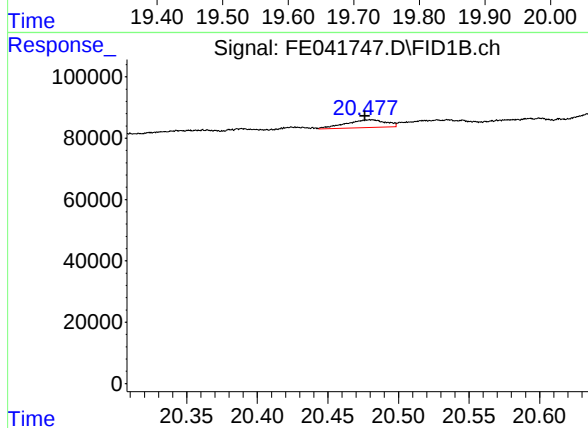

#20 n-Hexatriacontane (C36)

R.T.: 20.480 min
Delta R.T.: 0.004 min
Response: 48990
Conc: 0.37 ug/ml

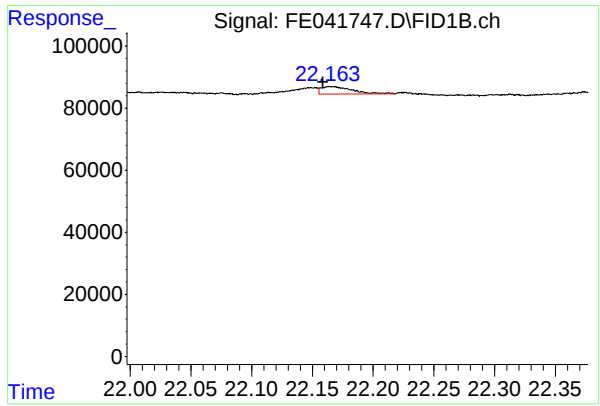

#22 n-Tetracontane (C40)

R.T.: 22.165 min
Delta R.T.: 0.006 min
Response: 41842
Conc: 0.33 ug/ml

Instrument :
FID_E
ClientSampleId :