

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050619\
 Data File : FE029965.D
 Signal(s) : FID1B.CH
 Acq On : 06 May 2019 12:16
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: May 07 02:01:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
 Quant Title :
 QLast Update : Wed Apr 10 08:20:21 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.661	9611791	47.380 ug/ml
Target Compounds			
2) N-DECANE	4.390	11215859	51.040 ug/ml
3) N-DODECANE	6.401	11388319	50.841 ug/ml
4) N-TETRADECANE	8.197	11512219	49.851 ug/ml
5) N-HEXADECANE	9.800	11554076	49.142 ug/ml
6) N-OCTADECANE	11.245	11525871	48.541 ug/ml
7) N-EICOSANE	12.559	11348741	47.896 ug/ml
8) N-DOCOSANE	13.761	11187896	47.640 ug/ml
10) N-TETRACOSANE	14.869	10980704	47.314 ug/ml
11) N-HEXACOSANE	15.892	10767746	46.695 ug/ml
12) N-OCTACOSANE	16.845	10553318	45.832 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050619\
Data File : FE029965.D
Signal(s) : FID1B.CH
Acq On : 06 May 2019 12:16
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: May 07 02:01:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
Quant Title :
QLast Update : Wed Apr 10 08:20:21 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

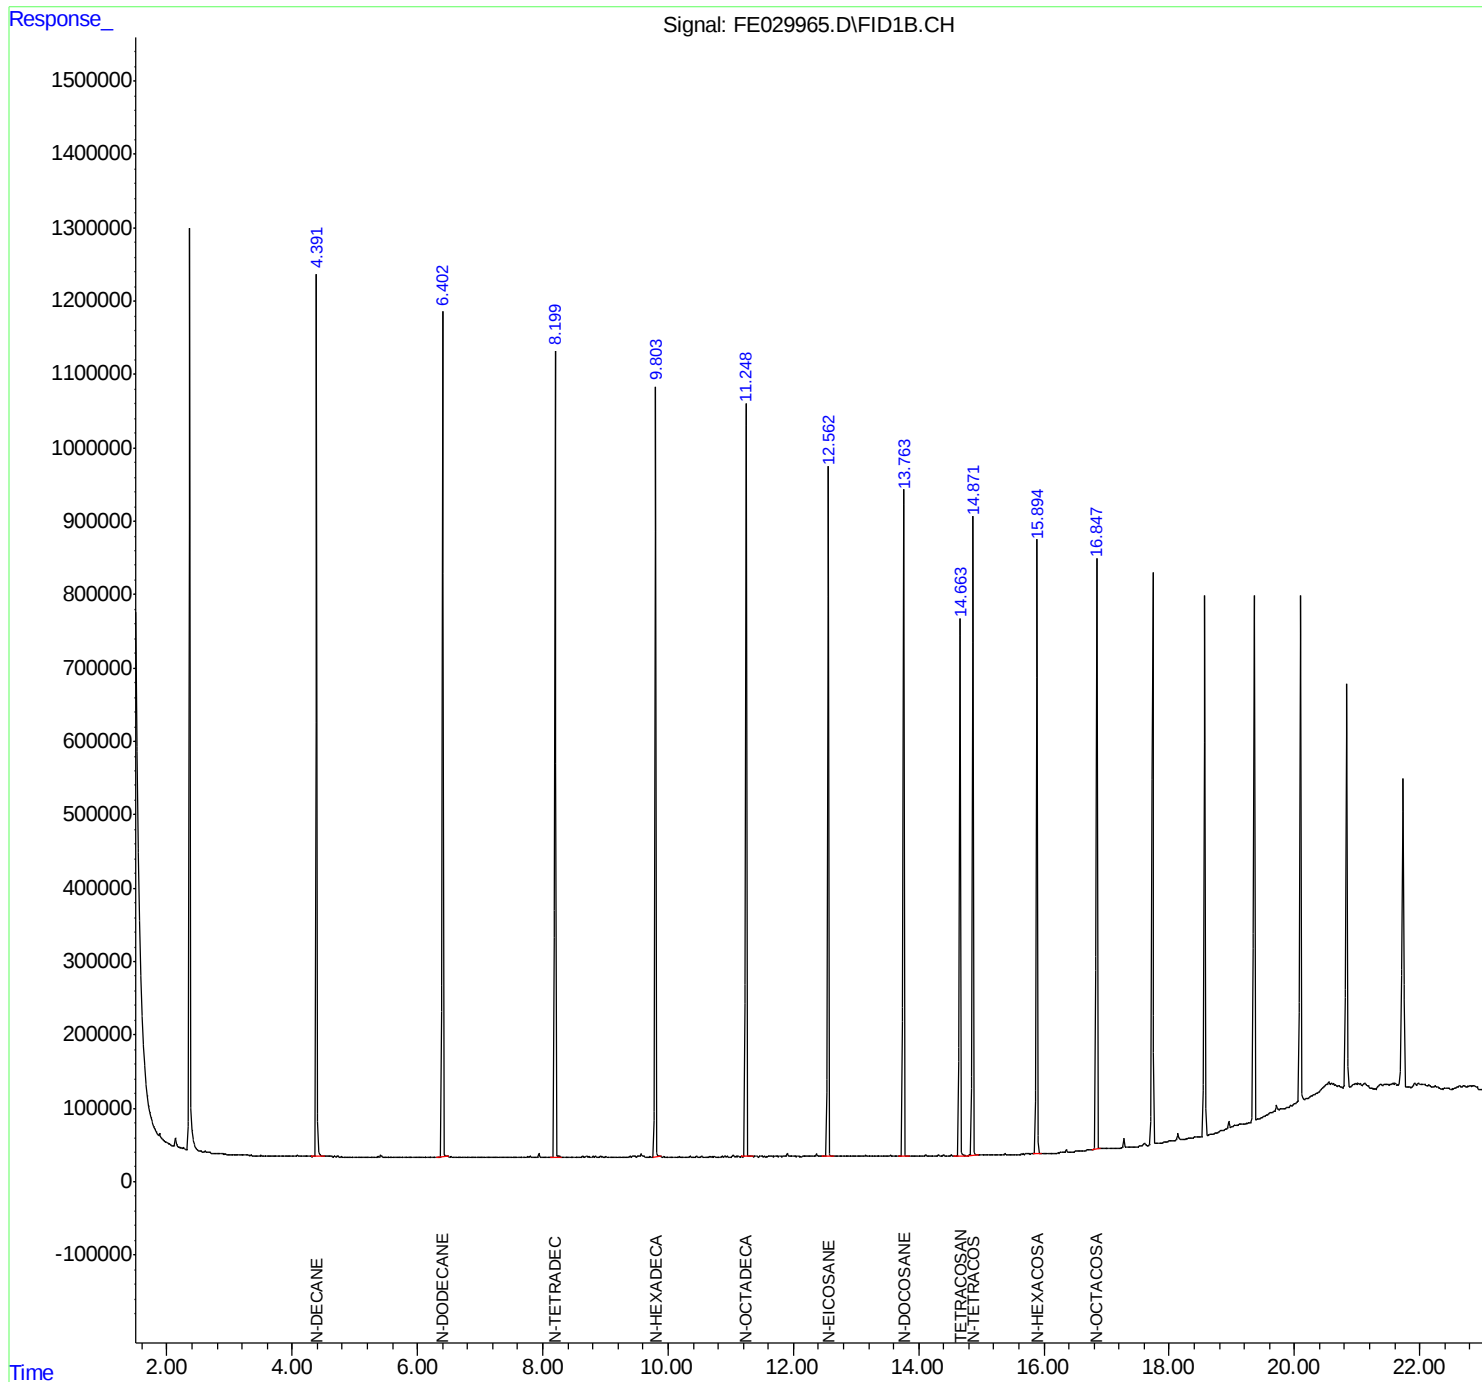

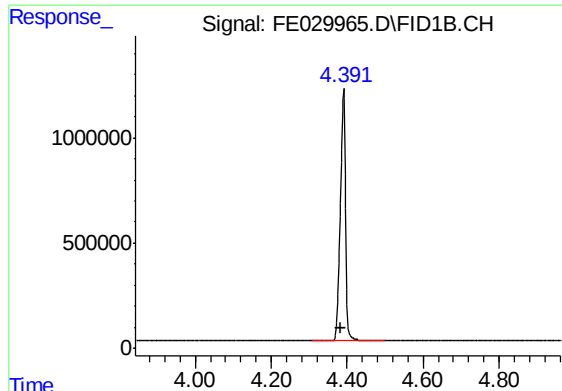


#2 N-DECANE

R.T.: 4.390 min
Delta R.T.: 0.005 min
Response: 11215859
Conc: 51.04 ug/ml

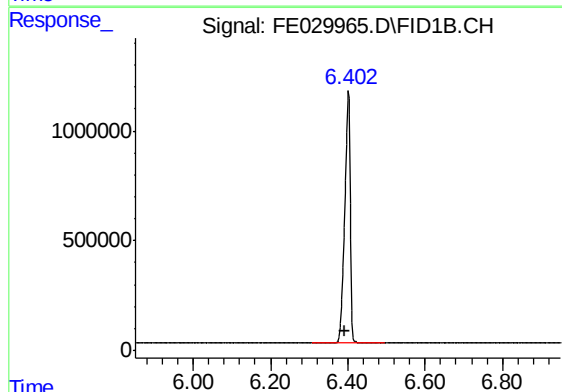


#3 N-DODECANE

R.T.: 6.401 min
Delta R.T.: 0.009 min
Response: 11388319
Conc: 50.84 ug/ml

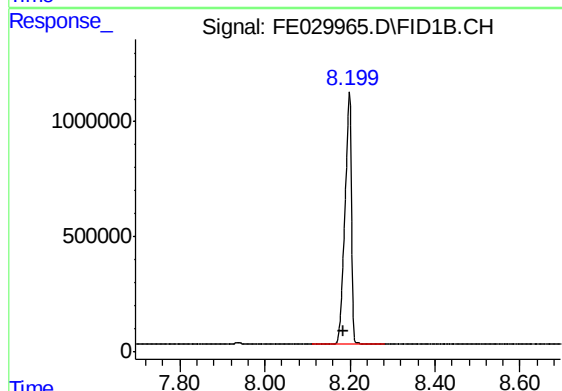


#4 N-TETRADECANE

R.T.: 8.197 min
Delta R.T.: 0.013 min
Response: 11512219
Conc: 49.85 ug/ml

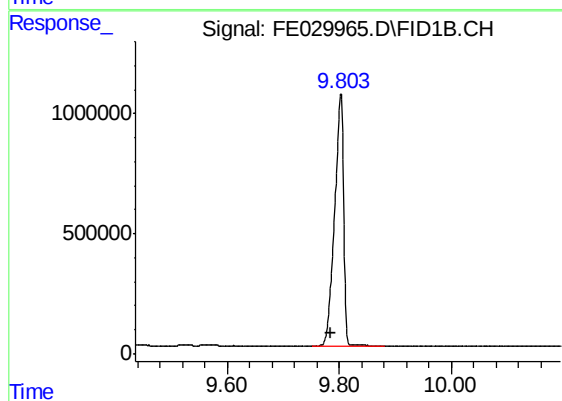


#5 N-HEXADECANE

R.T.: 9.800 min
Delta R.T.: 0.017 min
Response: 11554076
Conc: 49.14 ug/ml

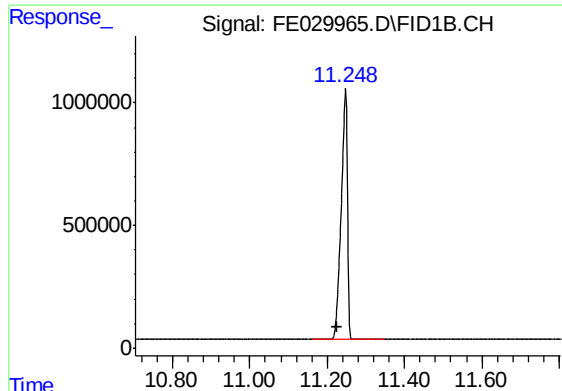


#6 N-OCTADECANE

R.T.: 11.245 min
Delta R.T.: 0.019 min
Response: 11525871
Conc: 48.54 ug/ml

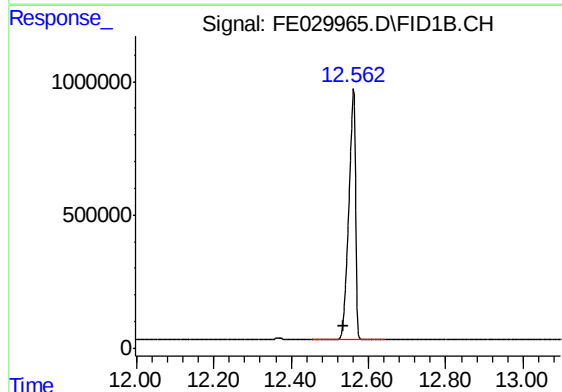


#7 N-EICOSANE

R.T.: 12.559 min
Delta R.T.: 0.023 min
Response: 11348741
Conc: 47.90 ug/ml

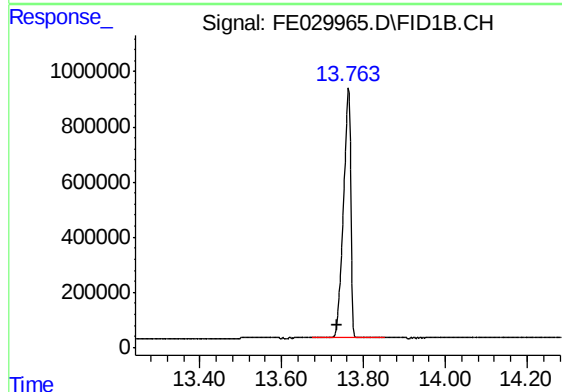


#8 N-DOCOSANE

R.T.: 13.761 min
Delta R.T.: 0.025 min
Response: 11187896
Conc: 47.64 ug/ml

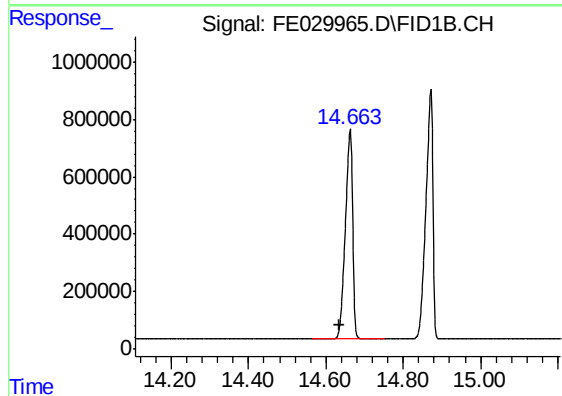


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.661 min
Delta R.T.: 0.024 min
Response: 9611791
Conc: 47.38 ug/ml

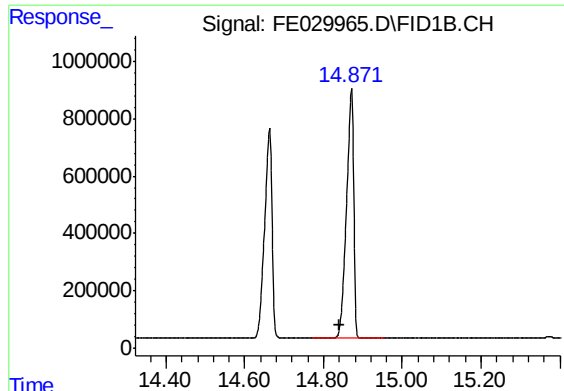


#10 N-TETRACOSANE

R.T.: 14.869 min
Delta R.T.: 0.029 min
Response: 10980704
Conc: 47.31 ug/ml

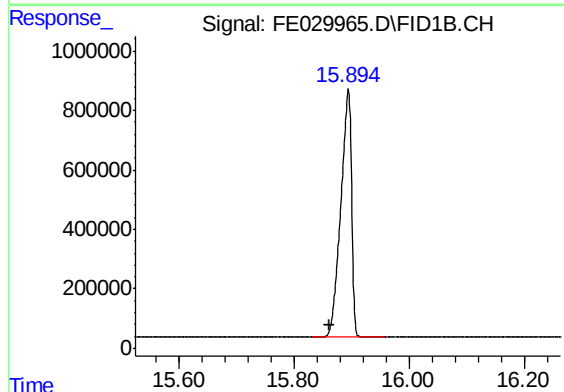

#11 N-HEXACOSANE

R.T.: 15.892 min
Delta R.T.: 0.030 min
Response: 10767746
Conc: 46.69 ug/ml

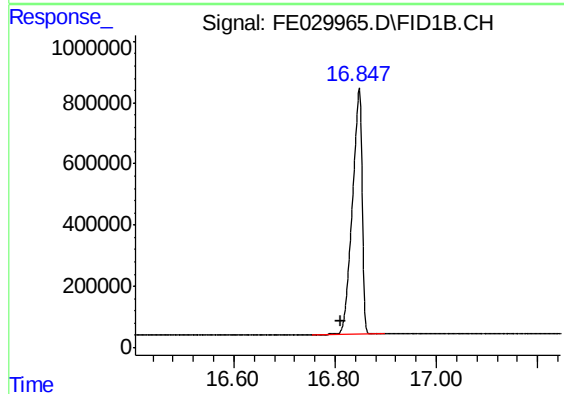

#12 N-OCTACOSANE

R.T.: 16.845 min
Delta R.T.: 0.032 min
Response: 10553318
Conc: 45.83 ug/ml