

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050621\
 Data File : FE033735.D
 Signal(s) : FID1B.CH
 Acq On : 06 May 2021 12:28
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 07 03:32:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
 Quant Title :
 QLast Update : Thu May 06 02:18:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.734	19904941	49.248 ug/ml
Target Compounds			
2) N-DECANE	4.471	21377780	49.830 ug/ml
3) N-DODECANE	6.483	21799413	49.818 ug/ml
4) N-TETRADECANE	8.280	22352597	49.621 ug/ml
5) N-HEXADECANE	9.881	22267055	49.410 ug/ml
6) N-OCTADECANE	11.325	22757863	49.405 ug/ml
7) N-EICOSANE	12.636	22644477	49.329 ug/ml
8) N-DOCOSANE	13.836	22672537	49.171 ug/ml
10) N-TETRACOSANE	14.940	22677837	49.115 ug/ml
11) N-HEXACOSANE	15.961	22425974	48.875 ug/ml
12) N-OCTACOSANE	16.913	22234863	48.479 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050621\
Data File : FE033735.D
Signal(s) : FID1B.CH
Acq On : 06 May 2021 12:28
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 07 03:32:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE050521.M
Quant Title :
QLast Update : Thu May 06 02:18:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

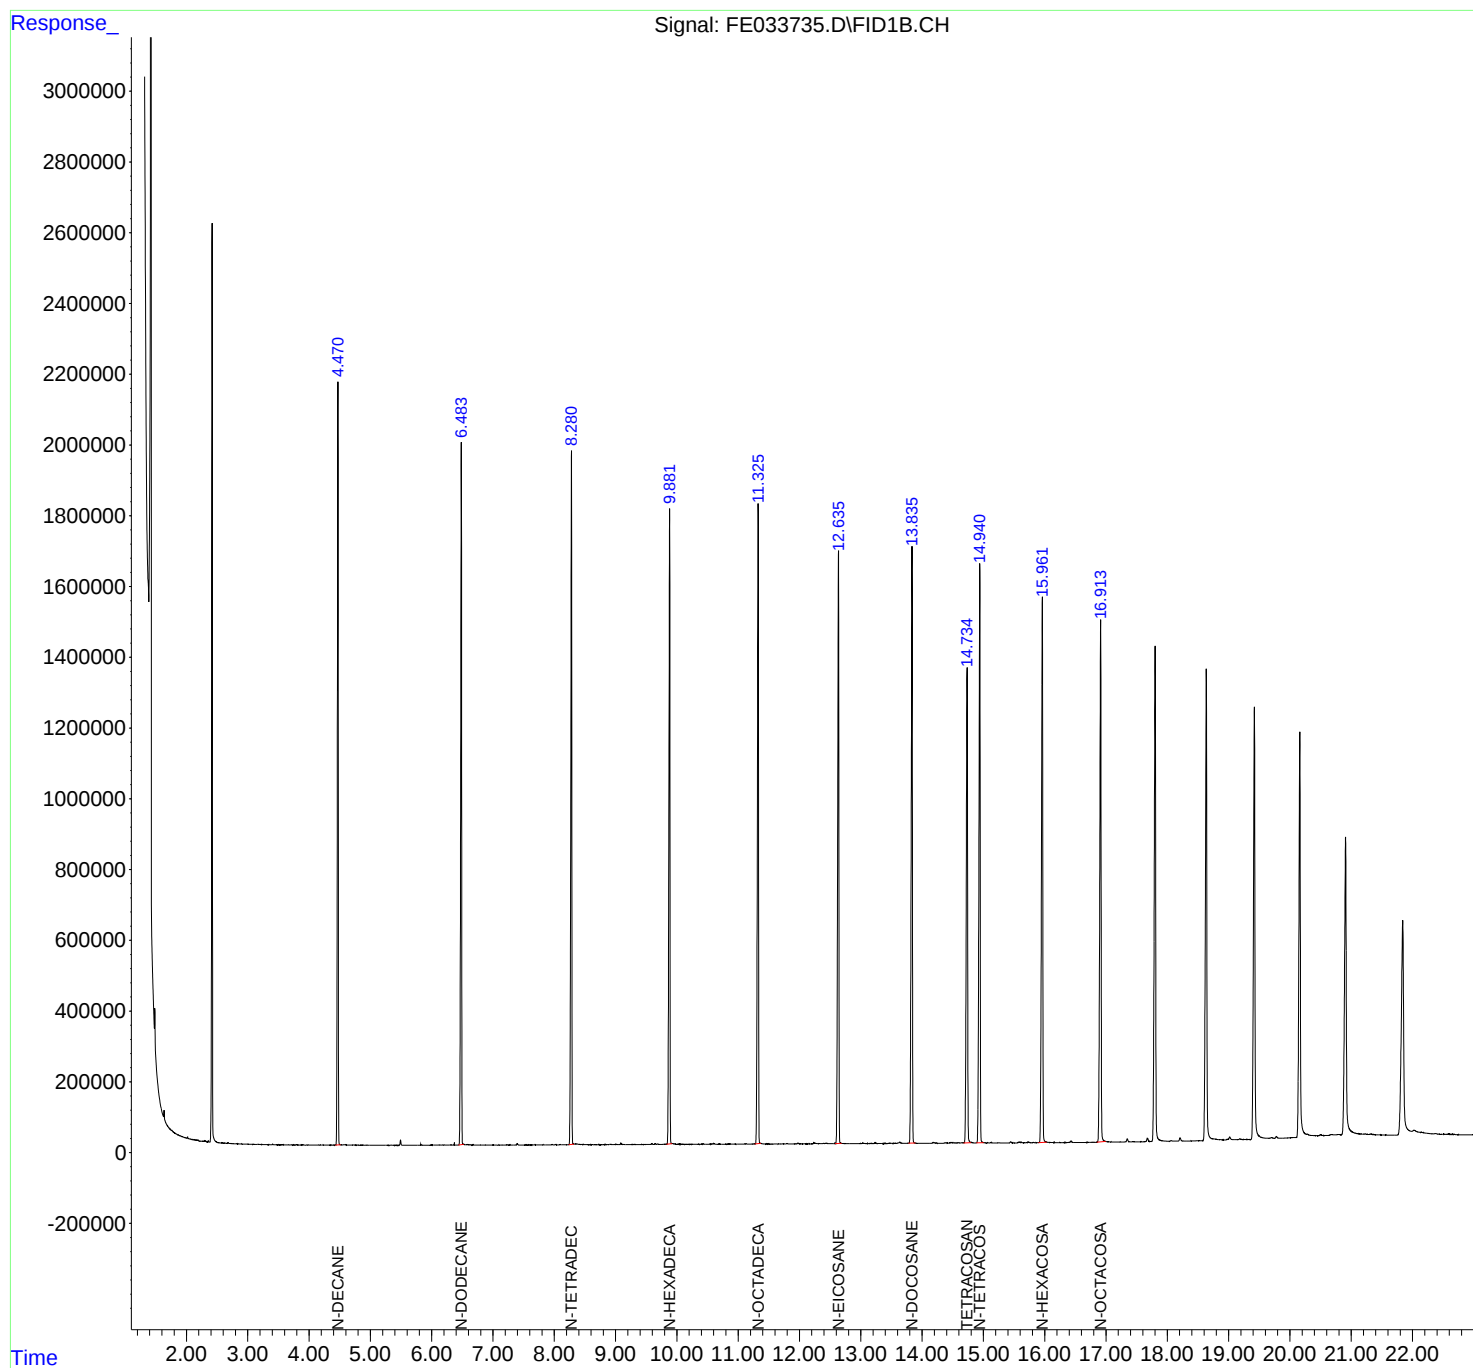

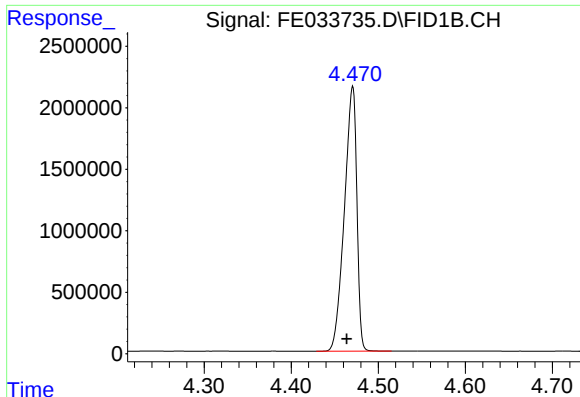


#2 N-DECANE

R.T.: 4.471 min
Delta R.T.: 0.007 min
Response: 21377780
Conc: 49.83 ug/ml

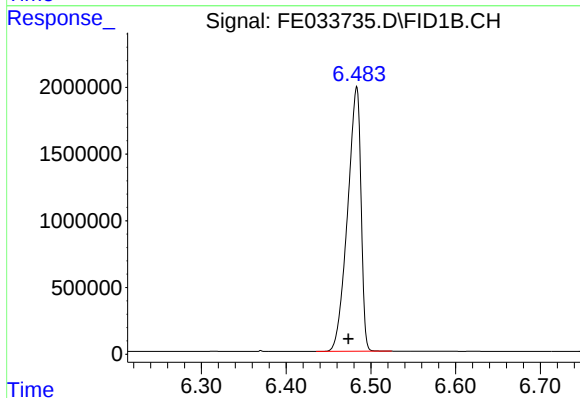


#3 N-DODECANE

R.T.: 6.483 min
Delta R.T.: 0.010 min
Response: 21799413
Conc: 49.82 ug/ml

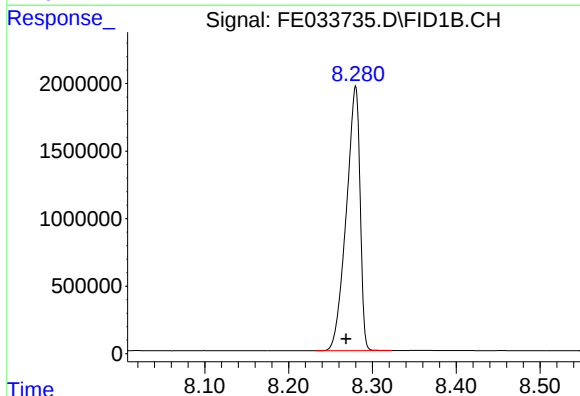


#4 N-TETRADECANE

R.T.: 8.280 min
Delta R.T.: 0.011 min
Response: 22352597
Conc: 49.62 ug/ml

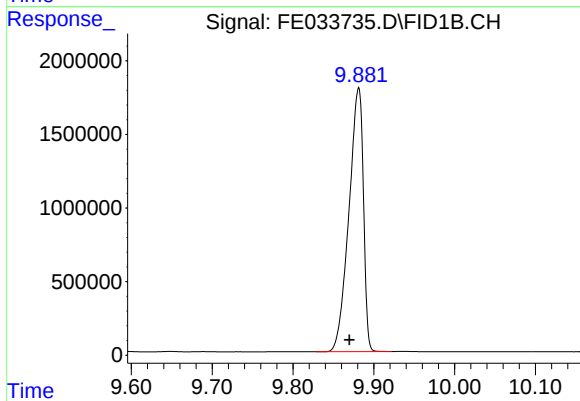


#5 N-HEXADECANE

R.T.: 9.881 min
Delta R.T.: 0.011 min
Response: 22267055
Conc: 49.41 ug/ml

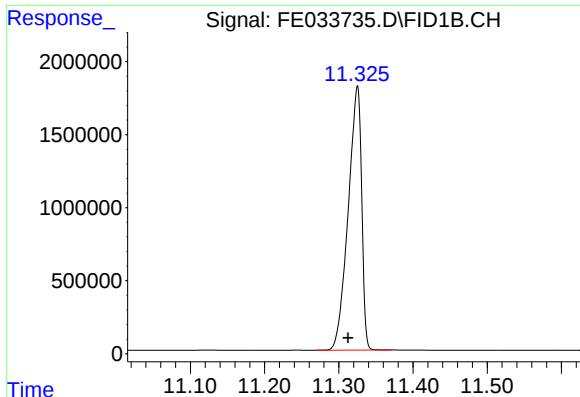


#6 N-OCTADECANE

R.T.: 11.325 min
Delta R.T.: 0.013 min
Response: 22757863
Conc: 49.41 ug/ml

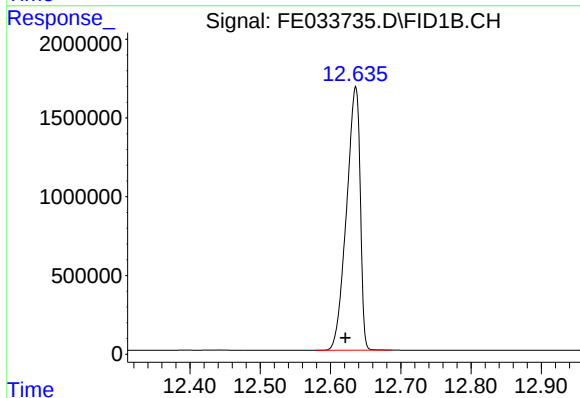


#7 N-EICOSANE

R.T.: 12.636 min
Delta R.T.: 0.014 min
Response: 22644477
Conc: 49.33 ug/ml

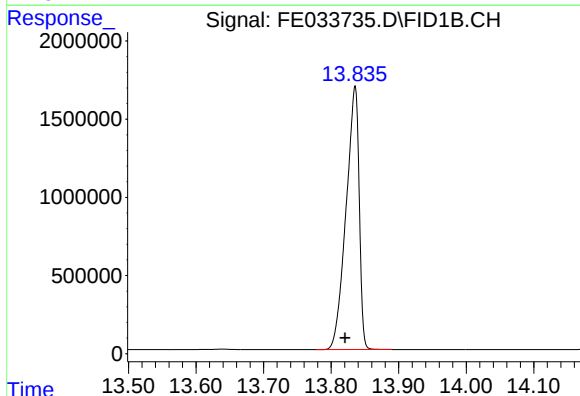


#8 N-DOCOSANE

R.T.: 13.836 min
Delta R.T.: 0.014 min
Response: 22672537
Conc: 49.17 ug/ml

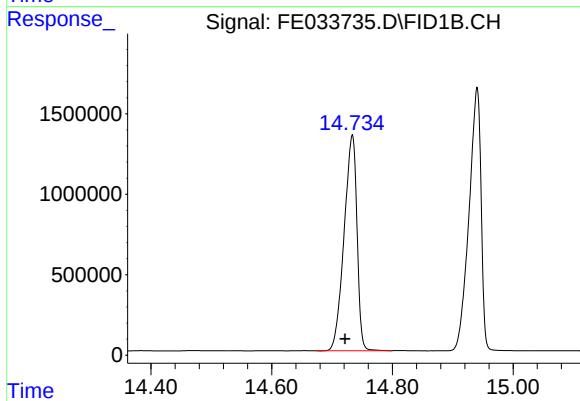


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.734 min
Delta R.T.: 0.012 min
Response: 19904941
Conc: 49.25 ug/ml

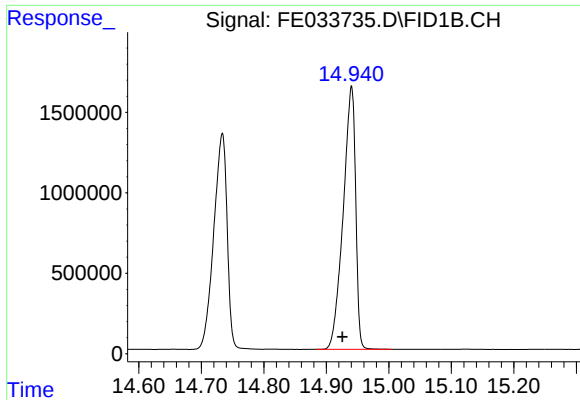


#10 N-TETRACOSANE

R.T.: 14.940 min
Delta R.T.: 0.015 min
Response: 22677837
Conc: 49.12 ug/ml

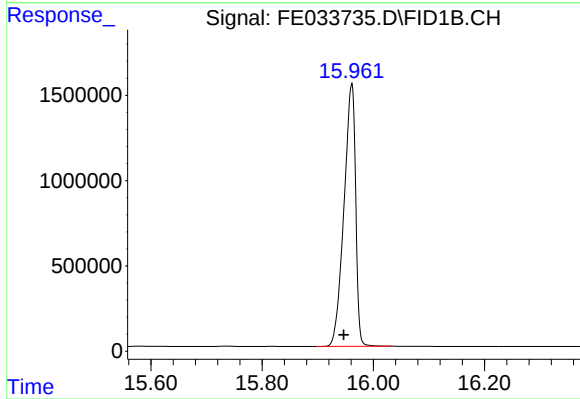

#11 N-HEXACOSANE

R.T.: 15.961 min
Delta R.T.: 0.014 min
Response: 22425974
Conc: 48.88 ug/ml

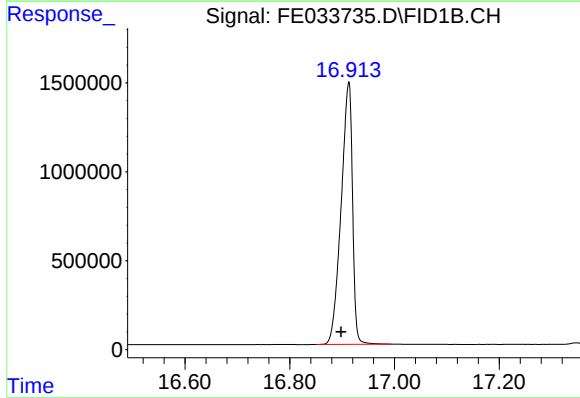

#12 N-OCTACOSANE

R.T.: 16.913 min
Delta R.T.: 0.015 min
Response: 22234863
Conc: 48.48 ug/ml