

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050719\
Data File : FE029995.D
Signal(s) : FID1B.CH
Acq On : 07 May 2019 9:15
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: May 08 02:19:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
Quant Title :
QLast Update : Wed Apr 10 08:20:21 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.549	197180	0.887 ug/ml
16)	N-HEXATRIACONTANE	20.105	786439	3.785 ug/ml
18)	N-TETRACONTANE	21.723f	1757939	9.248 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050719\
Data File : FE029995.D
Signal(s) : FID1B.CH
Acq On : 07 May 2019 9:15
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: May 08 02:19:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
Quant Title :
QLast Update : Wed Apr 10 08:20:21 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

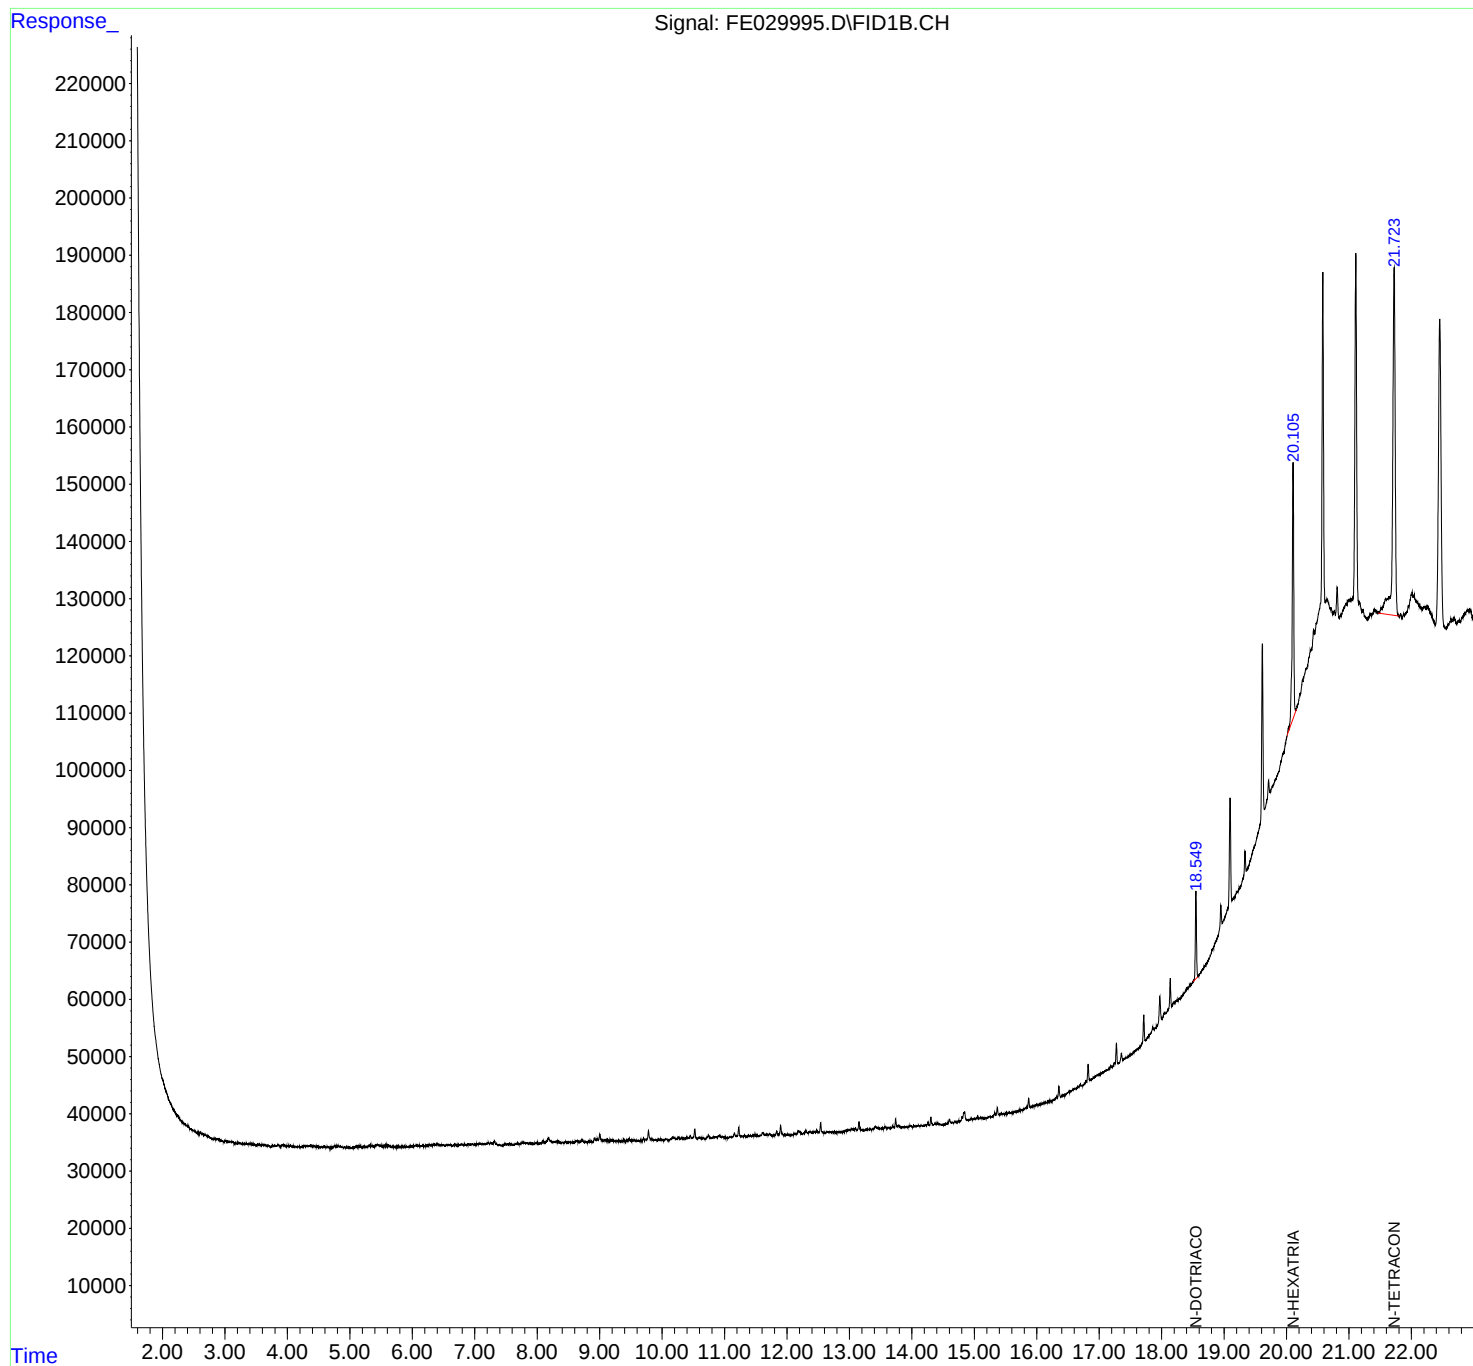


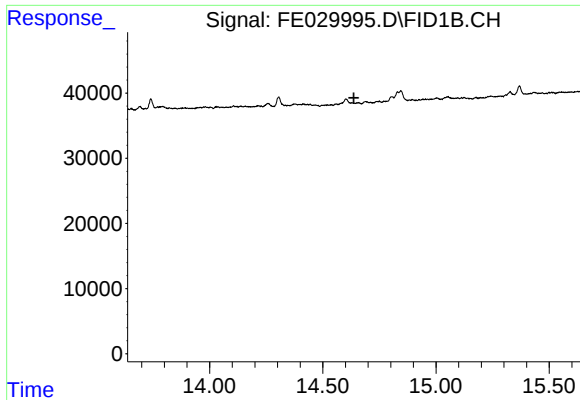

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.637 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2

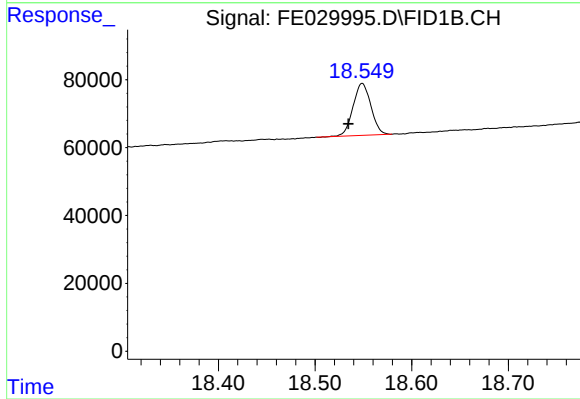


#14 N-DOTRIACONTANE

R.T.: 18.549 min
Delta R.T.: 0.014 min
Response: 197180
Conc: 0.89 ug/ml

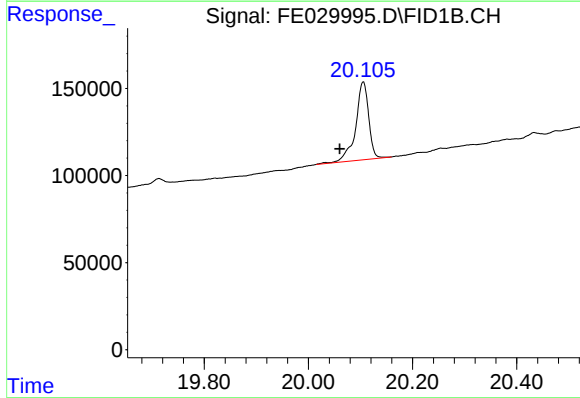

#16 N-HEXATRIACONTANE

R.T.: 20.105 min
Delta R.T.: 0.045 min
Response: 786439
Conc: 3.79 ug/ml

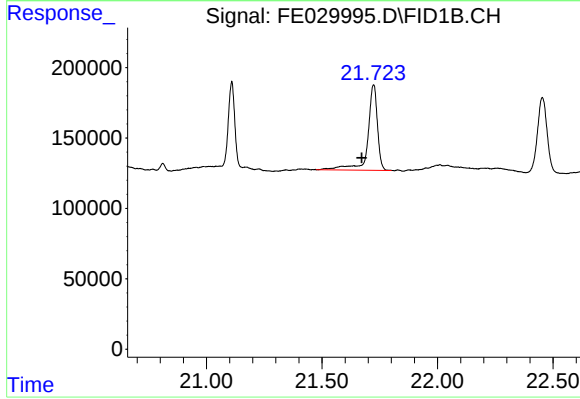

#18 N-TETRACONTANE

R.T.: 21.723 min
Delta R.T.: 0.050 min
Response: 1757939
Conc: 9.25 ug/ml