

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050719\
 Data File : FE029999.D
 Signal(s) : FID1B.CH
 Acq On : 07 May 2019 11:48
 Operator : AJ\SJ
 Sample : K2672-04 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 SB-02-COMP

Integration File: autoint1.e
 Quant Time: May 08 02:19:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
 Quant Title :
 QLast Update : Wed Apr 10 08:20:21 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.642	323684	1.596 ug/ml
Target Compounds			
7) N-EICOSANE	12.504	235494	0.994 ug/ml
10) N-TETRACOSANE	14.827	695477	2.997 ug/ml
12) N-OCTACOSANE	16.800	1266398	5.500 ug/ml
13) N-TRIACONTANE	17.692	160836	0.700 ug/ml
14) N-DOTRIACONTANE	18.558	331720	1.492 ug/ml
15) N-TETRATRIACONTANE	19.343	328731	1.519 ug/ml
16) N-HEXATRIACONTANE	20.089	243796	1.173 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050719\
Data File : FE029999.D
Signal(s) : FID1B.CH
Acq On : 07 May 2019 11:48
Operator : AJ\SJ
Sample : K2672-04 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SB-02-COMP

Integration File: autoint1.e
Quant Time: May 08 02:19:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
Quant Title :
QLast Update : Wed Apr 10 08:20:21 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

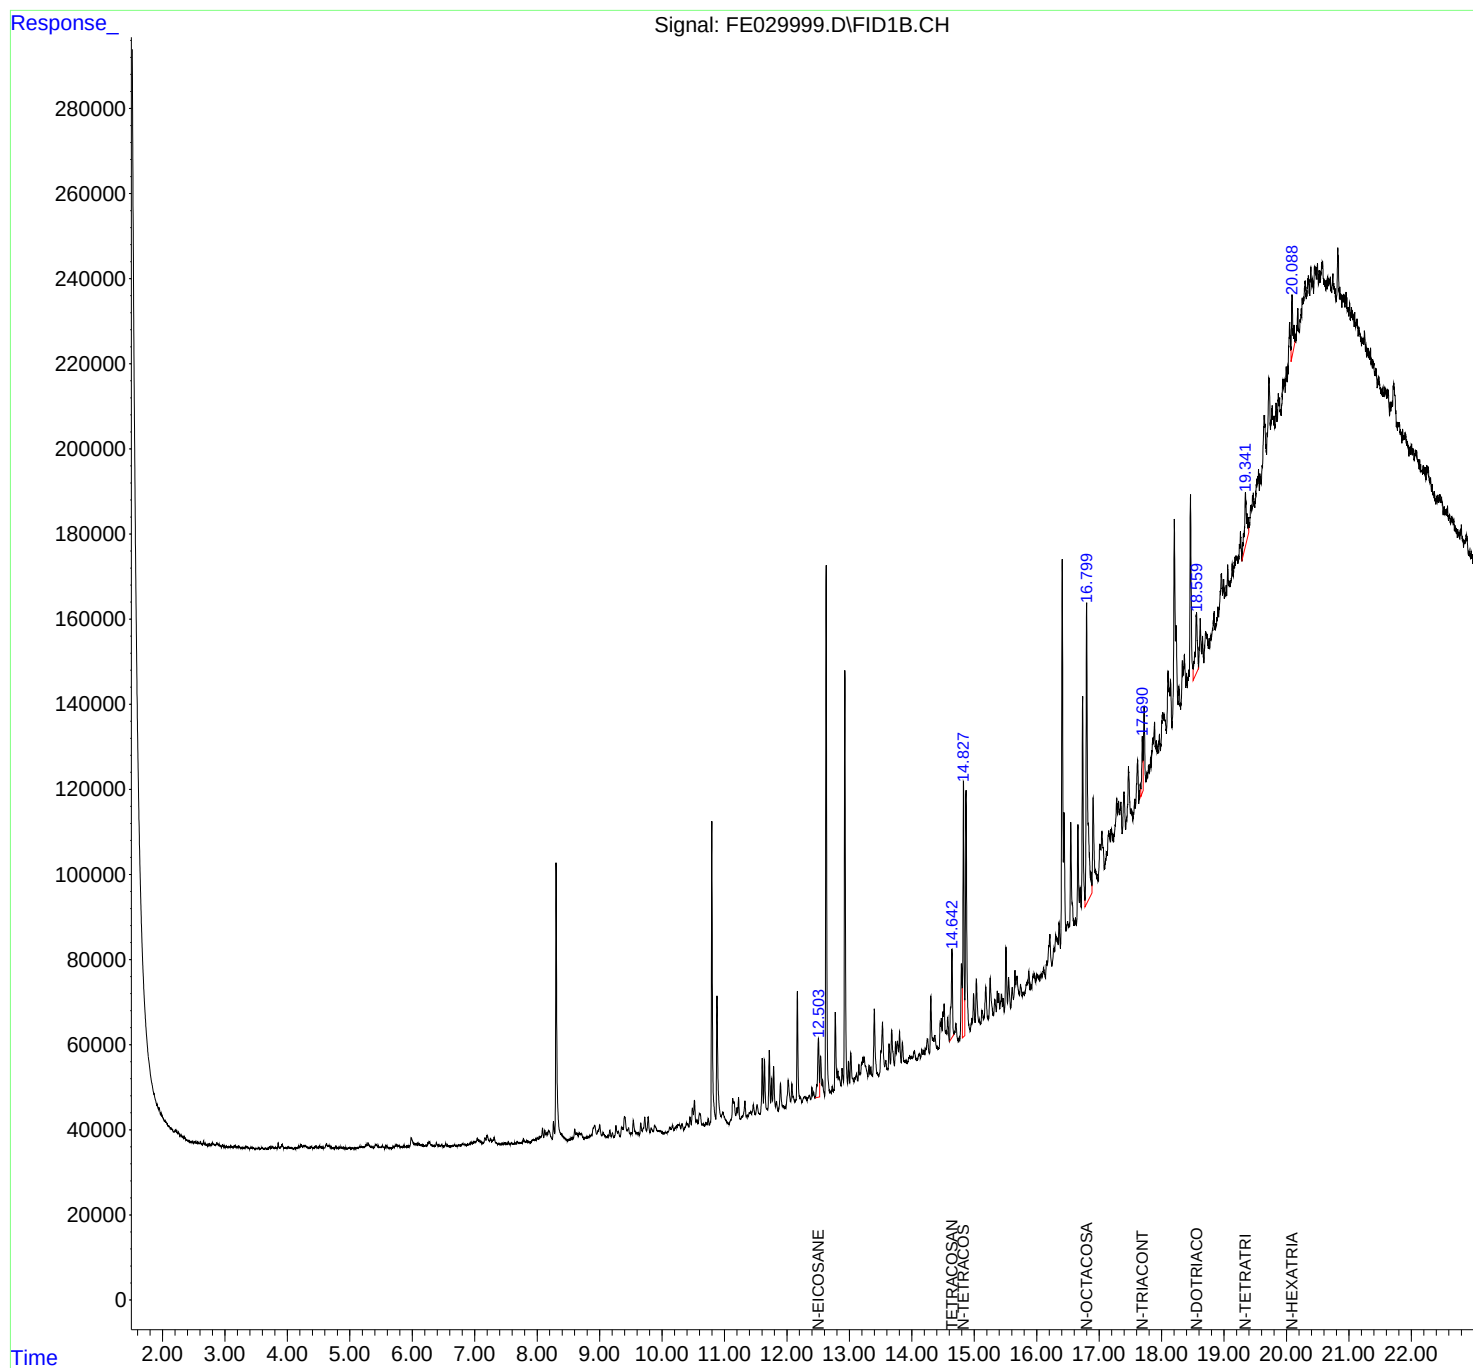


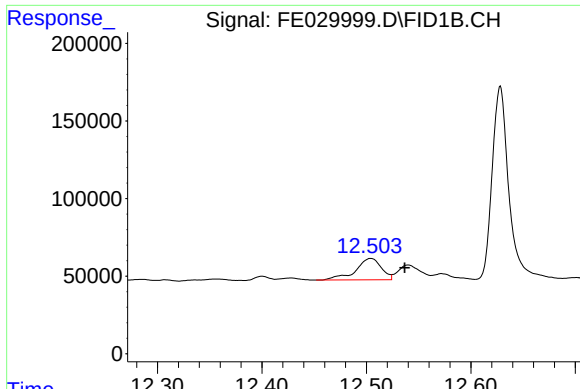

#7 N-EICOSANE


R.T.: 12.504 min
Delta R.T.: -0.033 min
Response: 235494
Conc: 0.99 ug/ml

Instrument :
FID_E
ClientSampleId :
SB-02-COMP

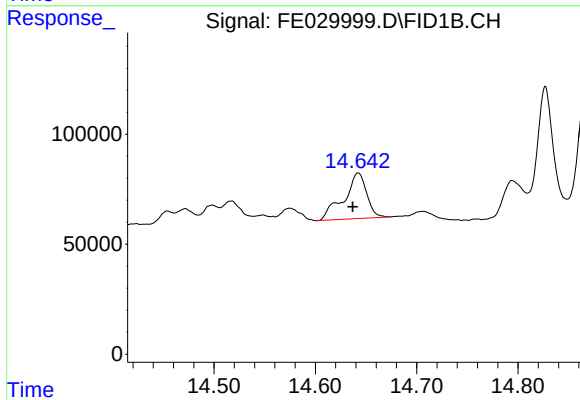


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.642 min
Delta R.T.: 0.005 min
Response: 323684
Conc: 1.60 ug/ml

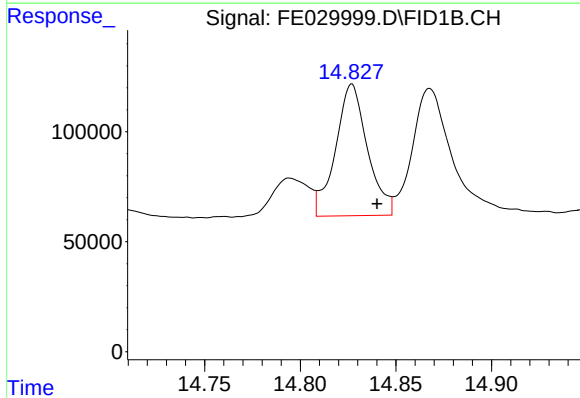


#10 N-TETRACOSANE

R.T.: 14.827 min
Delta R.T.: -0.013 min
Response: 695477
Conc: 3.00 ug/ml

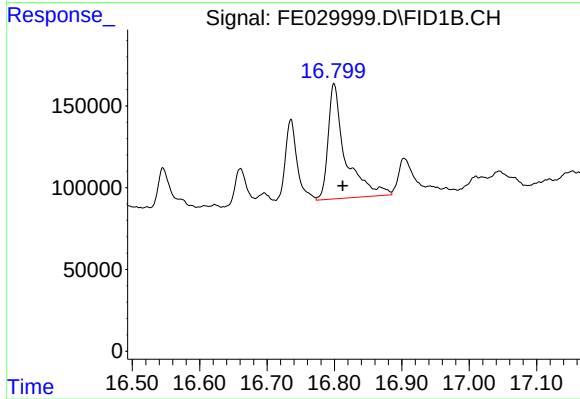

#12 N-OCTACOSANE


R.T.: 16.800 min
Delta R.T.: -0.013 min
Response: 1266398
Conc: 5.50 ug/ml

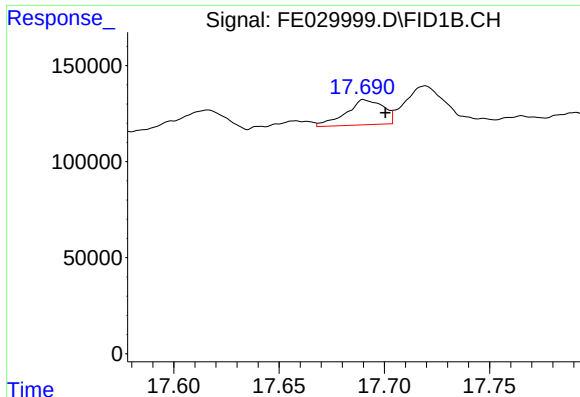

#13 N-TRIACONTANE


R.T.: 17.692 min
Delta R.T.: -0.008 min
Response: 160836
Conc: 0.70 ug/ml

Instrument :
FID_E
ClientSampleId :
SB-02-COMP

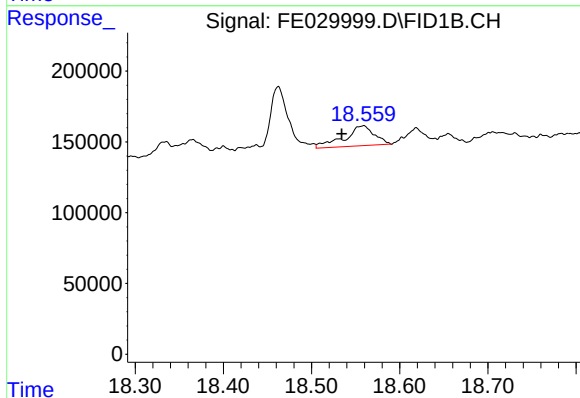


#14 N-DOTRIACONTANE

R.T.: 18.558 min
Delta R.T.: 0.023 min
Response: 331720
Conc: 1.49 ug/ml

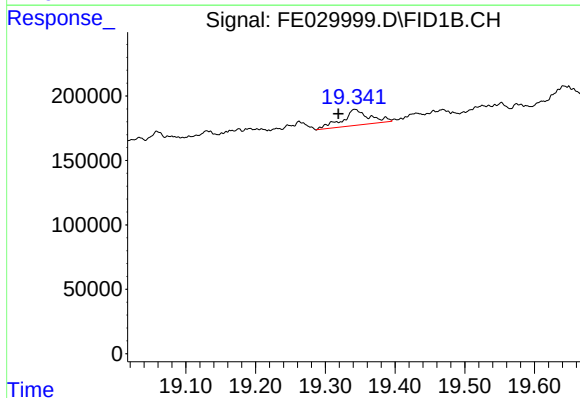

#15 N-TETRATRIACONTANE

R.T.: 19.343 min
Delta R.T.: 0.024 min
Response: 328731
Conc: 1.52 ug/ml

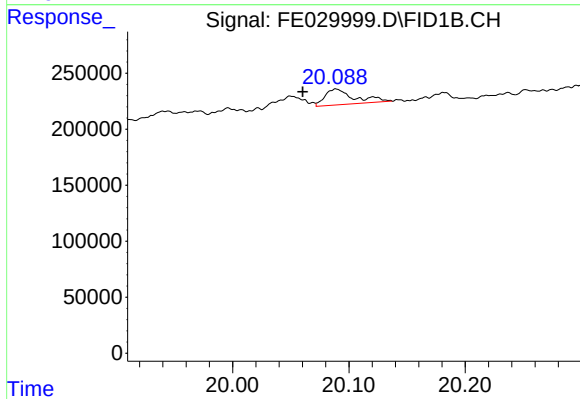

#16 N-HEXATRIACONTANE

R.T.: 20.089 min
Delta R.T.: 0.029 min
Response: 243796
Conc: 1.17 ug/ml