

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050719\
 Data File : FE030003.D
 Signal(s) : FID1B.CH
 Acq On : 07 May 2019 14:02
 Operator : AJ\SJ
 Sample : K2703-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 P-3-OW(0-10)

Integration File: autoint1.e
 Quant Time: May 08 02:20:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
 Quant Title :
 QLast Update : Wed Apr 10 08:20:21 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	2604394	12.838 ug/ml
Target Compounds			
7) N-EICOSANE	12.540	291104	1.229 ug/ml
8) N-DOCOSANE	13.740	186740	0.795 ug/ml
10) N-TETRACOSANE	14.828	1728837	7.449 ug/ml
11) N-HEXACOSANE	15.873	226062	0.980 ug/ml
12) N-OCTACOSANE	16.827	1037611	4.506 ug/ml
13) N-TRIACONTANE	17.718	1025265	4.460 ug/ml
14) N-DOTRIACONTANE	18.551	612389	2.754 ug/ml
15) N-TETRATRIACONTANE	19.339	67424	0.312 ug/ml
18) N-TETRACONTANE	21.714	1393574	7.331 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE050719\
Data File : FE030003.D
Signal(s) : FID1B.CH
Acq On : 07 May 2019 14:02
Operator : AJ\SJ
Sample : K2703-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
P-3-OW(0-10)

Integration File: autoint1.e
Quant Time: May 08 02:20:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE041019.M
Quant Title :
QLast Update : Wed Apr 10 08:20:21 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

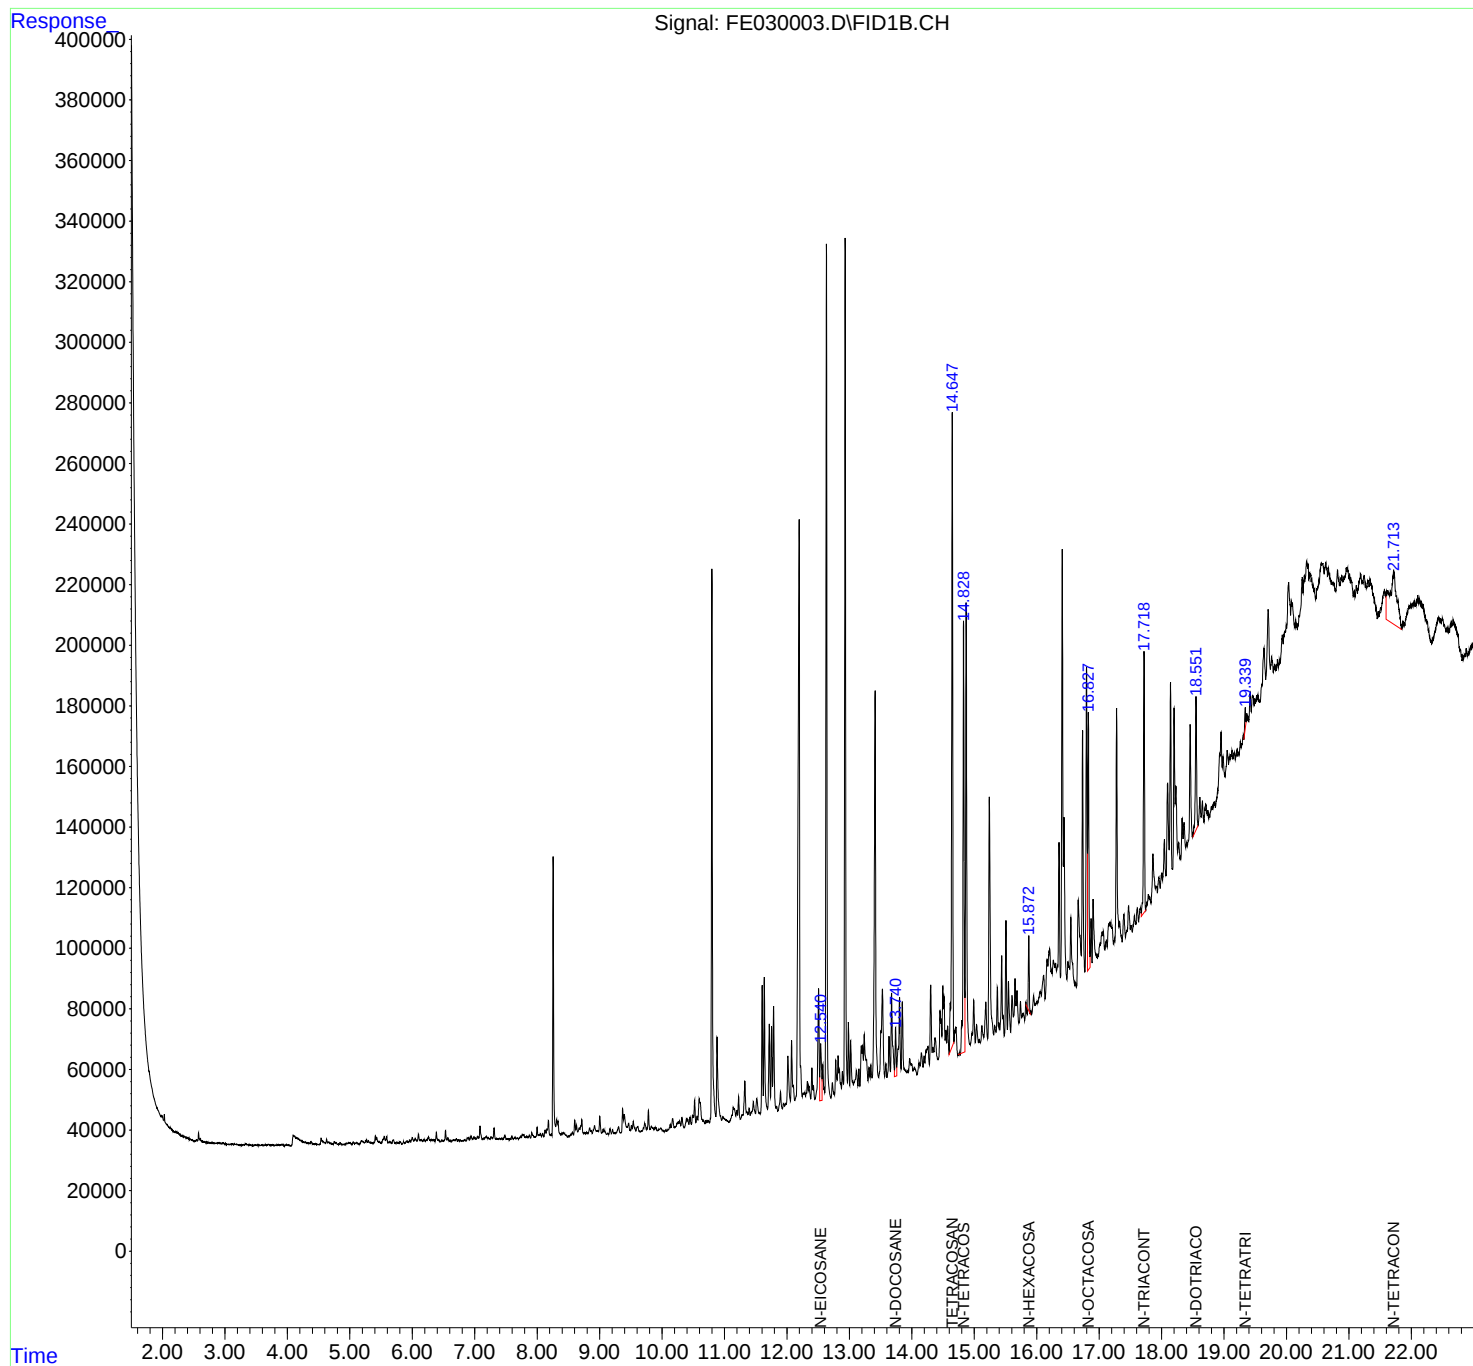


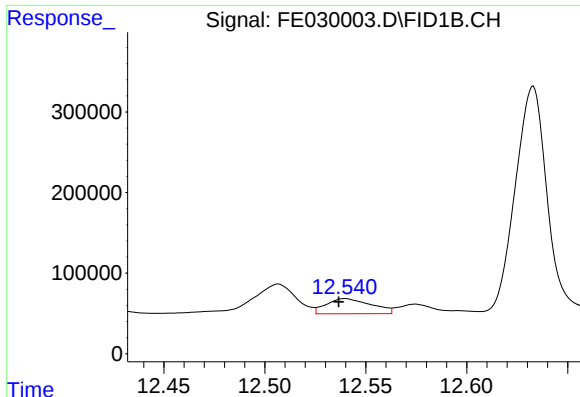

#7 N-EICOSANE


R.T.: 12.540 min
Delta R.T.: 0.003 min
Response: 291104
Conc: 1.23 ug/ml

Instrument :
FID_E
ClientSampleId :
P-3-OW(0-10)

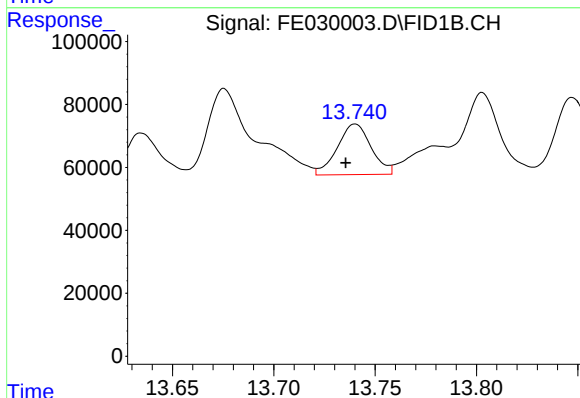


#8 N-DOCOSANE

R.T.: 13.740 min
Delta R.T.: 0.005 min
Response: 186740
Conc: 0.80 ug/ml

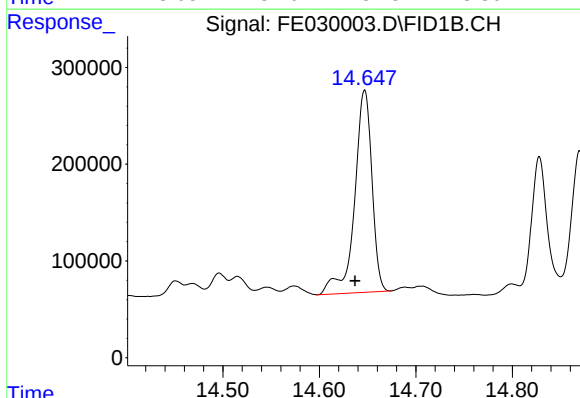


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.647 min
Delta R.T.: 0.010 min
Response: 2604394
Conc: 12.84 ug/ml

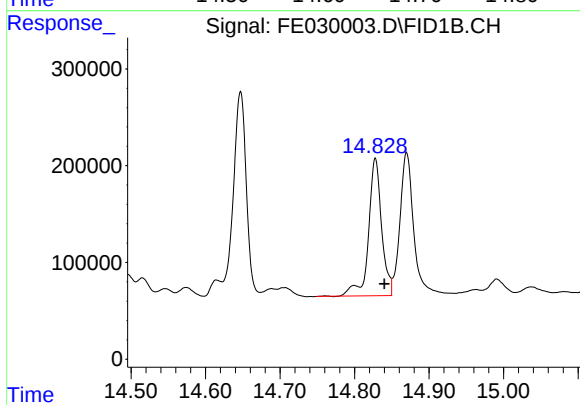

#10 N-TETRACOSANE


R.T.: 14.828 min
Delta R.T.: -0.012 min
Response: 1728837
Conc: 7.45 ug/ml

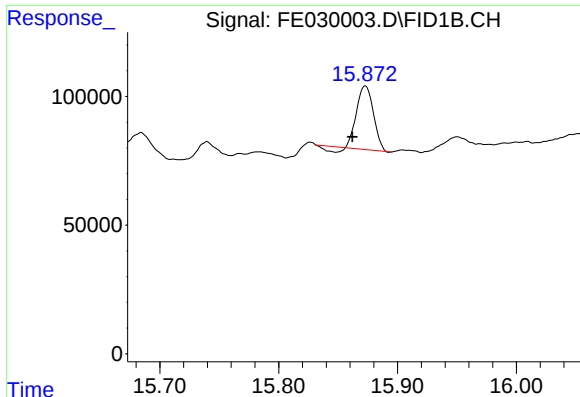

#11 N-HEXACOSANE


R.T.: 15.873 min
Delta R.T.: 0.011 min
Response: 226062
Conc: 0.98 ug/ml

Instrument :
FID_E
ClientSampleId :
P-3-OW(0-10)

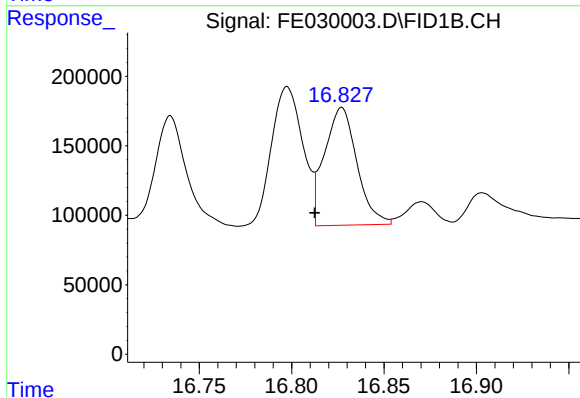


#12 N-OCTACOSANE

R.T.: 16.827 min
Delta R.T.: 0.014 min
Response: 1037611
Conc: 4.51 ug/ml

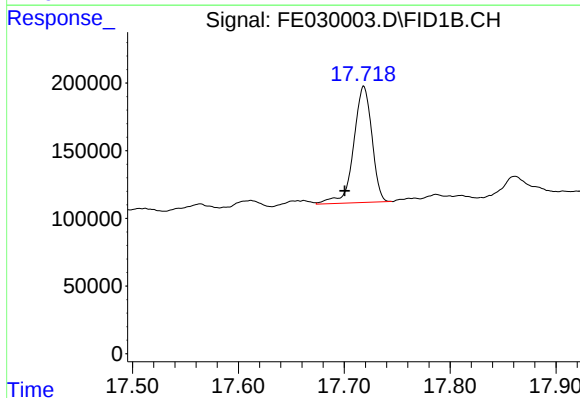


#13 N-TRIACONTANE

R.T.: 17.718 min
Delta R.T.: 0.018 min
Response: 1025265
Conc: 4.46 ug/ml

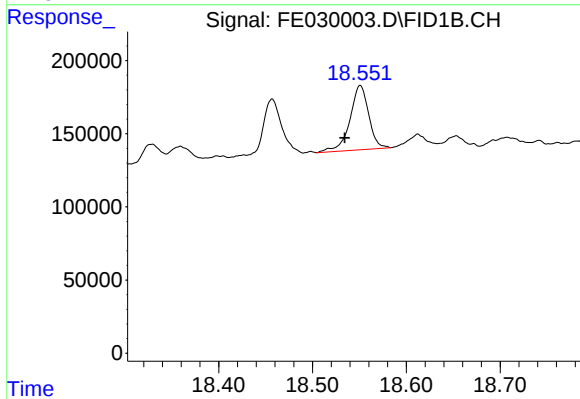

#14 N-DOTRIACONTANE


R.T.: 18.551 min
Delta R.T.: 0.017 min
Response: 612389
Conc: 2.75 ug/ml

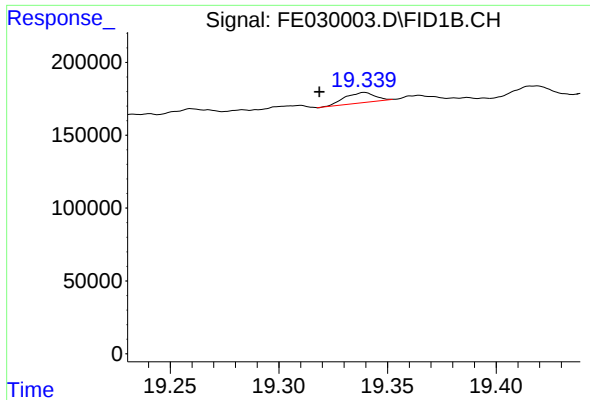

#15 N-TETRATRIACONTANE

R.T.: 19.339 min
Delta R.T.: 0.020 min
Response: 67424
Conc: 0.31 ug/ml

Instrument :
FID_E
ClientSampleId :
P-3-OW(0-10)

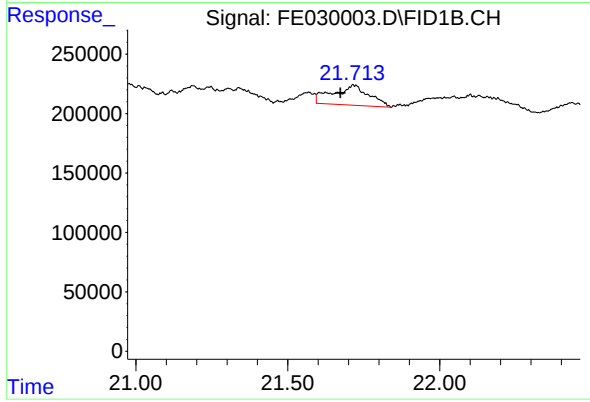

#18 N-TETRACONTANE

R.T.: 21.714 min
Delta R.T.: 0.042 min
Response: 1393574
Conc: 7.33 ug/ml