

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE050719\  
 Data File : FE030000.D  
 Signal(s) : FID1B.CH  
 Acq On : 07 May 2019 12:21  
 Operator : AJ\SJ  
 Sample : K2673-08 5X  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 SB-14-COMP

Manual Integrations  
 APPROVED

Ankita  
 5/8/2019 3:24:17 PM

Integration File: autoint1.e  
 Quant Time: May 08 02:20:13 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE041019.M  
 Quant Title :  
 QLast Update : Wed Apr 10 08:20:21 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.642 | 759651   | 3.745 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE050719\  
Data File : FE030000.D  
Signal(s) : FID1B.CH  
Acq On : 07 May 2019 12:21  
Operator : AJ\SJ  
Sample : K2673-08 5X  
Misc :  
ALS Vial : 6 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
SB-14-COMP


Manual Integrations  
APPROVED

Ankita  
5/8/2019 3:24:17 PM

Integration File: autoint1.e  
Quant Time: May 08 02:20:13 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE041019.M  
Quant Title :  
QLast Update : Wed Apr 10 08:20:21 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

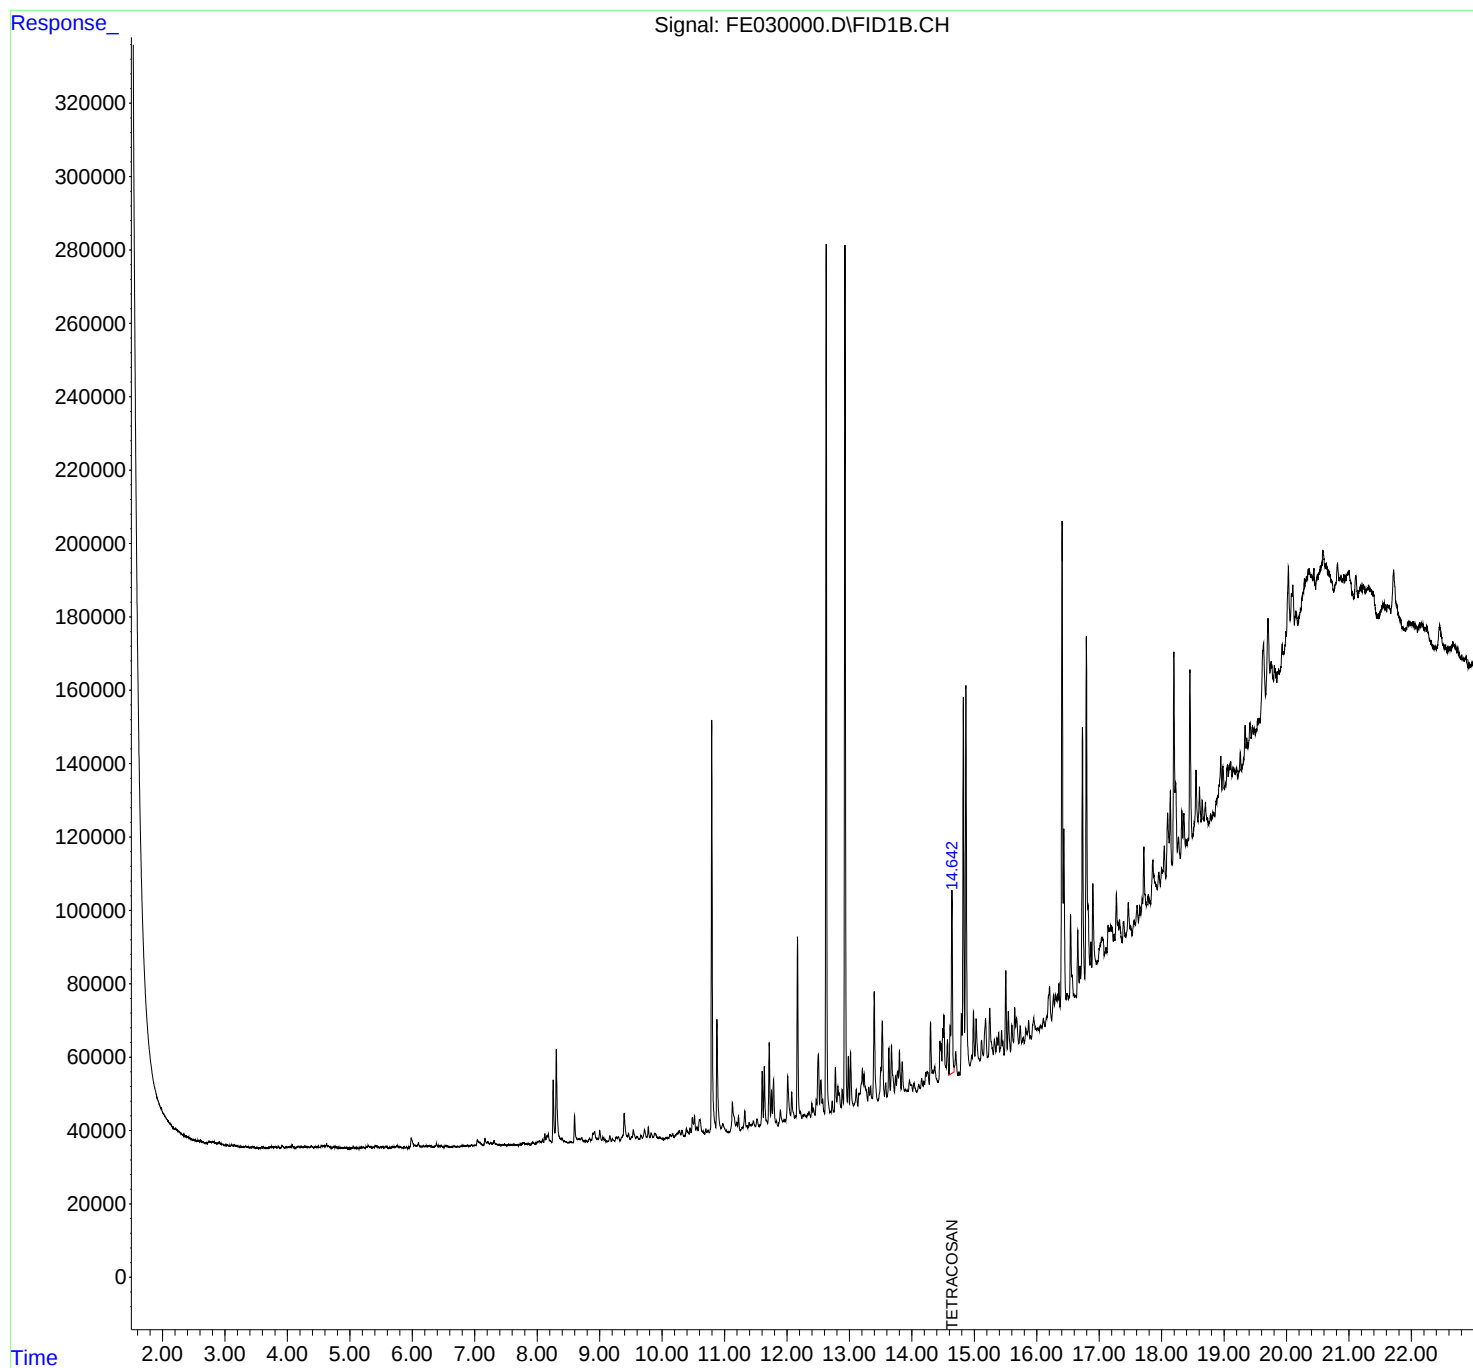

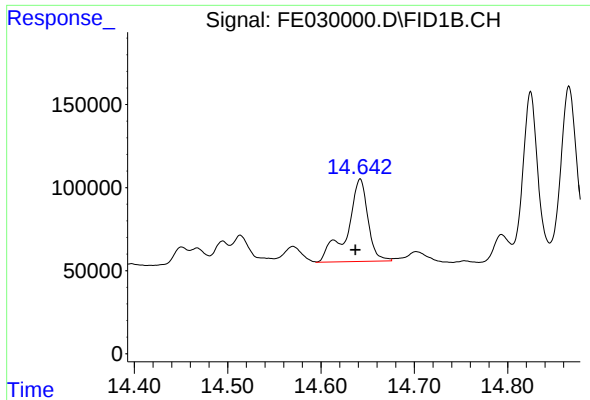

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.642 min  
Delta R.T.: 0.005 min  
Response: 759651  
Conc: 3.74 ug/ml m

Instrument :  
FID\_E  
ClientSampleId :  
SB-14-COMP

Manual Integrations  
APPROVED

Ankita  
5/8/2019 3:24:17 PM