

Data Path : P:\HPCHEM1\FID_E\Data\FE050818\
 Data File : FE027008.D
 Signal(s) : FID1B.CH
 Acq On : 09 May 2018 6:25
 Operator : UA/AJ
 Sample : J2677-03 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 09 08:47:19 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.293	302699	2.056 ug/ml
Target Compounds			
7) N-EICOSANE	13.185	220523	1.158 ug/ml
10) N-TETRACOSANE	15.509	293148	1.741 ug/ml
12) N-OCTACOSANE	17.483	255548	1.546 ug/ml
13) N-TRIACONTANE	18.377	271626	1.615 ug/ml
14) N-DOTRIACONTANE	19.217	392834	2.286 ug/ml
15) N-TETRATRIACONTANE	20.006	382426	2.134 ug/ml
16) N-HEXATRIACONTANE	20.772	1131693	6.431 ug/ml
17) N-OCTATRIACONTANE	21.687	274591	1.672 ug/ml
18) N-TETRACONTANE	22.861	616625	3.714 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE050818\
Data File : FE027008.D
Signal(s) : FID1B.CH
Acq On : 09 May 2018 6:25
Operator : UA/AJ
Sample : J2677-03 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: May 09 08:47:19 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

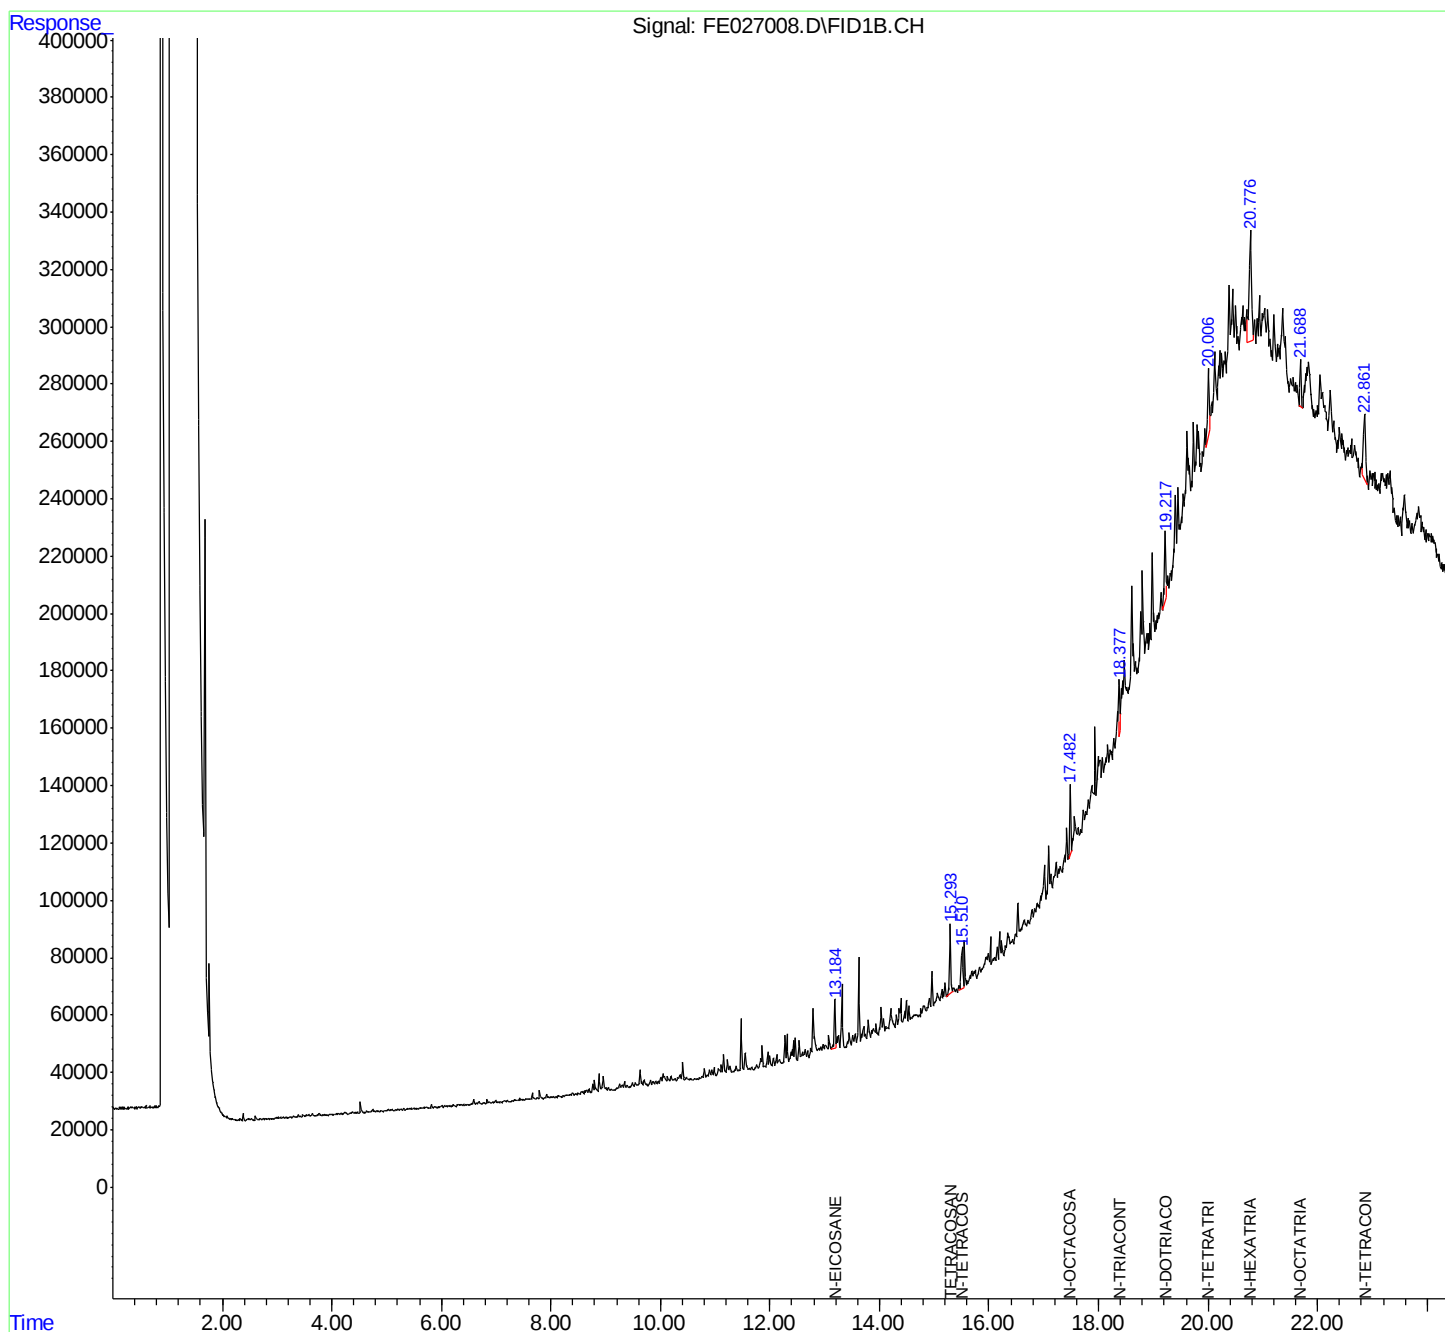


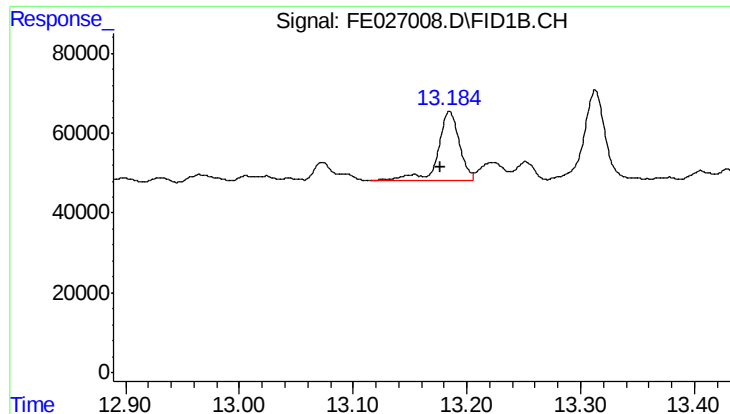

#7 N-EICOSANE


R.T.: 13.185 min
Delta R.T.: 0.008 min
Response: 220523
Conc: 1.16 ug/ml

Instrument :
FID_E
ClientSampleId :

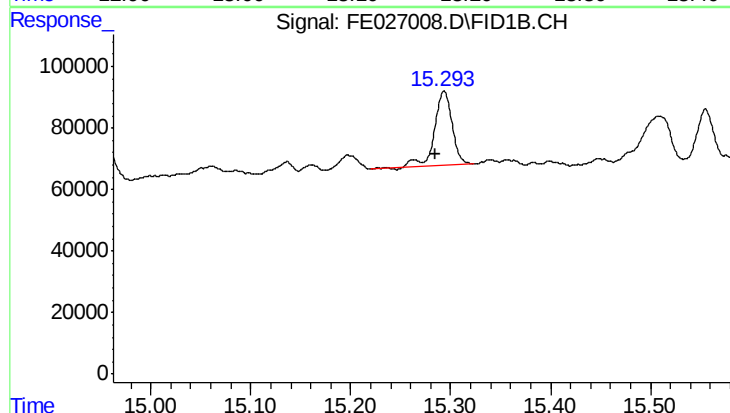


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.293 min
Delta R.T.: 0.009 min
Response: 302699
Conc: 2.06 ug/ml

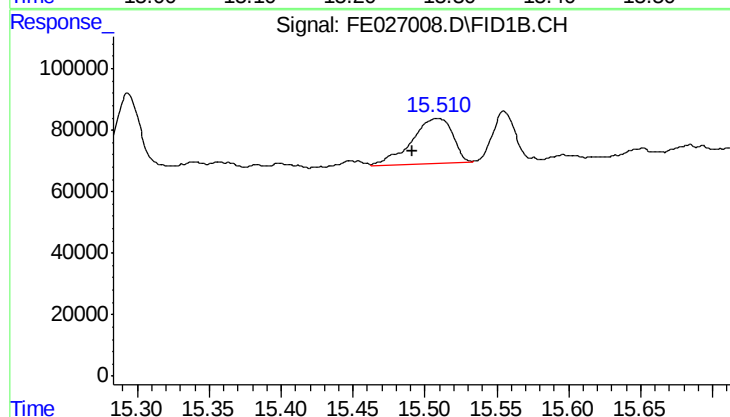


#10 N-TETRACOSANE

R.T.: 15.509 min
Delta R.T.: 0.018 min
Response: 293148
Conc: 1.74 ug/ml

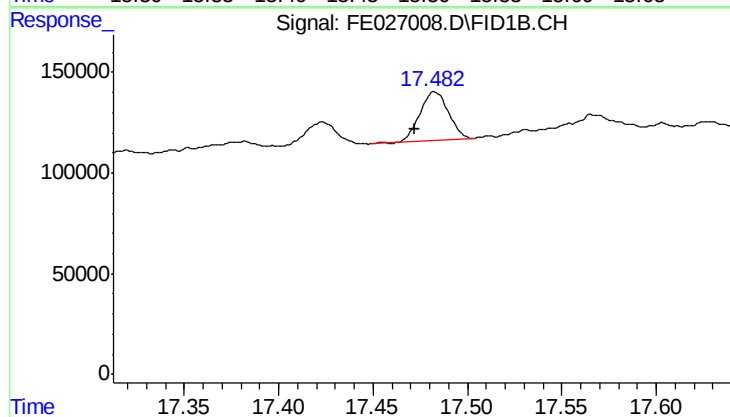

#12 N-OCTACOSANE


R.T.: 17.483 min
Delta R.T.: 0.011 min
Response: 255548
Conc: 1.55 ug/ml

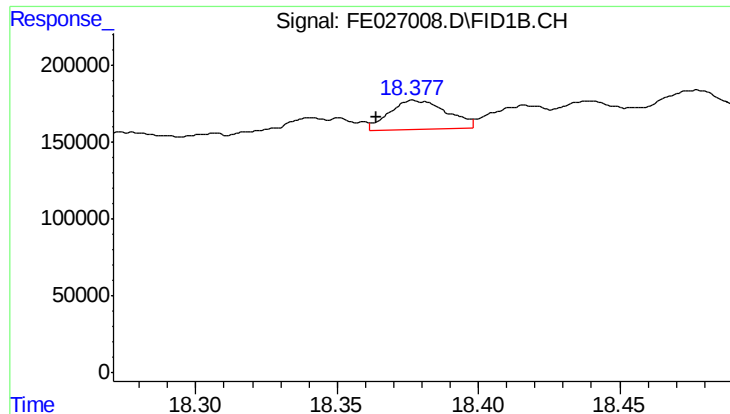

#13 N-TRIACONTANE


R.T.: 18.377 min
Delta R.T.: 0.013 min
Response: 271626
Conc: 1.61 ug/ml

Instrument :
FID_E
ClientSampleId :

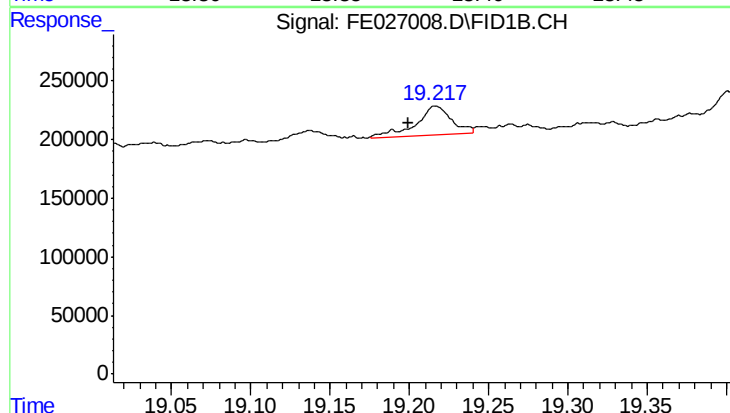


#14 N-DOTRIACONTANE

R.T.: 19.217 min
Delta R.T.: 0.017 min
Response: 392834
Conc: 2.29 ug/ml

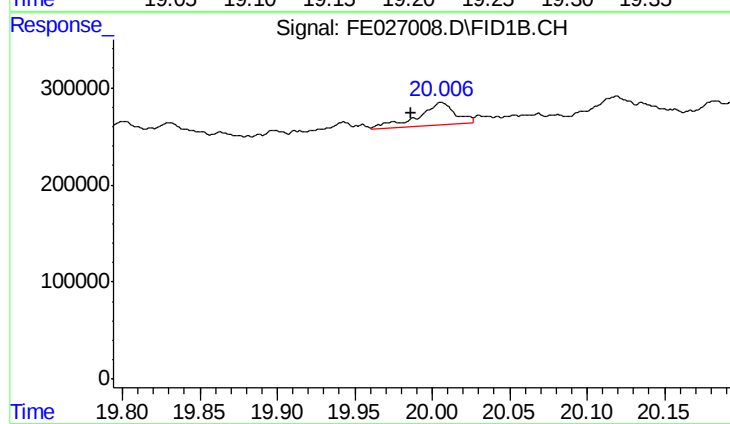


#15 N-TETRATRIACONTANE

R.T.: 20.006 min
Delta R.T.: 0.020 min
Response: 382426
Conc: 2.13 ug/ml

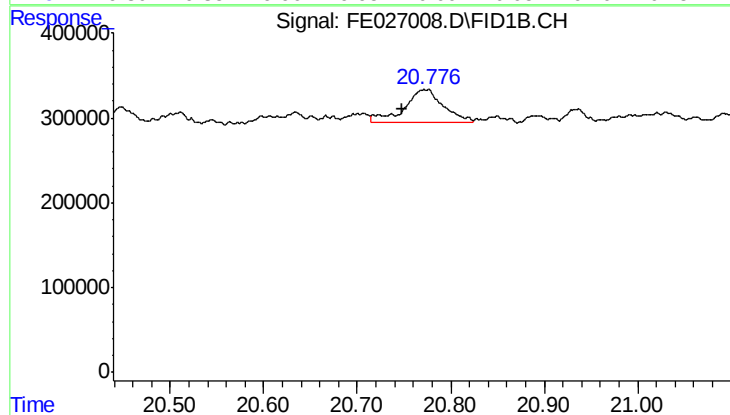

#16 N-HEXATRIACONTANE


R.T.: 20.772 min
Delta R.T.: 0.024 min
Response: 1131693
Conc: 6.43 ug/ml

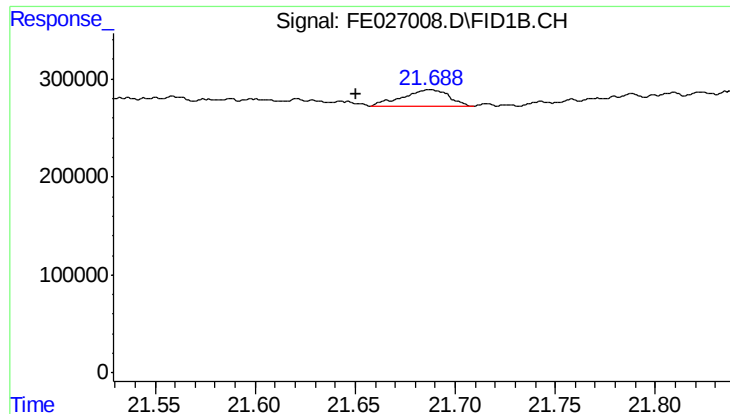

#17 N-OCTATRIACONTANE

R.T.: 21.687 min
Delta R.T.: 0.037 min
Response: 274591
Conc: 1.67 ug/ml

Instrument :
FID_E
ClientSampleId :

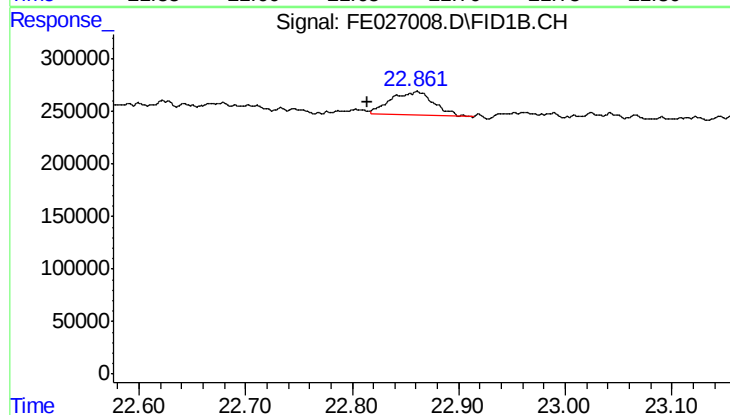

#18 N-TETRACONTANE

R.T.: 22.861 min
Delta R.T.: 0.046 min
Response: 616625
Conc: 3.71 ug/ml