

Data Path : P:\HPCHEM1\FID_E\Data\FE050818\
 Data File : FE027009.D
 Signal(s) : FID1B.CH
 Acq On : 09 May 2018 6:59
 Operator : UA/AJ
 Sample : J2759-05 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 09 08:47:37 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.295	221951	1.507 ug/ml
Target Compounds			
7) N-EICOSANE	13.190	467261	2.454 ug/ml
8) N-DOCOSANE	14.364	321333	1.801 ug/ml
10) N-TETRACOSANE	15.521	2122241	12.601 ug/ml
11) N-HEXACOSANE	16.531	163854	0.992 ug/ml
12) N-OCTACOSANE	17.496	1833090	11.093 ug/ml
13) N-TRIACONTANE	18.350	183543	1.091 ug/ml
14) N-DOTRIACONTANE	19.221	726833	4.230 ug/ml
15) N-TETRATRIACONTANE	19.974	23057	0.129 ug/ml
16) N-HEXATRIACONTANE	20.778	995058	5.655 ug/ml
17) N-OCTATRIACONTANE	21.688	299346	1.822 ug/ml
18) N-TETRACONTANE	22.871f	455084	2.741 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE050818\
Data File : FE027009.D
Signal(s) : FID1B.CH
Acq On : 09 May 2018 6:59
Operator : UA/AJ
Sample : J2759-05 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 09 08:47:37 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

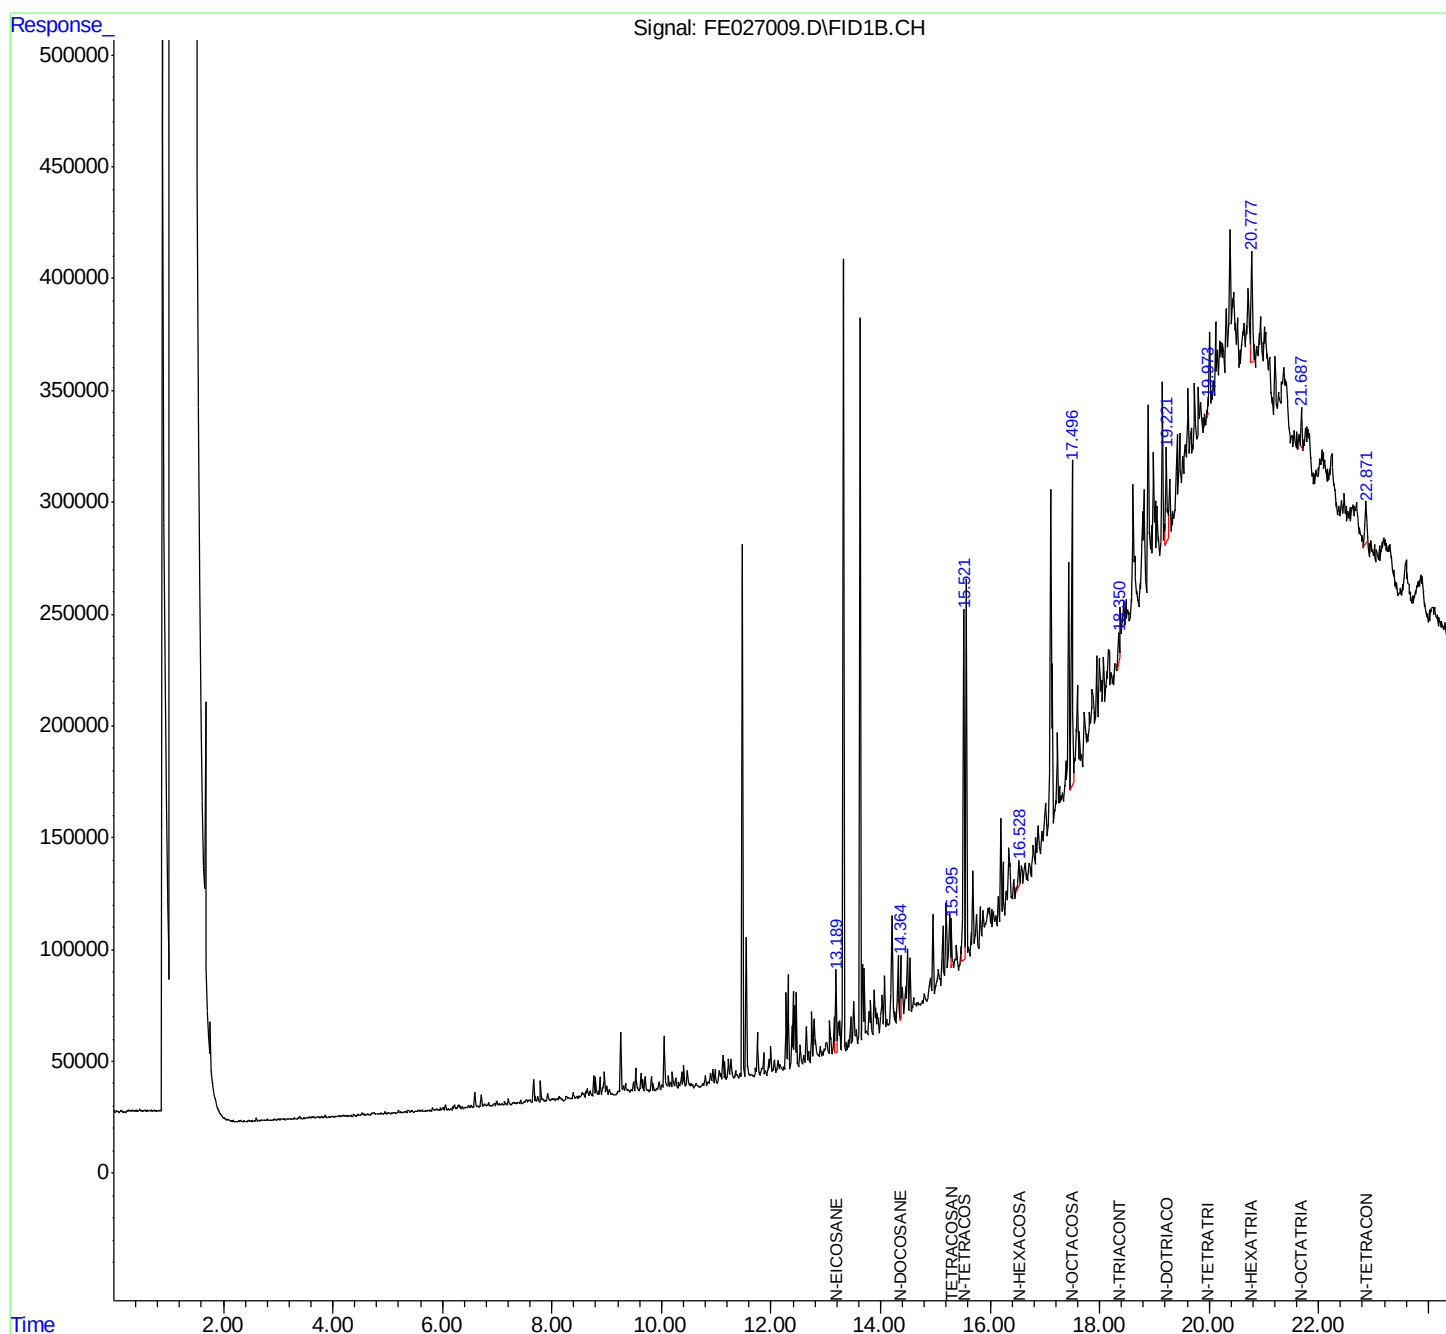


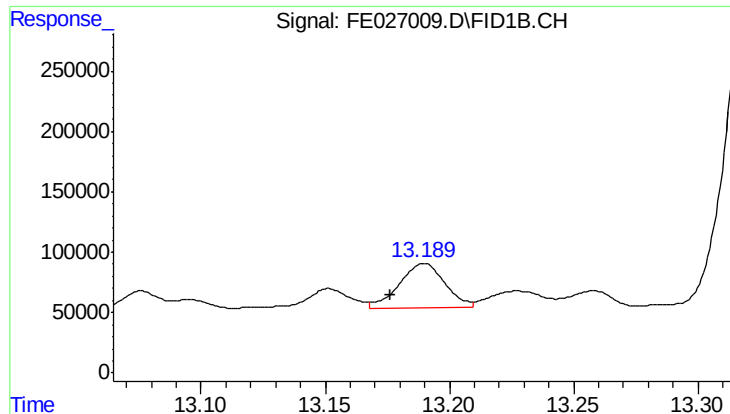

#7 N-EICOSANE


R.T.: 13.190 min
Delta R.T.: 0.014 min
Response: 467261
Conc: 2.45 ug/ml

Instrument :
FID_E
ClientSampleId :

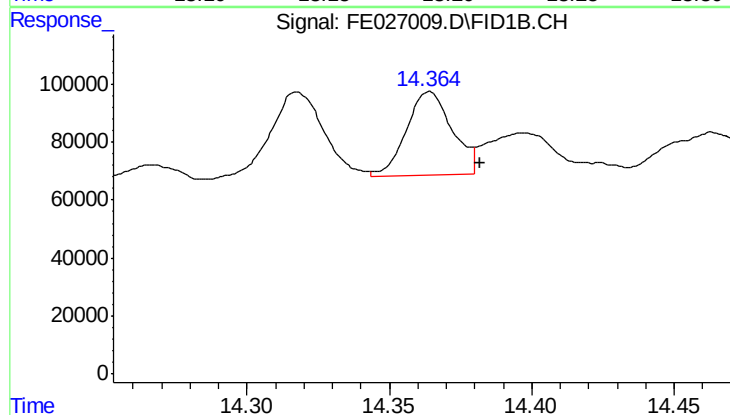


#8 N-DOCOSANE

R.T.: 14.364 min
Delta R.T.: -0.018 min
Response: 321333
Conc: 1.80 ug/ml

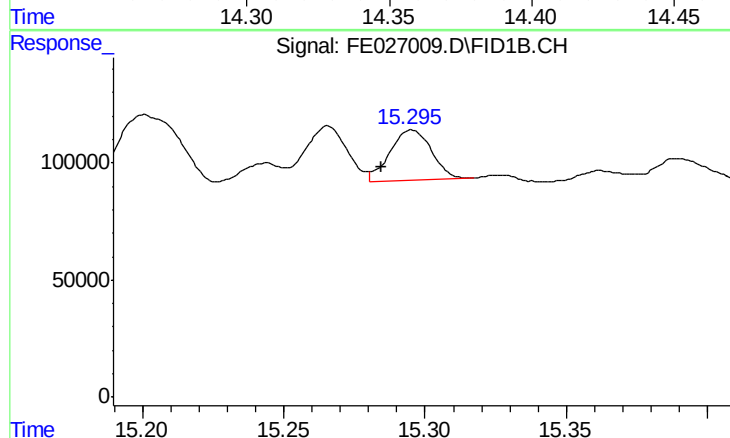


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.295 min
Delta R.T.: 0.011 min
Response: 221951
Conc: 1.51 ug/ml

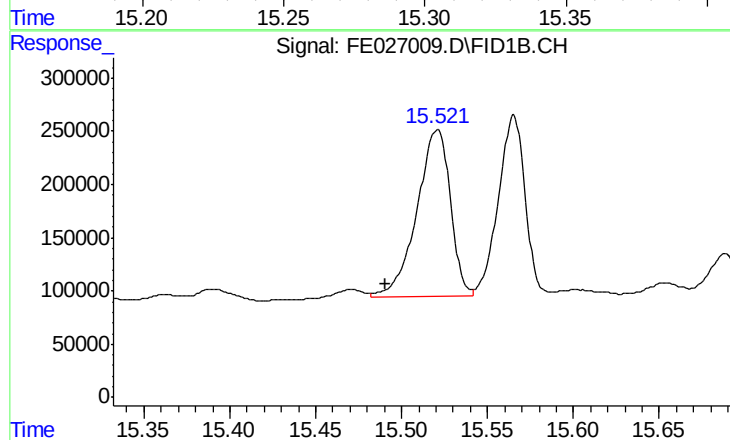

#10 N-TETRACOSANE


R.T.: 15.521 min
Delta R.T.: 0.030 min
Response: 212241
Conc: 12.60 ug/ml

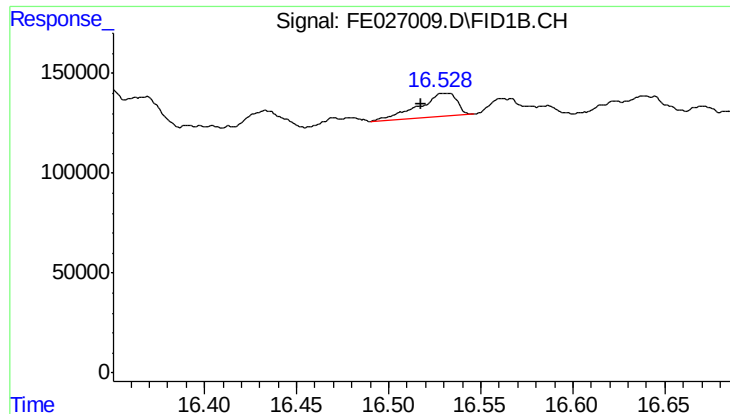

#11 N-HEXACOSANE


R.T.: 16.531 min
Delta R.T.: 0.013 min
Response: 163854
Conc: 0.99 ug/ml

Instrument :
FID_E
ClientSampleId :

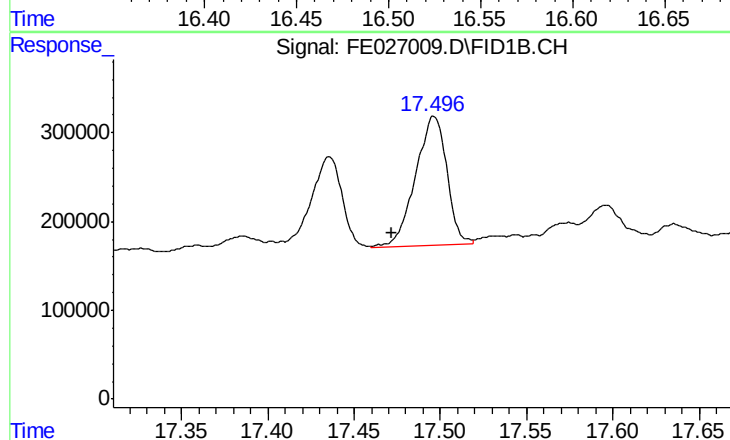


#12 N-OCTACOSANE

R.T.: 17.496 min
Delta R.T.: 0.024 min
Response: 1833090
Conc: 11.09 ug/ml

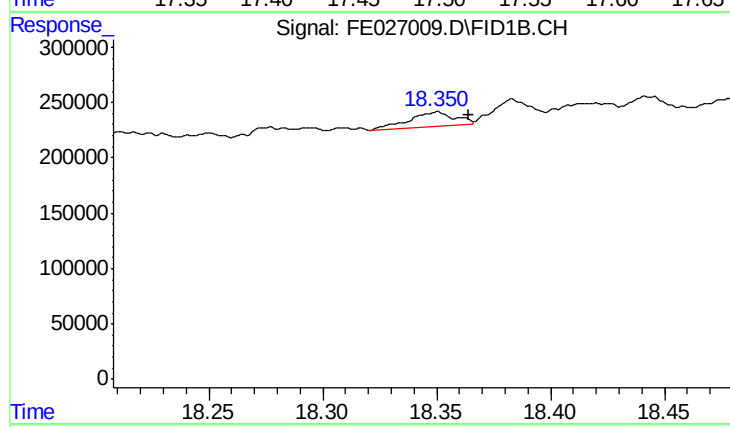


#13 N-TRIACONTANE

R.T.: 18.350 min
Delta R.T.: -0.014 min
Response: 183543
Conc: 1.09 ug/ml

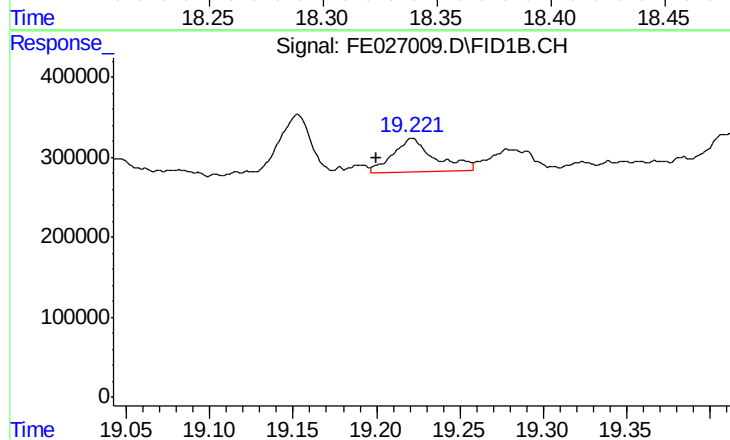

#14 N-DOTRIACONTANE


R.T.: 19.221 min
Delta R.T.: 0.022 min
Response: 726833
Conc: 4.23 ug/ml

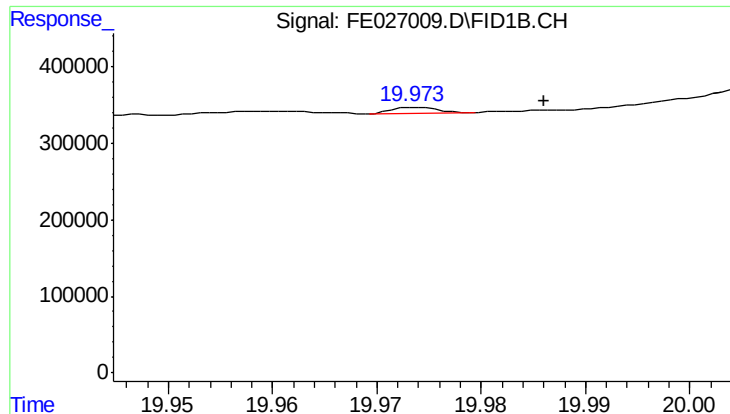

#15 N-TETRATRIACONTANE


R.T.: 19.974 min
Delta R.T.: -0.012 min
Response: 23057
Conc: 0.13 ug/ml

Instrument :
FID_E
ClientSampleId :

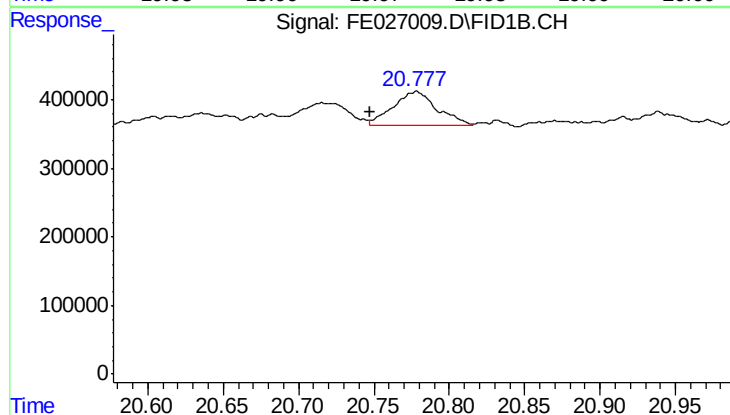


#16 N-HEXATRIACONTANE

R.T.: 20.778 min
Delta R.T.: 0.030 min
Response: 995058
Conc: 5.65 ug/ml

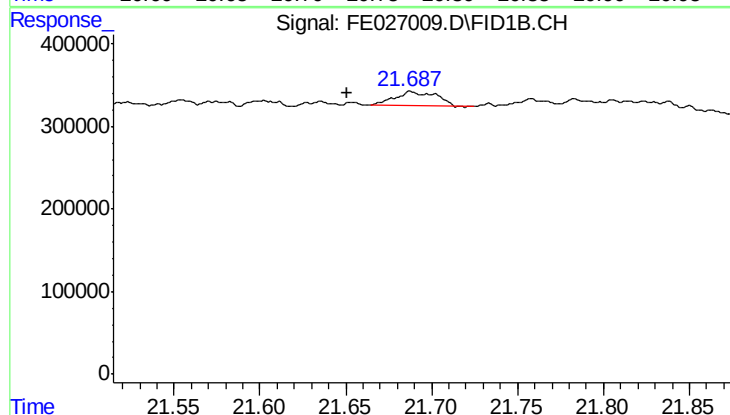

#17 N-OCTATRIACONTANE

R.T.: 21.688 min
Delta R.T.: 0.038 min
Response: 299346
Conc: 1.82 ug/ml

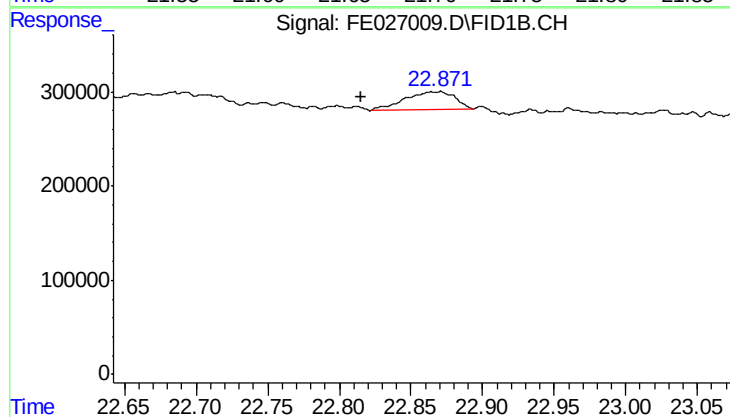

#18 N-TETRACONTANE

R.T.: 22.871 min
Delta R.T.: 0.056 min
Response: 455084
Conc: 2.74 ug/ml