

Data Path : P:\HPCHEM1\FID_E\Data\FE050818\
 Data File : FE027012.D
 Signal(s) : FID1B.CH
 Acq On : 09 May 2018 8:39
 Operator : UA/AJ
 Sample : J2676-03 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 09 10:39:43 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
 Quant Title :
 QLast Update : Wed May 09 08:38:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.279	1473881	10.009 ug/ml
Target Compounds			
4) N-TETRADECANE	8.796	1361423	7.203 ug/ml
5) N-HEXADECANE	10.412	494058	2.513 ug/ml
6) N-OCTADECANE	11.867	869494	4.330 ug/ml
7) N-EICOSANE	13.167	1421157	7.463 ug/ml
8) N-DOCOSANE	14.384	4729812	26.515 ug/ml
10) N-TETRACOSANE	15.490	483618	2.872 ug/ml
11) N-HEXACOSANE	16.520	477988	2.894 ug/ml
12) N-OCTACOSANE	17.452	3927845	23.769 ug/ml
13) N-TRIACONTANE	18.343	486598	2.892 ug/ml
14) N-DOTRIACONTANE	19.165	2996330	17.440 ug/ml
16) N-HEXATRIACONTANE	20.775	295373	1.679 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE050818\
Data File : FE027012.D
Signal(s) : FID1B.CH
Acq On : 09 May 2018 8:39
Operator : UA/AJ
Sample : J2676-03 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 09 10:39:43 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE050818.M
Quant Title :
QLast Update : Wed May 09 08:38:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

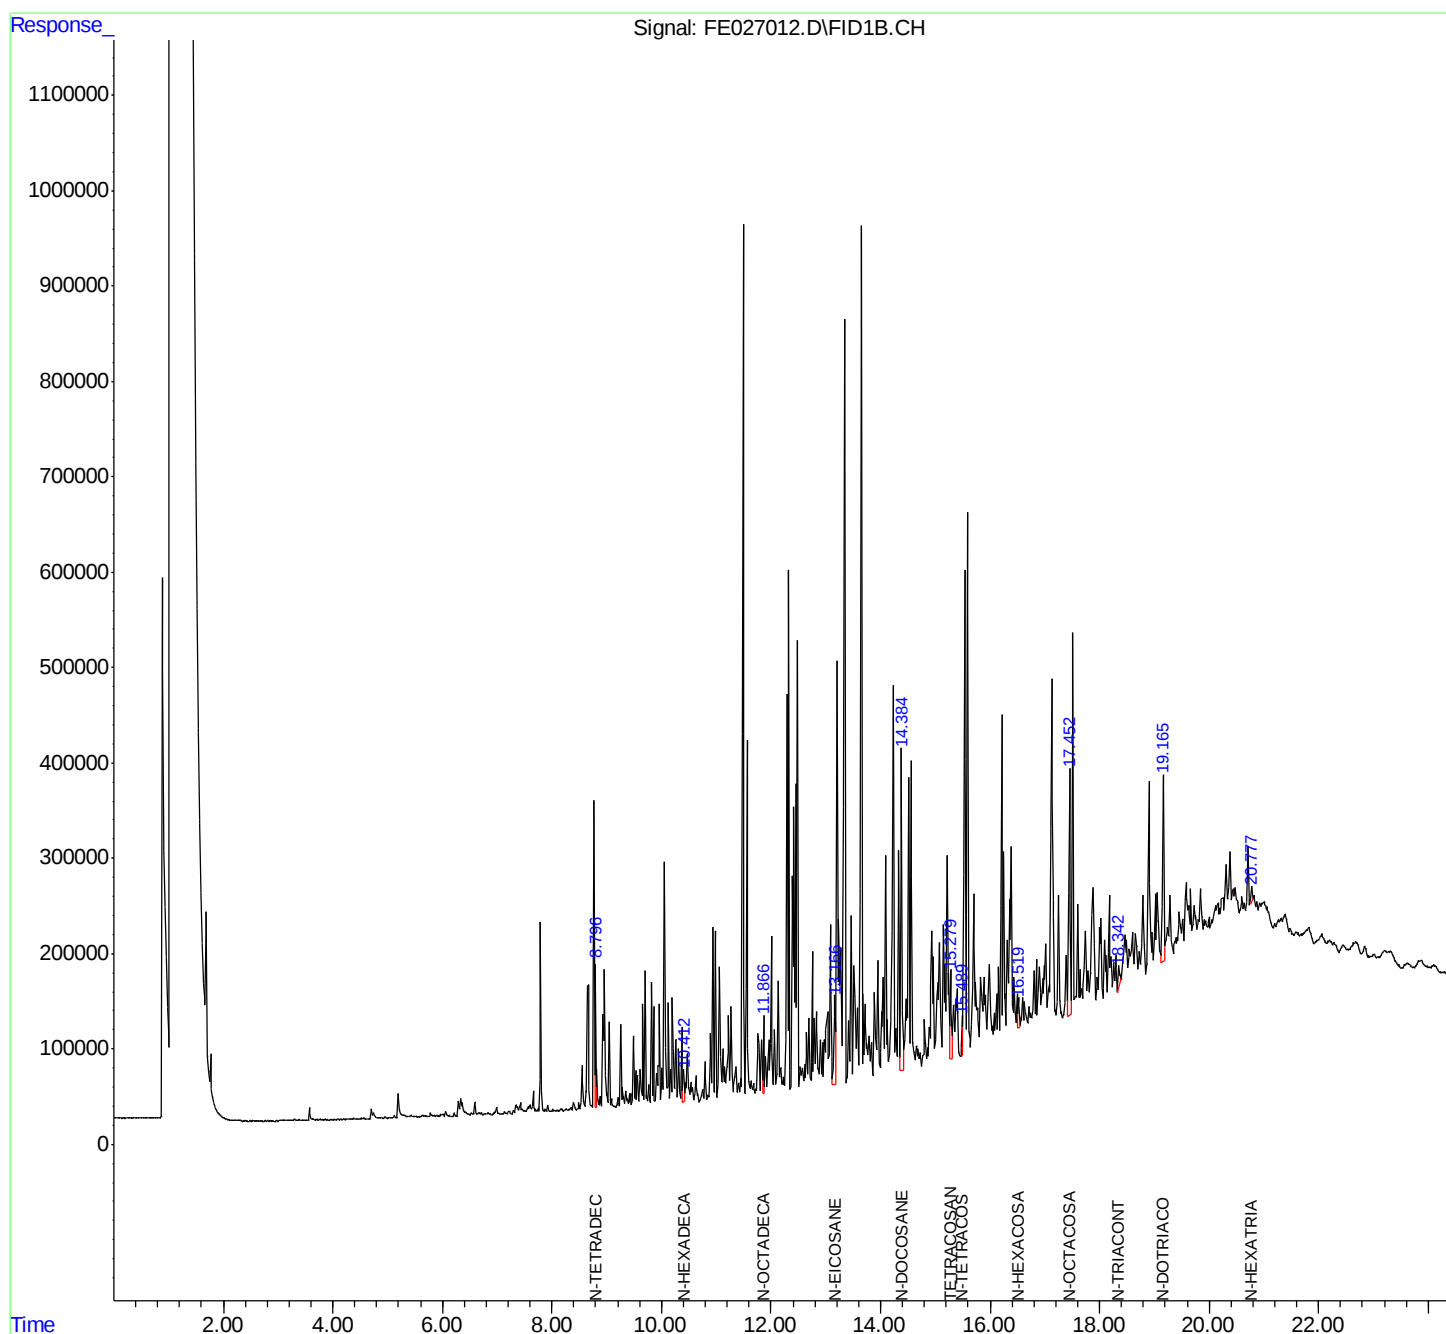


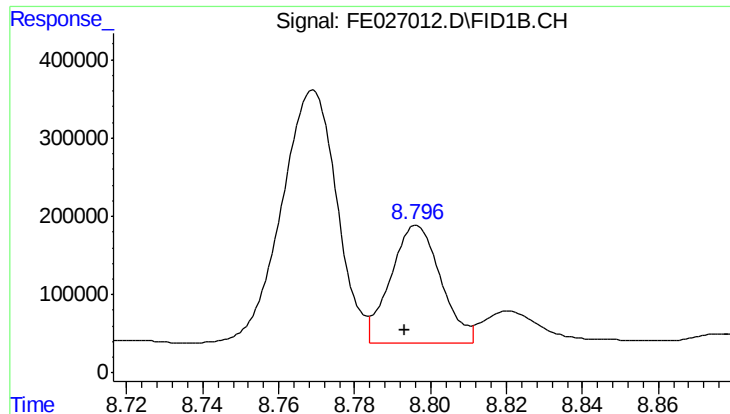

#4 N-TETRADECANE


R.T.: 8.796 min
Delta R.T.: 0.003 min
Response: 1361423
Conc: 7.20 ug/ml

Instrument :
FID_E
ClientSampleId :

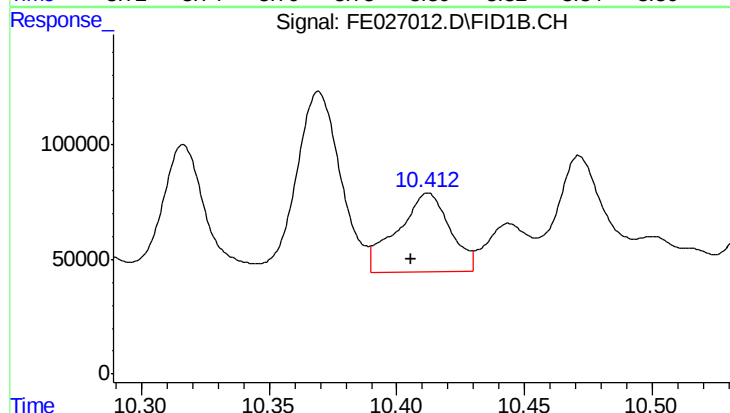


#5 N-HEXADECANE

R.T.: 10.412 min
Delta R.T.: 0.007 min
Response: 494058
Conc: 2.51 ug/ml

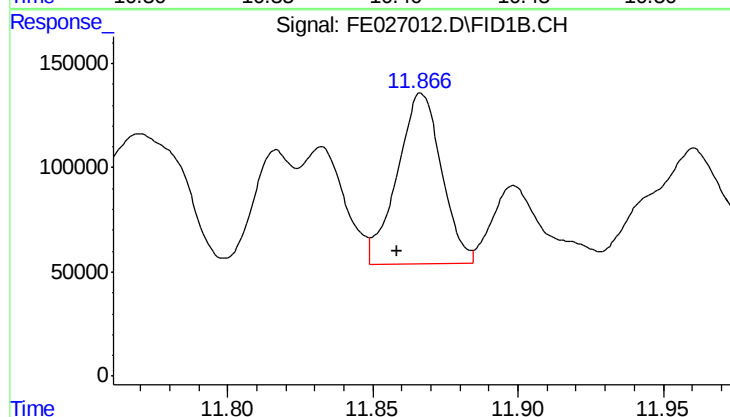


#6 N-OCTADECANE

R.T.: 11.867 min
Delta R.T.: 0.008 min
Response: 869494
Conc: 4.33 ug/ml

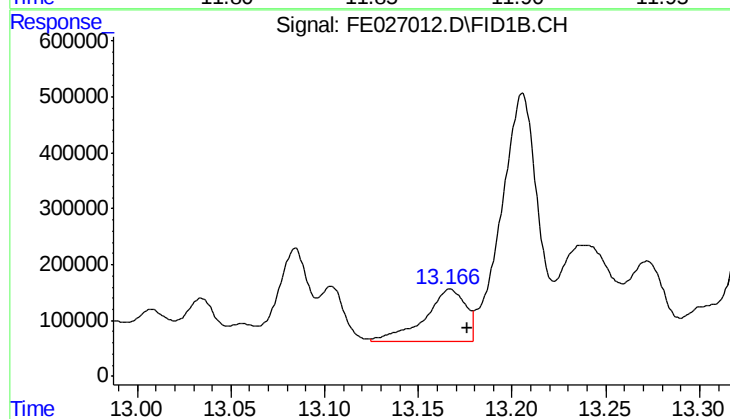

#7 N-EICOSANE


R.T.: 13.167 min
Delta R.T.: -0.009 min
Response: 1421157
Conc: 7.46 ug/ml

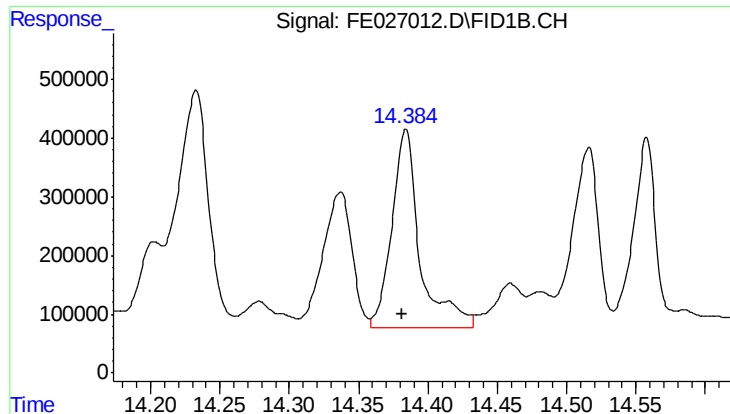

#8 N-DOCOSANE


R.T.: 14.384 min
Delta R.T.: 0.002 min
Response: 4729812
Conc: 26.52 ug/ml

Instrument :
FID_E
ClientSampleId :

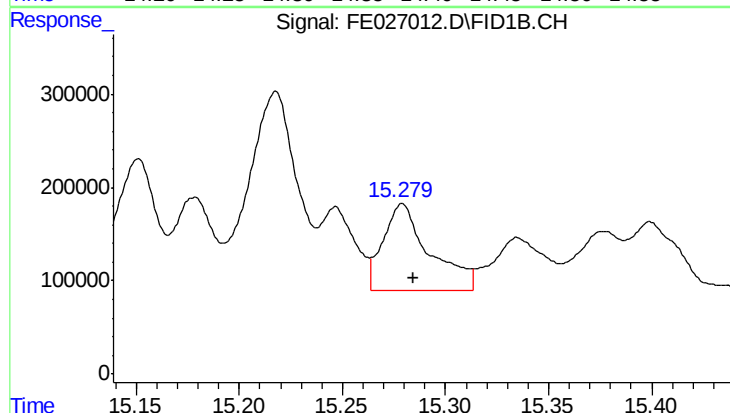


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.279 min
Delta R.T.: -0.006 min
Response: 1473881
Conc: 10.01 ug/ml

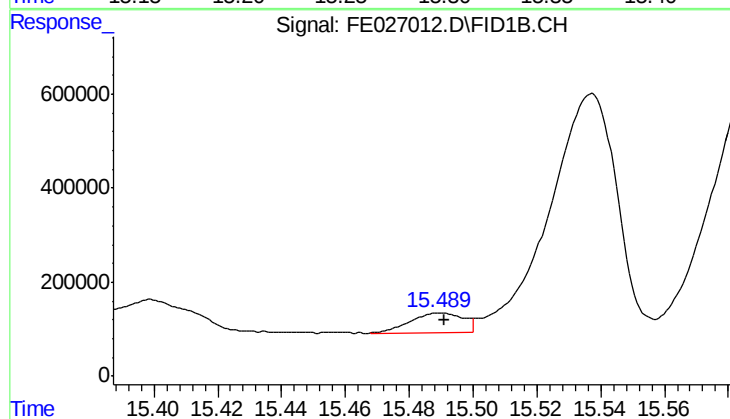


#10 N-TETRACOSANE

R.T.: 15.490 min
Delta R.T.: 0.000 min
Response: 483618
Conc: 2.87 ug/ml

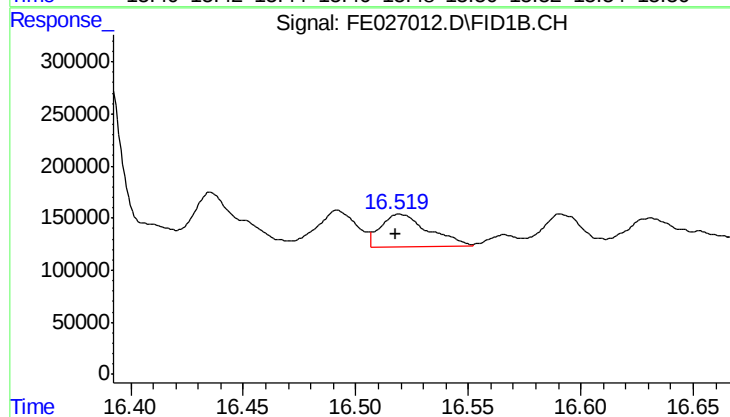

#11 N-HEXACOSANE


R.T.: 16.520 min
Delta R.T.: 0.002 min
Response: 477988
Conc: 2.89 ug/ml

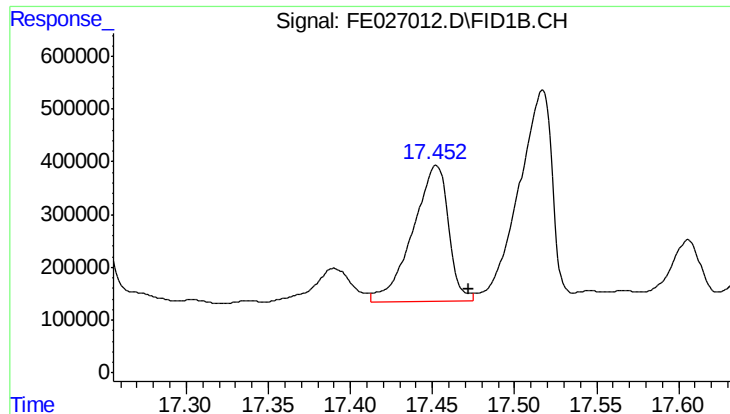

#12 N-OCTACOSANE


R.T.: 17.452 min
Delta R.T.: -0.020 min
Response: 3927845
Conc: 23.77 ug/ml

Instrument :
FID_E
ClientSampleId :

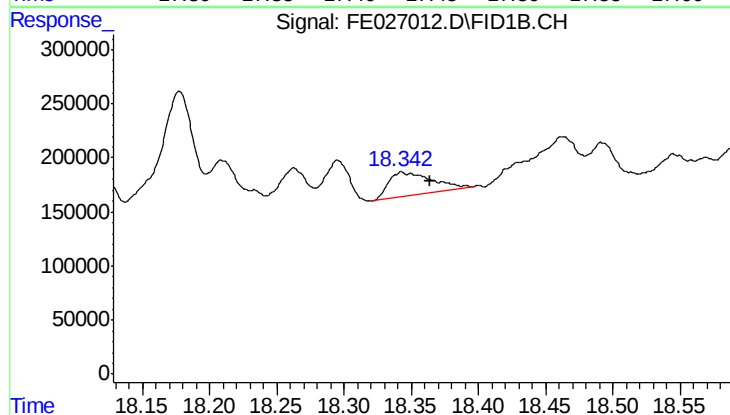


#13 N-TRIACONTANE

R.T.: 18.343 min
Delta R.T.: -0.021 min
Response: 486598
Conc: 2.89 ug/ml

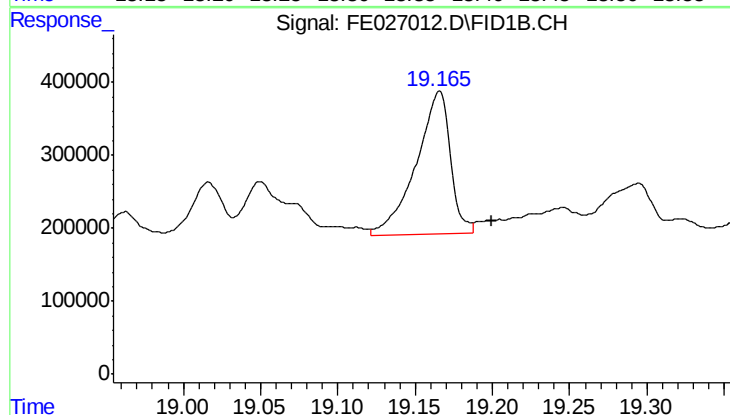

#14 N-DOTRIACONTANE

R.T.: 19.165 min
Delta R.T.: -0.035 min
Response: 2996330
Conc: 17.44 ug/ml

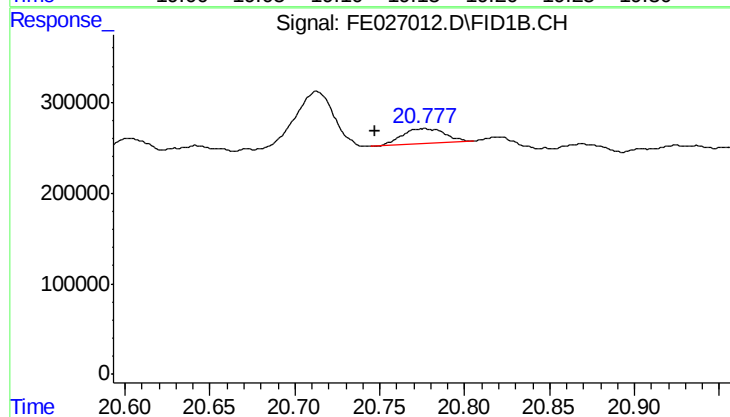

#16 N-HEXATRIACONTANE

R.T.: 20.775 min
Delta R.T.: 0.028 min
Response: 295373
Conc: 1.68 ug/ml